

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025027.D
 Acq On : 16 Mar 2022 03:32
 Operator : SY/MD
 Sample : N1933-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDB4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	97	rVB	97337	99623	18.10%	2.204%
2	1.568	157	164	175	rBV	71697	81348	14.78%	1.800%
3	2.111	322	333	347	rBV	145910	210847	38.31%	4.666%
4	2.182	347	355	375	rVB2	4742	11615	2.11%	0.257%
5	3.892	878	887	935	rBV	51162	173024	31.44%	3.829%
6	4.352	1013	1030	1062	rBV	96996	258483	46.97%	5.720%
7	4.831	1162	1179	1198	rBV2	10991	26251	4.77%	0.581%
8	5.047	1230	1246	1276	rBV3	221436	550324	100.00%	12.178%
9	5.619	1411	1424	1451	rBV	179439	366407	66.58%	8.108%
10	5.915	1504	1516	1536	rBV8	6702	15501	2.82%	0.343%
11	6.069	1549	1564	1590	rBV	122222	254101	46.17%	5.623%
12	6.989	1838	1850	1880	rBV	56713	104395	18.97%	2.310%
13	7.317	1941	1952	1970	rBV	273847	473041	85.96%	10.468%
14	7.625	2039	2048	2072	rBV2	31095	56478	10.26%	1.250%
15	7.934	2132	2144	2151	rBV3	3196	5535	1.01%	0.122%
16	7.979	2151	2158	2168	rVB3	5763	9793	1.78%	0.217%
17	8.088	2183	2192	2234	rBV	224035	430008	78.14%	9.515%
18	8.850	2418	2429	2456	rBV	270433	446471	81.13%	9.880%
19	10.214	2843	2853	2872	rBV	79191	125751	22.85%	2.783%
20	10.381	2891	2905	2915	rBV2	6339	10131	1.84%	0.224%
21	11.249	3163	3175	3202	rBV	265264	409302	74.37%	9.057%
22	11.532	3254	3263	3280	rBV2	12030	23286	4.23%	0.515%
23	11.622	3280	3291	3313	rVB	242349	377401	68.58%	8.351%




Sum of corrected areas: 4519116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025027.D
Acq On : 16 Mar 2022 03:32
Operator : SY/MD
Sample : N1933-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

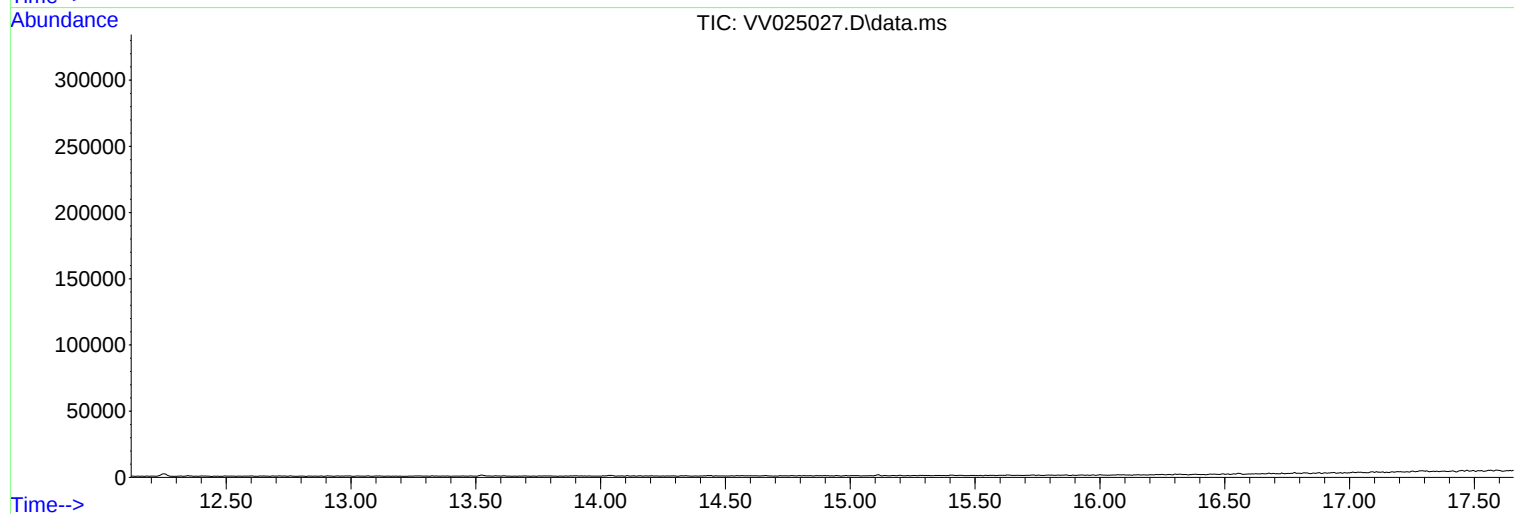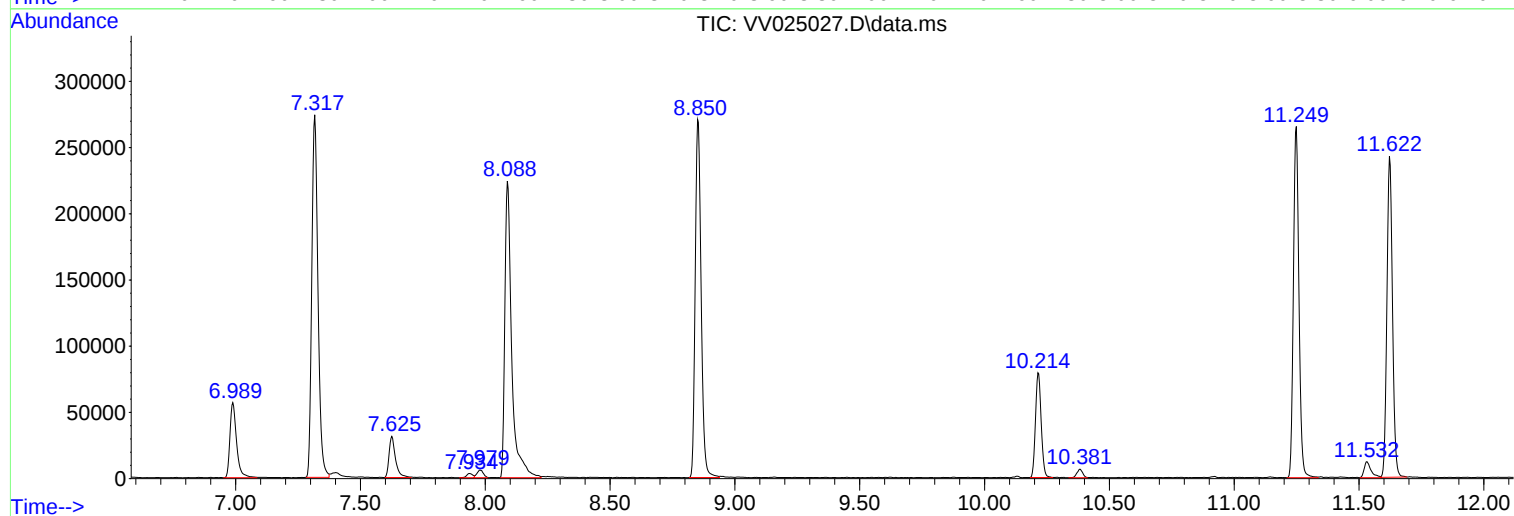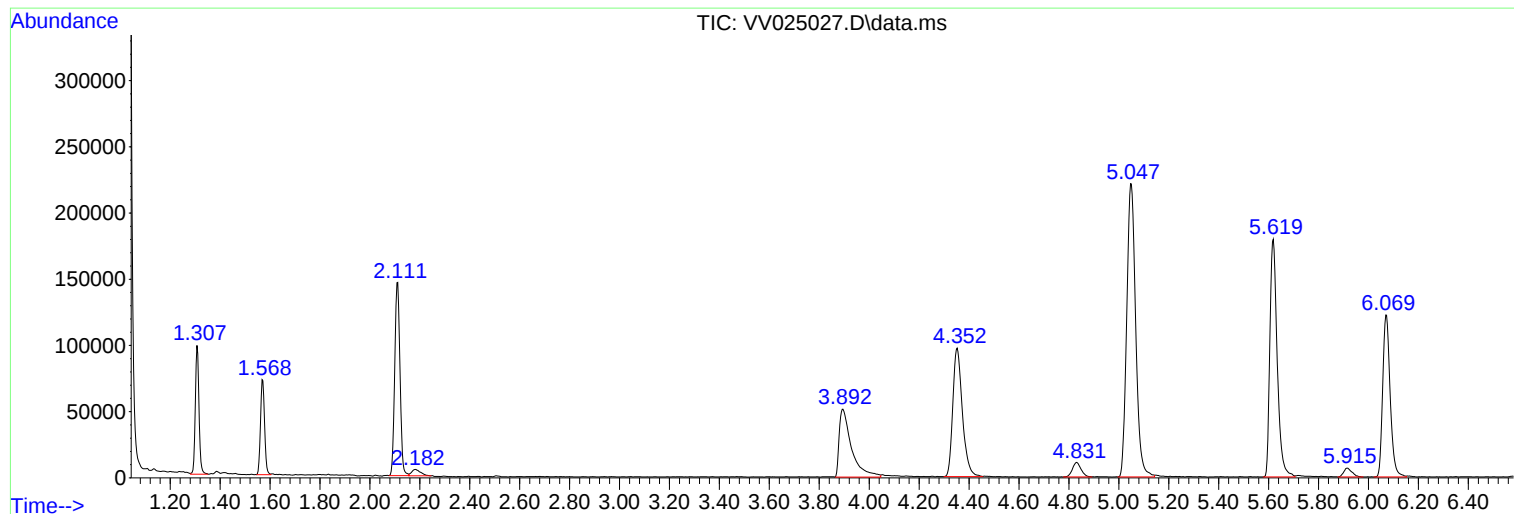

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025027.D
Acq On : 16 Mar 2022 03:32
Operator : SY/MD
Sample : N1933-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025027.D
Acq On : 16 Mar 2022 03:32
Operator : SY/MD
Sample : N1933-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc