

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025030.D
 Acq On : 16 Mar 2022 04:42
 Operator : SY/MD
 Sample : N1933-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDD2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rVB	92411	94846	4.11%	1.259%
2	1.571	155	165	177	rBV	71059	80647	3.50%	1.070%
3	2.111	322	333	344	rBV	140985	205120	8.89%	2.722%
4	2.182	345	355	376	rVB	21648	52540	2.28%	0.697%
5	3.892	869	887	900	rBV	58958	157510	6.83%	2.090%
6	3.969	901	911	952	rVB	131115	394299	17.09%	5.233%
7	4.342	1010	1027	1062	rBV3	254335	715163	31.00%	9.491%
8	4.828	1155	1178	1216	rBV	978275	2306770	100.00%	30.615%
9	5.050	1231	1247	1279	rBV2	223933	548190	23.76%	7.275%
10	5.619	1412	1424	1451	rBV	174185	353655	15.33%	4.694%
11	6.069	1552	1564	1592	rBV	120442	248453	10.77%	3.297%
12	6.989	1840	1850	1871	rBV	56475	103133	4.47%	1.369%
13	7.317	1941	1952	1970	rBV	268021	463282	20.08%	6.149%
14	7.625	2039	2048	2069	rBV	31693	55784	2.42%	0.740%
15	8.088	2182	2192	2227	rBV	217498	421064	18.25%	5.588%
16	8.850	2418	2429	2453	rBV	259618	426855	18.50%	5.665%
17	10.214	2840	2853	2872	rVB	76402	119917	5.20%	1.592%
18	11.249	3164	3175	3199	rBV	255164	392015	16.99%	5.203%
19	11.532	3254	3263	3280	rBV2	14485	27722	1.20%	0.368%
20	11.622	3280	3291	3312	rVB	233872	367824	15.95%	4.882%




Sum of corrected areas: 7534789

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025030.D
Acq On : 16 Mar 2022 04:42
Operator : SY/MD
Sample : N1933-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

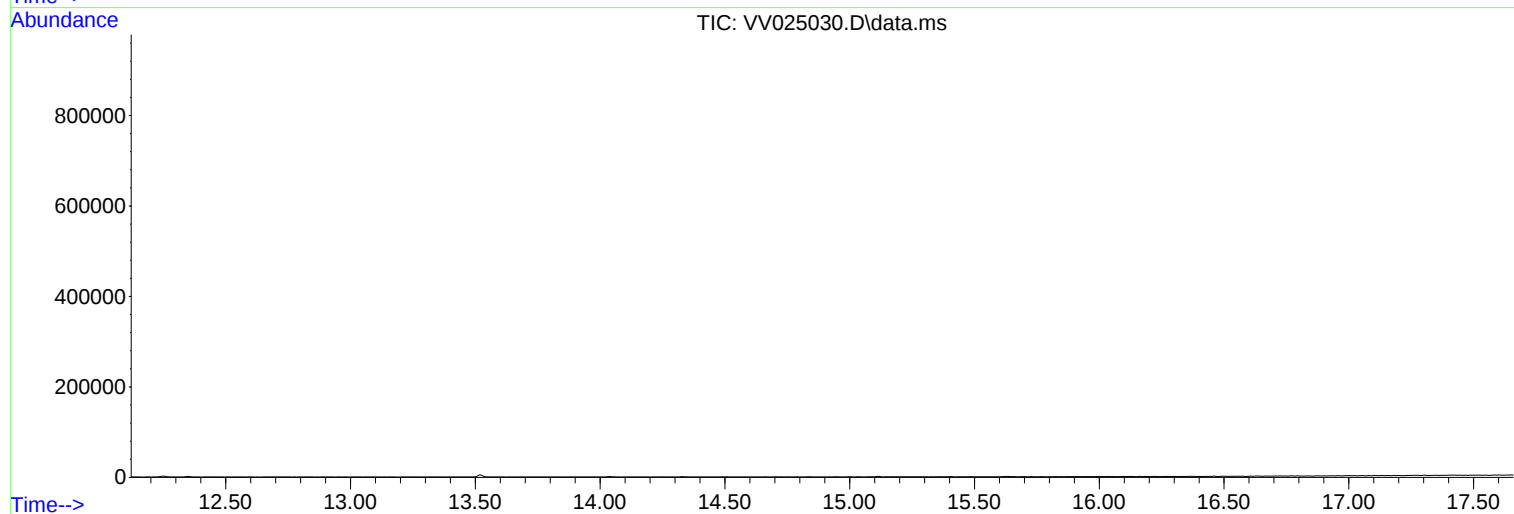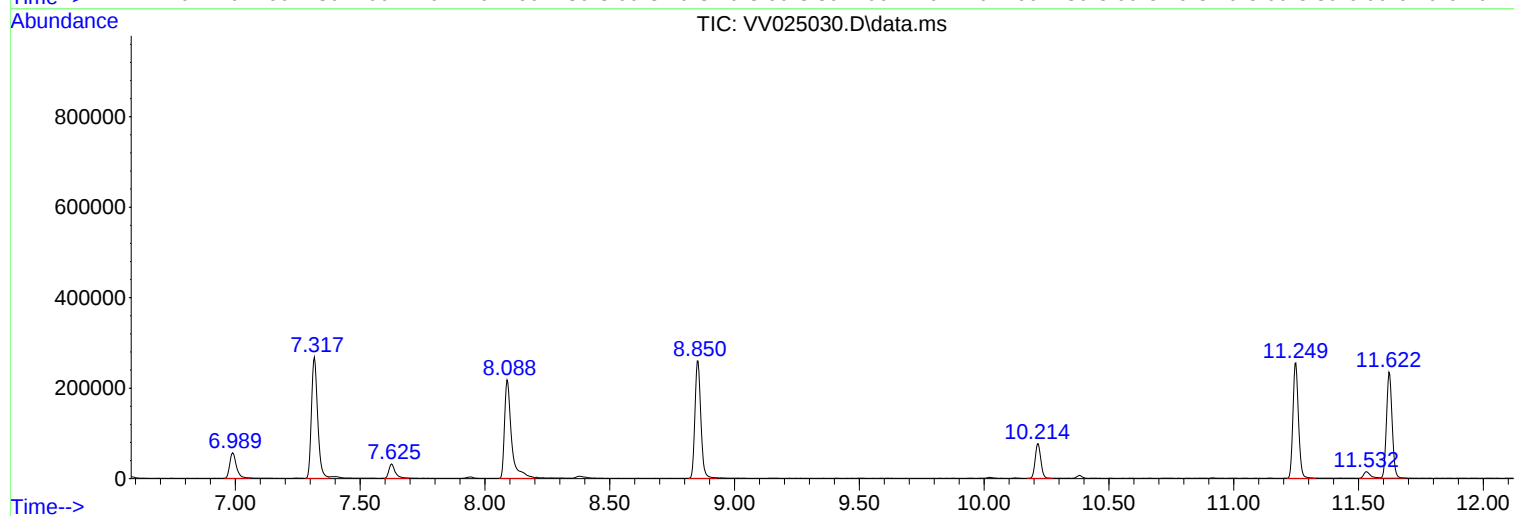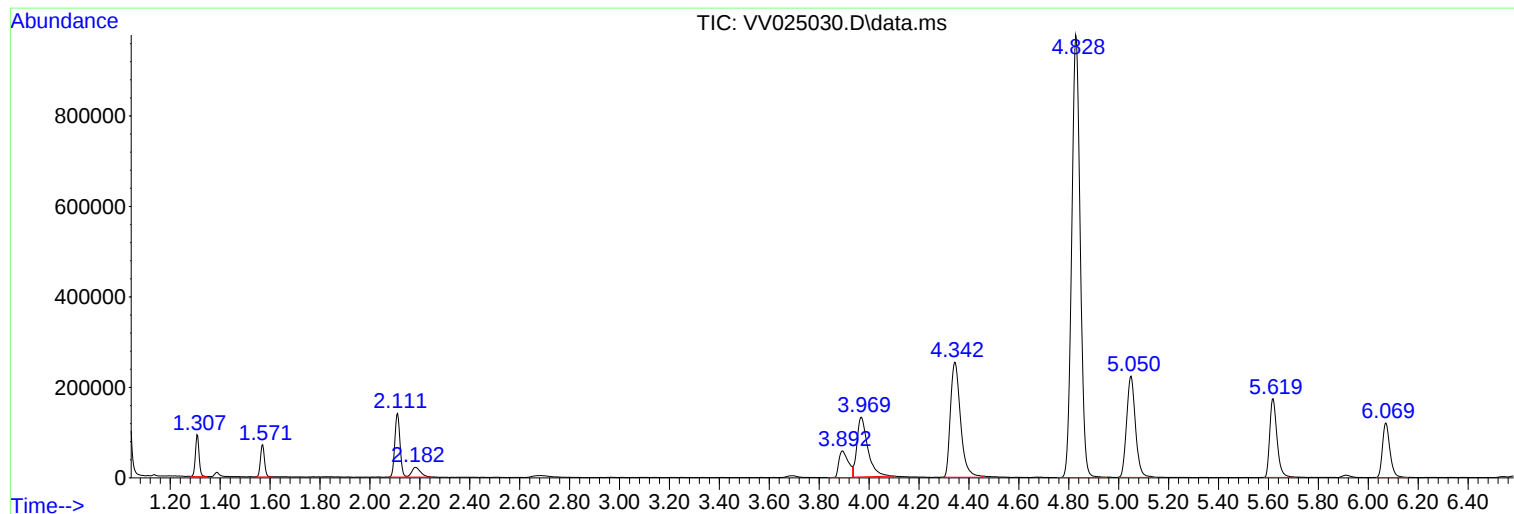

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025030.D
Acq On : 16 Mar 2022 04:42
Operator : SY/MD
Sample : N1933-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025030.D
Acq On : 16 Mar 2022 04:42
Operator : SY/MD
Sample : N1933-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------