


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV024988.D
 Acq On : 15 Mar 2022 09:29
 Operator : SY/MD
 Sample : BFB279
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB279

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 18 02:20:05 2022

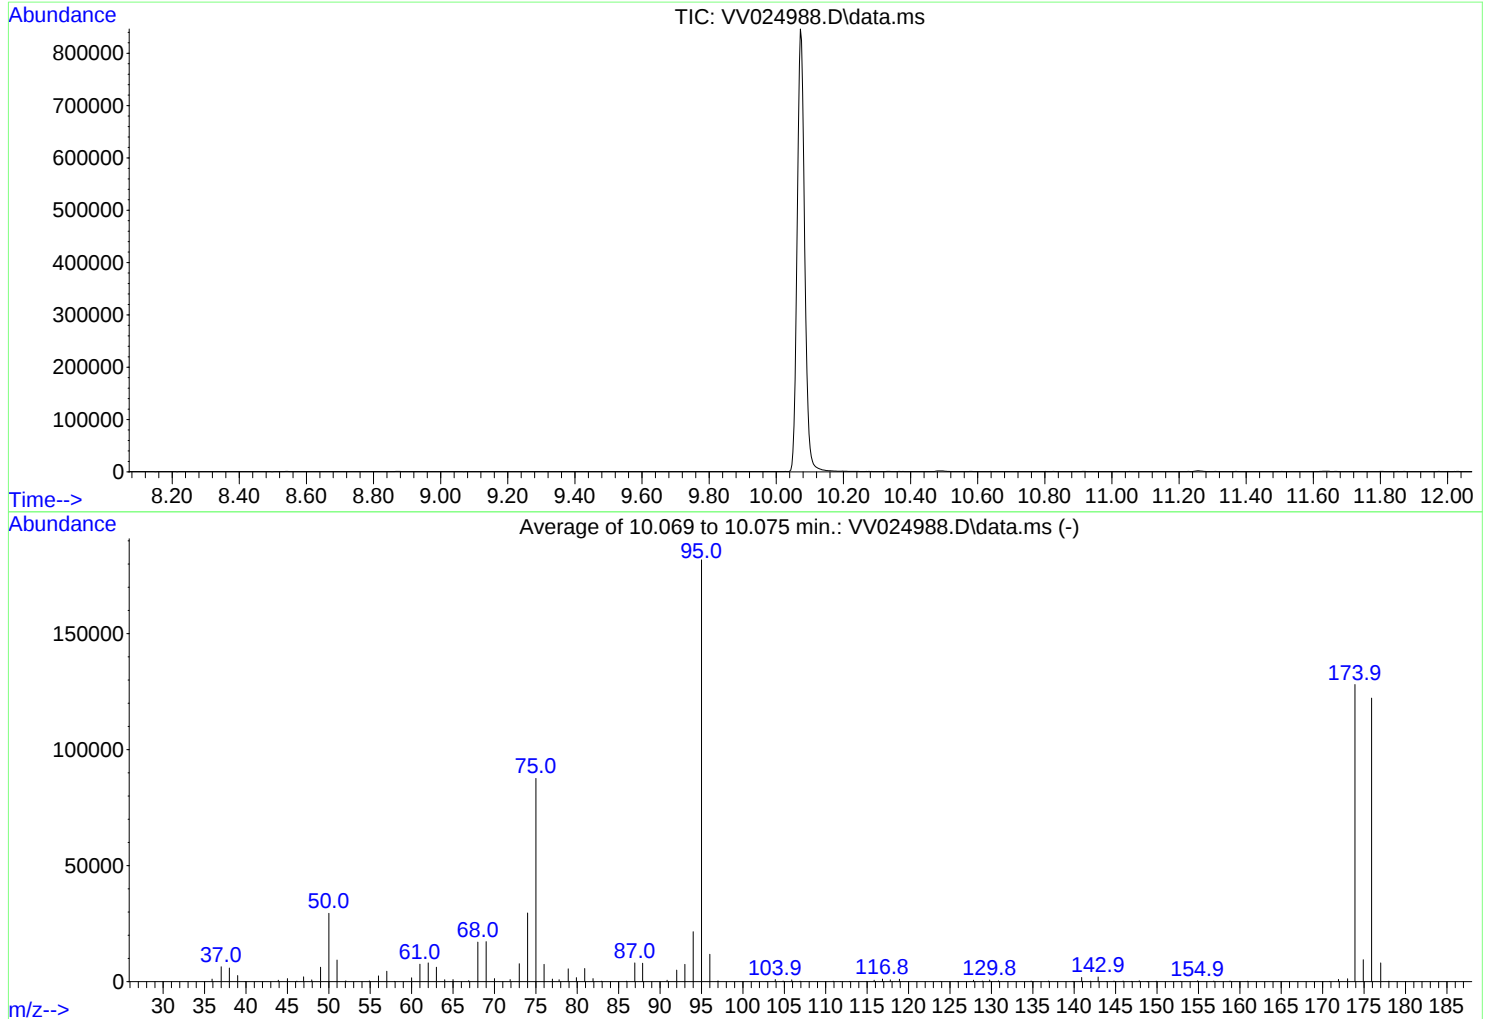

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	29453	PASS
75	95	30	80	48.2	87597	PASS
95	95	100	100	100.0	181781	PASS
96	95	5	9	6.5	11828	PASS
173	174	0.00	2	1.0	1273	PASS
174	95	50	120	70.4	128024	PASS
175	174	5	9	7.4	9472	PASS
176	174	95	105	95.5	122200	PASS
177	176	5	10	6.6	8087	PASS

Scan 2796 (10.030 min): VV024988.D\data.ms
BFB279

m/z	Abundance
39.90	402.0
43.90	370.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

m/z	Abundance
35.90	1041.0
37.00	6273.0
38.00	5834.0
39.00	2511.0
39.90	488.0
44.00	899.0
45.00	1388.0
46.10	209.0
47.00	2014.0
48.00	738.0
49.00	6139.0
50.00	28976.0
51.00	9017.0
52.00	340.0
54.90	375.0
56.00	2502.0
57.00	4434.0
57.90	152.0
60.00	1523.0
61.00	7289.0
62.00	7914.0
63.00	6180.0
64.00	831.0
65.00	951.0
66.90	444.0
68.00	16496.0
69.00	16299.0
70.00	1383.0
71.90	814.0
73.00	7400.0
74.00	28744.0
75.00	84640.0
76.00	7340.0
77.00	1116.0
77.80	769.0
78.90	5280.0
79.90	1654.0
80.90	5535.0
81.90	1377.0
82.90	239.0
86.00	239.0
86.90	7886.0
87.90	7719.0
90.90	658.0
92.00	4666.0
93.00	7222.0
94.00	20656.0
95.00	174208.0
96.00	11978.0
97.00	334.0
103.90	814.0
104.80	266.0
105.90	769.0
106.90	213.0
110.90	149.0
112.90	145.0
114.90	188.0
115.80	625.0
116.90	1073.0
117.80	675.0
118.90	993.0
123.80	152.0
127.80	583.0
128.90	305.0
129.80	582.0
130.80	284.0
134.80	258.0
136.90	284.0
139.80	149.0
140.90	1653.0
142.00	188.0
142.90	1864.0
143.90	118.0
144.80	286.0
145.90	264.0
146.90	133.0
147.90	433.0
148.80	104.0
149.90	165.0
152.80	121.0
154.90	449.0
156.80	292.0
158.80	253.0
161.00	198.0
170.90	151.0
171.90	950.0
173.00	1185.0
173.90	118984.0
174.90	8928.0
175.90	113064.0
177.00	7526.0
178.00	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

m/z	Abundance
35.90	1167.0
37.00	6692.0
38.00	6042.0
39.00	2704.0
39.90	510.0
44.00	1036.0
45.00	1395.0
46.10	208.0
47.00	2117.0
47.90	744.0
49.00	6532.0
50.00	30552.0
51.00	9593.0
52.10	357.0
54.90	391.0
56.00	2610.0
57.00	4589.0
58.00	137.0
60.00	1712.0
61.00	7826.0
62.00	8388.0
63.00	6407.0
64.00	861.0
65.00	929.0
66.90	437.0
68.00	17688.0
69.00	17832.0
70.00	1339.0
71.90	918.0
73.00	8020.0
74.00	30600.0
75.00	90784.0
76.00	7704.0
77.00	1197.0
77.80	858.0
78.90	5735.0
79.90	1837.0
80.90	5790.0
81.90	1354.0
82.90	257.0
85.90	245.0
86.90	8374.0
87.90	8232.0
90.90	657.0
92.00	5155.0
93.00	7692.0
94.00	22416.0
95.00	188672.0
96.00	12199.0
97.00	386.0
102.80	113.0
103.90	918.0
104.80	293.0
105.90	826.0
106.90	195.0
110.90	186.0
111.80	114.0
112.80	177.0
114.90	159.0
115.80	664.0
116.90	1176.0
117.80	791.0
118.90	1060.0
123.80	131.0
127.80	660.0
128.90	311.0
129.80	709.0
130.90	334.0
134.80	264.0
136.90	283.0
139.80	139.0
140.90	1899.0
141.90	220.0
142.90	2098.0
143.90	104.0
144.80	275.0
145.90	275.0
146.90	168.0
147.80	467.0
149.90	187.0
152.90	158.0
154.90	481.0
156.80	326.0
158.80	295.0
160.90	223.0
170.80	157.0
171.90	981.0
173.00	1316.0
173.90	132352.0
174.90	9806.0
175.90	126472.0
177.00	8469.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

178.00

238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

m/z	Abundance
35.90	1183.0
37.00	6309.0
38.00	5655.0
39.00	2699.0
39.90	458.0
43.90	1020.0
45.00	1243.0
46.20	167.0
46.90	2064.0
47.90	725.0
49.00	6029.0
50.00	28832.0
51.00	9263.0
52.10	331.0
54.90	382.0
56.00	2391.0
57.00	4353.0
58.00	126.0
60.00	1657.0
61.00	7476.0
62.00	7937.0
63.00	6050.0
64.00	777.0
65.00	828.0
66.90	368.0
68.00	16872.0
69.00	17512.0
70.00	1237.0
71.90	941.0
73.00	7730.0
74.00	29520.0
75.00	87368.0
76.00	7302.0
77.00	1069.0
77.80	870.0
78.90	5541.0
79.90	1775.0
80.90	5556.0
81.90	1240.0
82.90	206.0
85.90	222.0
87.00	7939.0
87.90	7905.0
90.80	609.0
92.00	5110.0
93.00	7430.0
94.00	21480.0
95.00	182464.0
96.00	11308.0
97.00	420.0
102.80	107.0
103.90	897.0
104.90	296.0
105.90	796.0
106.90	148.0
110.90	205.0
111.80	137.0
112.80	173.0
115.00	153.0
115.90	640.0
116.80	1174.0
117.80	804.0
118.90	1021.0
123.80	107.0
125.90	103.0
127.90	658.0
128.90	296.0
129.80	720.0
130.90	346.0
134.80	247.0
136.90	253.0
139.90	113.0
140.90	1894.0
141.90	245.0
142.90	2093.0
144.80	249.0
145.90	254.0
146.90	168.0
147.80	433.0
149.90	181.0
152.90	168.0
154.90	419.0
156.90	297.0
158.80	265.0
160.90	222.0
170.80	158.0
171.90	974.0
173.00	1319.0
173.90	132736.0
174.90	9682.0
175.90	127064.0
177.00	8267.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

178.00

188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279