

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031622\
 Data File : VW025041.D
 Acq On : 16 Mar 2022 12:42
 Operator : SY/MD
 Sample : N1934-09DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1


Instrument :
 MSVOA_V
 ClientSampleId :


Quant Time: Mar 17 02:02:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 01:58:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	149547	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	142489	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60520	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	51113	4.329	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	86.600%	
7) Chloroethane-d5	1.568	69	41341	4.782	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.600%	
11) 1,1-Dichloroethene-d2	2.108	63	66584	3.489	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.800%	
20) 2-Butanone-d5	3.911	46	79625	55.804	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	111.600%	
24) Chloroform-d	4.349	84	93190	4.759	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.200%	
26) 1,2-Dichloroethane-d4	5.037	65	40991	5.007	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.200%	
32) Benzene-d6	5.050	84	192701	4.662	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.200%	
36) 1,2-Dichloropropane-d6	6.069	67	57312	4.822	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.400%	
41) Toluene-d8	7.316	98	163823	4.349	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.000%	
43) trans-1,3-Dichloroprop...	7.625	79	17379	4.194	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.800%	
46) 2-Hexanone-d5	8.091	63	66769	47.242	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.480%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33802	4.834	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	51638	5.040	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.800%	
Target Compounds						
					Qvalue	
8) Chloroethane	1.307	64	604	0.076	ug/L #	1
21) 2-Butanone	4.002	43	1795	1.192	ug/L	96
25) Chloroform	4.375	83	2425	0.119	ug/L	87
27) 1,2-Dichloroethane	5.056	62	981	0.097	ug/L #	71
31) Carbon tetrachloride	4.828	117	117625	7.545	ug/L	100
35) Methylcyclohexane	6.072	83	14051	0.719	ug/L #	21
37) 1,2-Dichloropropane	6.069	63	5705	0.536	ug/L #	86
39) cis-1,3-Dichloropropene	6.995	75	1100	0.074	ug/L #	57
61) 1,2,3-Trichloropropane	11.246	75	7647	1.502	ug/L #	66

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Mar 17 02:02:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 01:58:56 2022
Response via : Initial Calibration



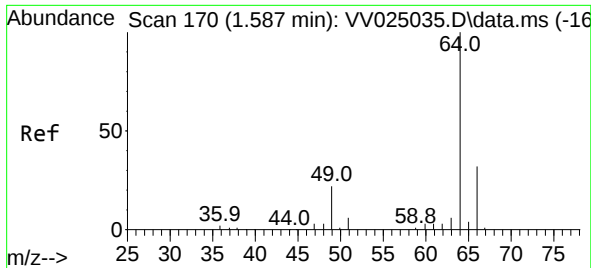

#8

Chloroethane

Concen: 0.076 ug/L

RT: 1.307 min Scan# 81

Delta R.T. -0.280 min

Lab File: VV025041.D

Acq: 16 Mar 2022 12:42

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 64 Resp: 604

Ion Ratio Lower Upper

64 100

66 238.2 22.5 41.7#

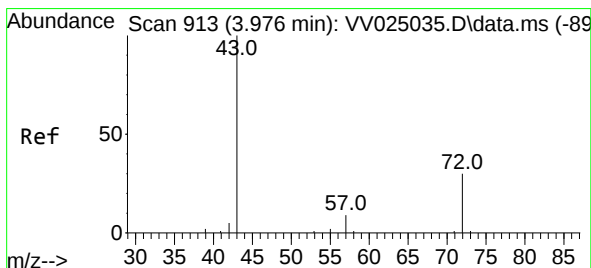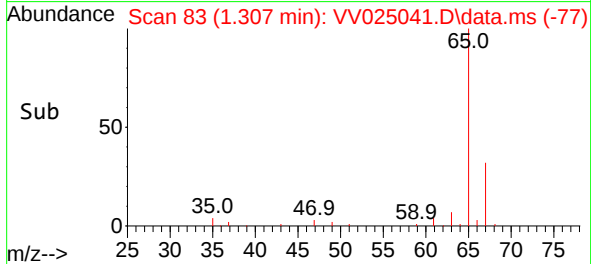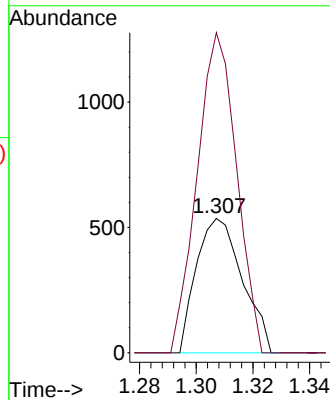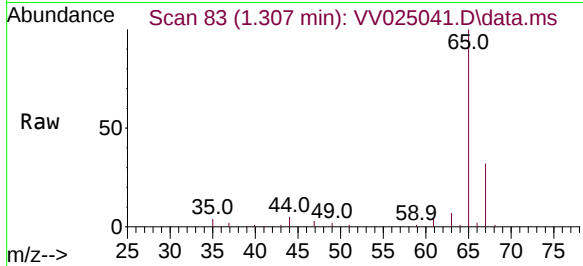

#21

2-Butanone

Concen: 1.192 ug/L

RT: 4.002 min Scan# 921

Delta R.T. 0.026 min

Lab File: VV025041.D




Acq: 16 Mar 2022 12:42


Tgt Ion: 43 Resp: 1795

Ion Ratio Lower Upper

43 100

72 22.5 10.4 31.2

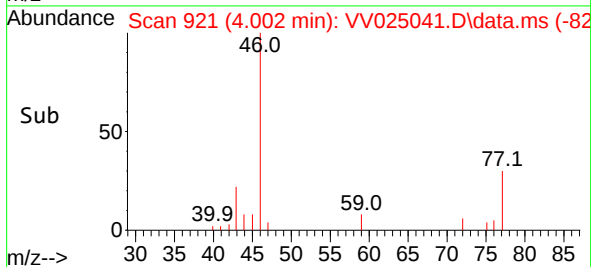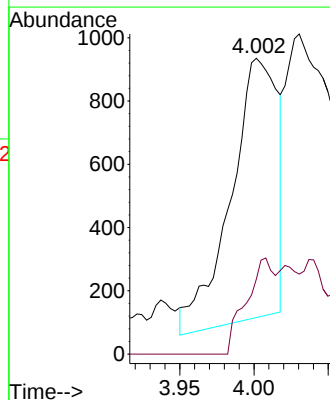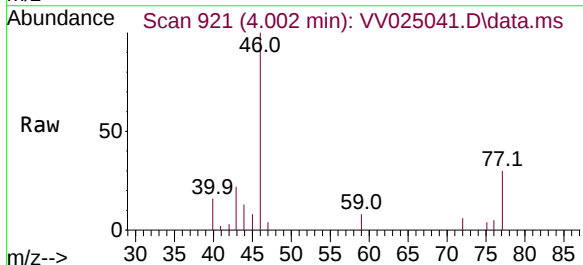

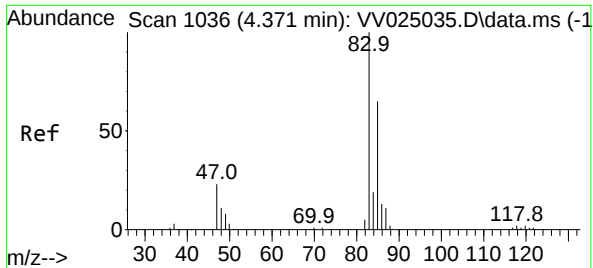

#25

Chloroform

Concen: 0.119 ug/L

RT: 4.375 min Scan# 1

Delta R.T. 0.003 min

Lab File: VV025041.D

Acq: 16 Mar 2022 12:42

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 83 Resp: 2425

Ion Ratio Lower Upper

83 100

85 73.8 44.5 82.7

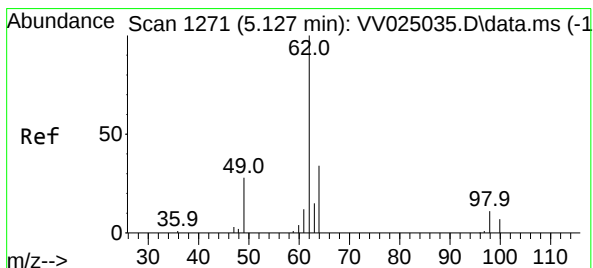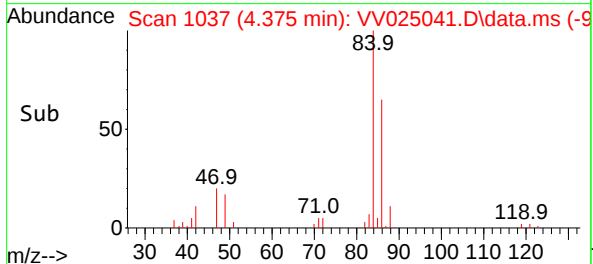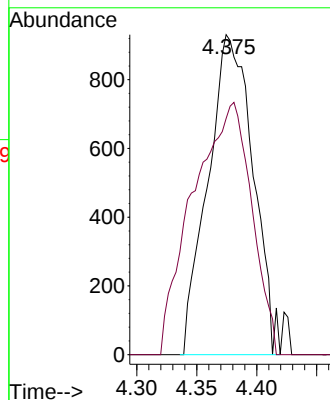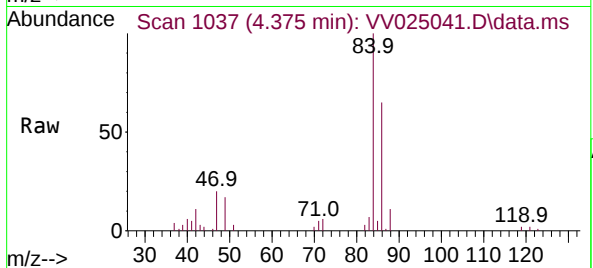

#27

1,2-Dichloroethane

Concen: 0.097 ug/L

RT: 5.056 min Scan# 1249

Delta R.T. -0.071 min

Lab File: VV025041.D




Acq: 16 Mar 2022 12:42


Tgt Ion: 62 Resp: 981

Ion Ratio Lower Upper

62 100

98 0.0 9.0 13.4#


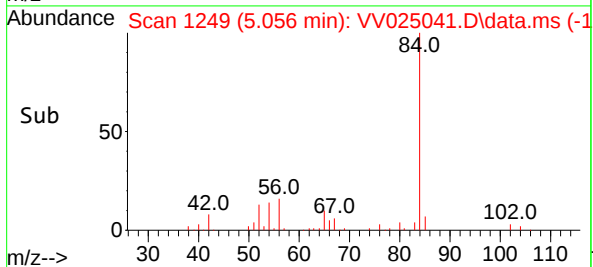
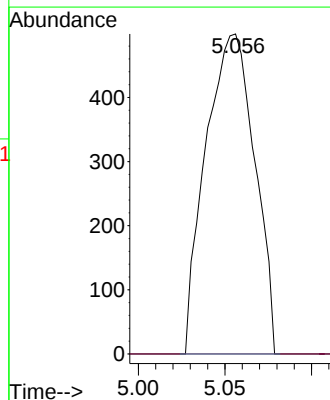
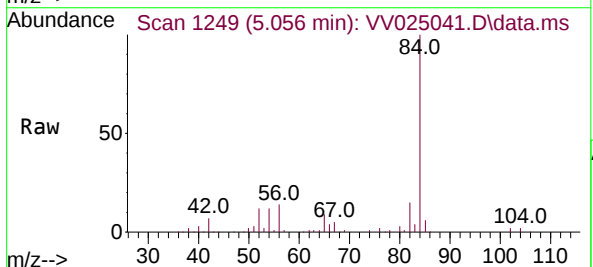


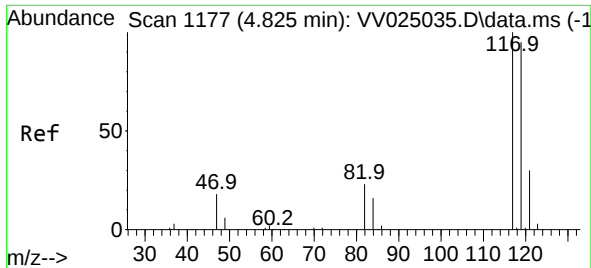

#31
Carbon tetrachloride
Concen: 7.545 ug/L
RT: 4.828 min Scan# 1177
Delta R.T. 0.003 min
Lab File: VV025041.D
Acq: 16 Mar 2022 12:42




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion:117 Resp: 117625
Ion Ratio Lower Upper
117 100
119 95.6 76.8 115.2

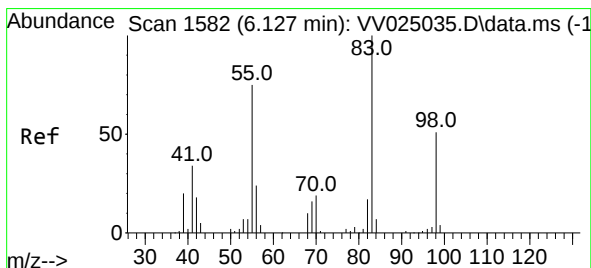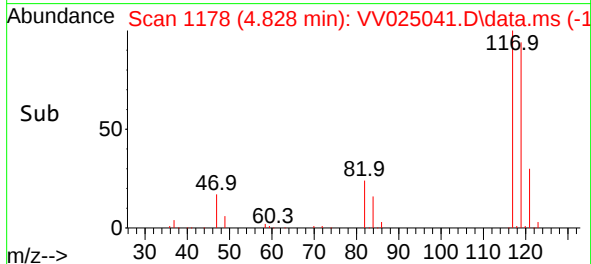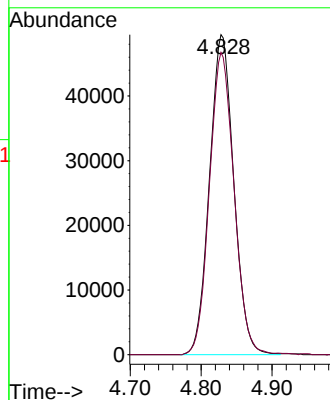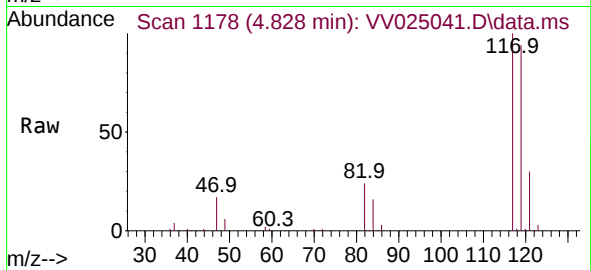

#35
Methylcyclohexane
Concen: 0.719 ug/L
RT: 6.072 min Scan# 1565
Delta R.T. -0.055 min
Lab File: VV025041.D
Acq: 16 Mar 2022 12:42

Tgt Ion: 83 Resp: 14051
Ion Ratio Lower Upper
83 100
55 0.0 55.4 83.0#
98 0.7 38.4 57.6#

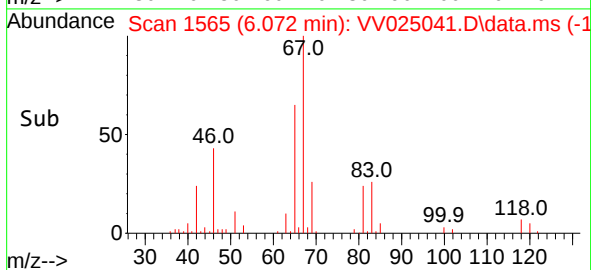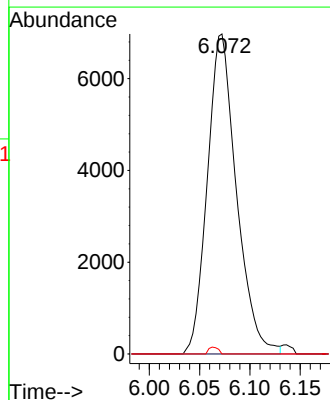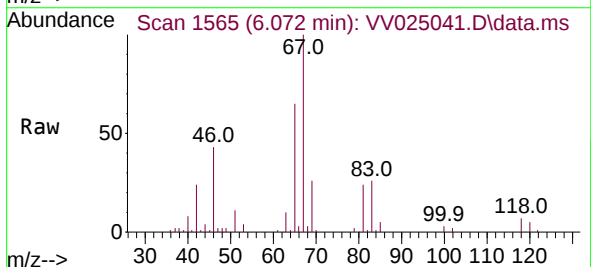

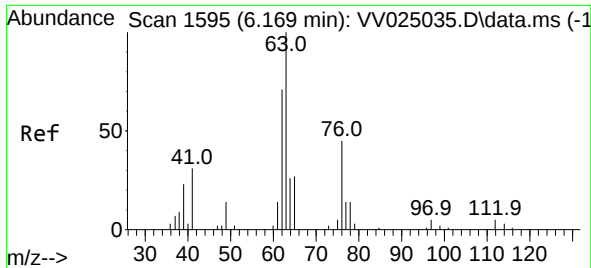

#37

1,2-Dichloropropane

Concen: 0.536 ug/L

RT: 6.069 min Scan# 11

Delta R.T. -0.100 min

Lab File: VV025041.D

Acq: 16 Mar 2022 12:42

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 63 Resp: 5705

Ion Ratio Lower Upper

63 100

112 0.0 3.8 5.6#

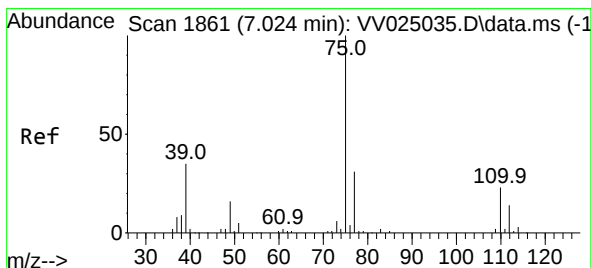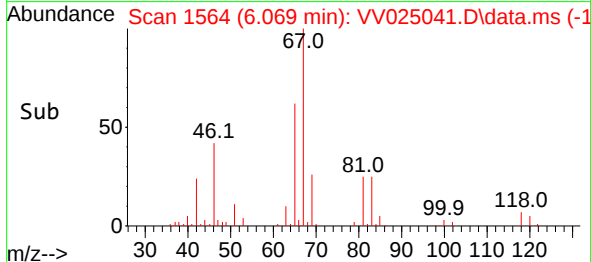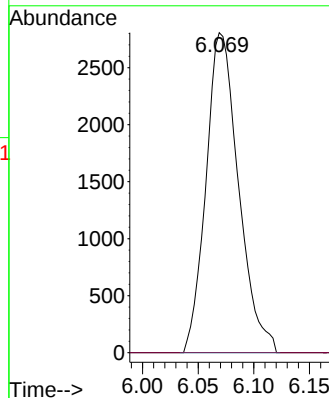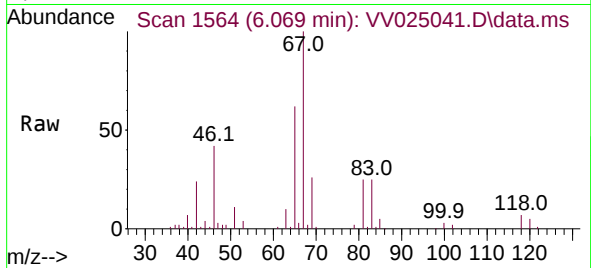

#39

cis-1,3-Dichloropropene

Concen: 0.074 ug/L

RT: 6.995 min Scan# 1852

Delta R.T. -0.029 min

Lab File: VV025041.D




Acq: 16 Mar 2022 12:42


Tgt Ion: 75 Resp: 1100

Ion Ratio Lower Upper

75 100

77 57.3 23.0 42.8#

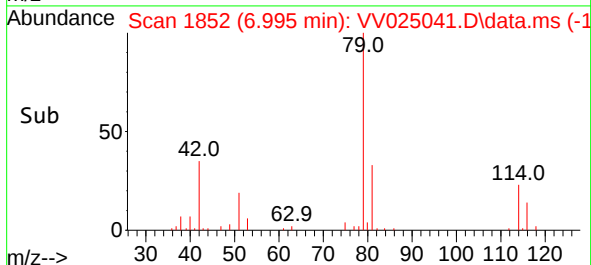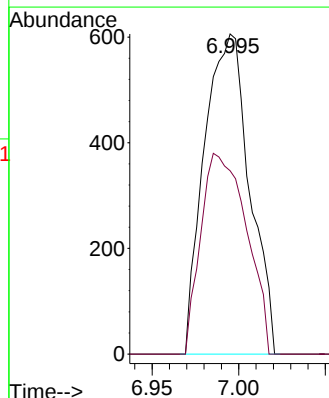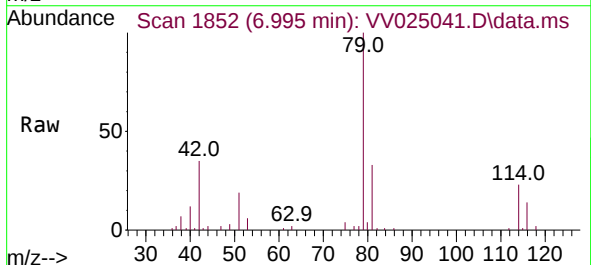

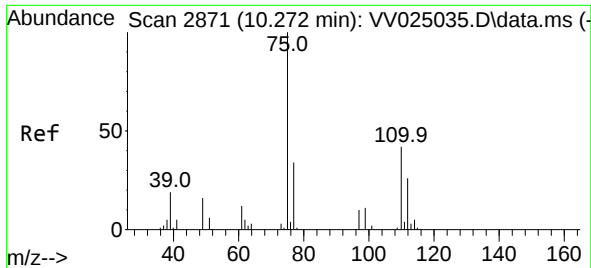

#61

1,2,3-Trichloropropane

Concen: 1.502 ug/L

RT: 11.246 min Scan# 31

Delta R.T. 0.974 min


Lab File: VV025041.D

Acq: 16 Mar 2022 12:42

Instrument :

MSVOA_V

ClientSampleId :

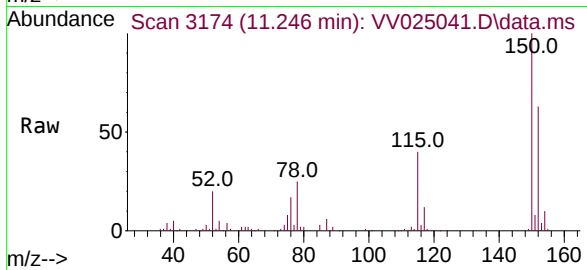

Tgt Ion: 75	Resp:	7647
Ion Ratio	Lower	Upper
75	100	
77	33.5	25.7 38.5
110	2.0	31.2 46.8#

