




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025039.D
 Acq On : 16 Mar 2022 11:56
 Operator : SY/MD
 Sample : N1934-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDE0

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:01:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 01:58:56 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/17/2022
 Supervised By :Mahesh Dadoda 03/17/2022

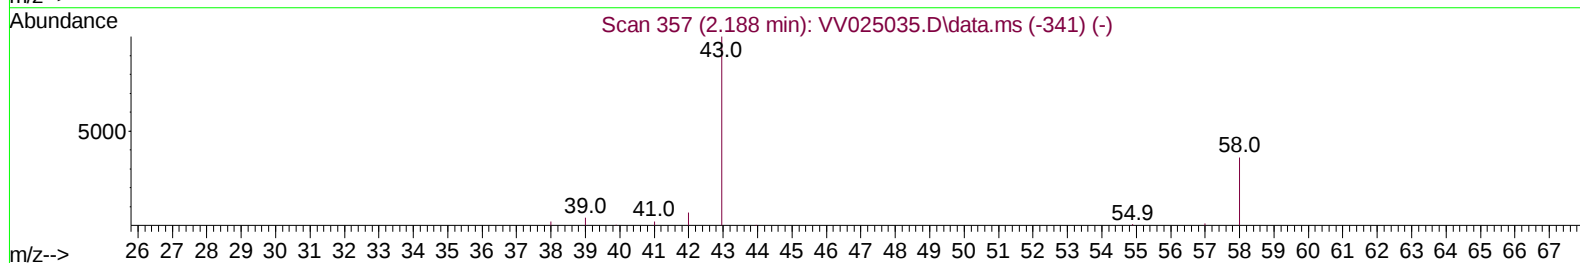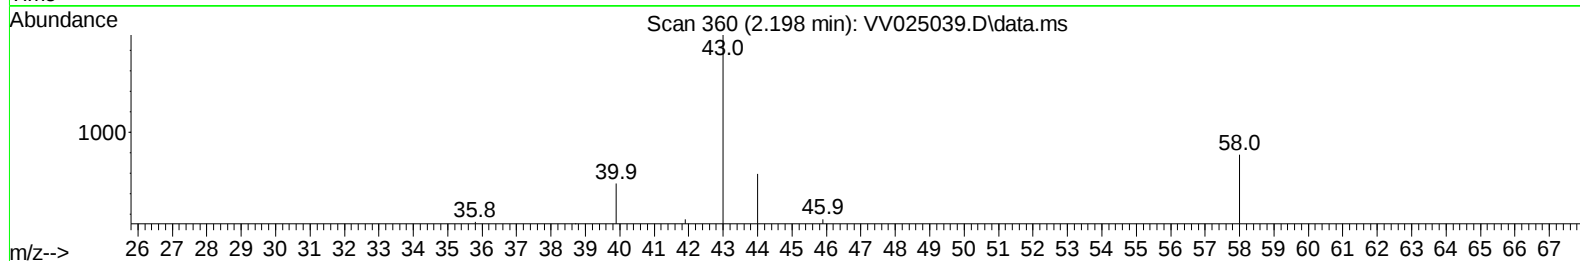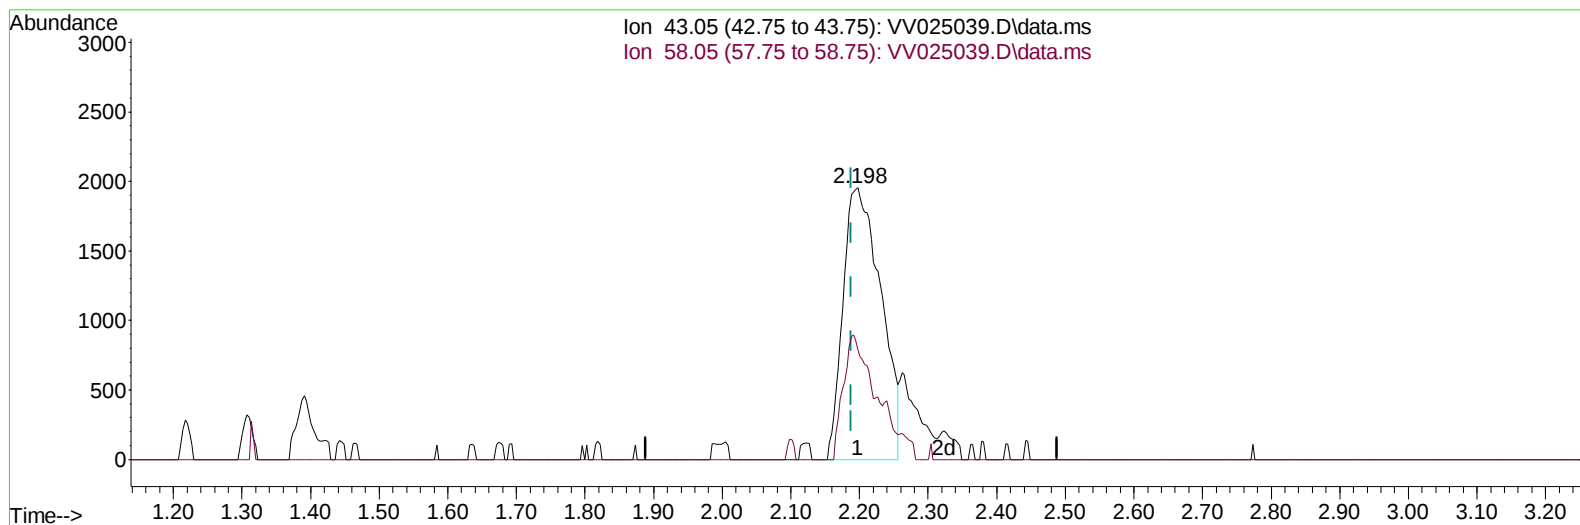

TIC: VV025039.D\data.ms

(13) Acetone (T)

2.198min (+ 0.010) 7.50 ug/L

response 7454

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.10	33.58
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025039.D
Acq On : 16 Mar 2022 11:56
Operator : SY/MD
Sample : N1934-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDE0

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:01:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 01:58:56 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/17/2022
Supervised By :Mahesh Dadoda 03/17/2022

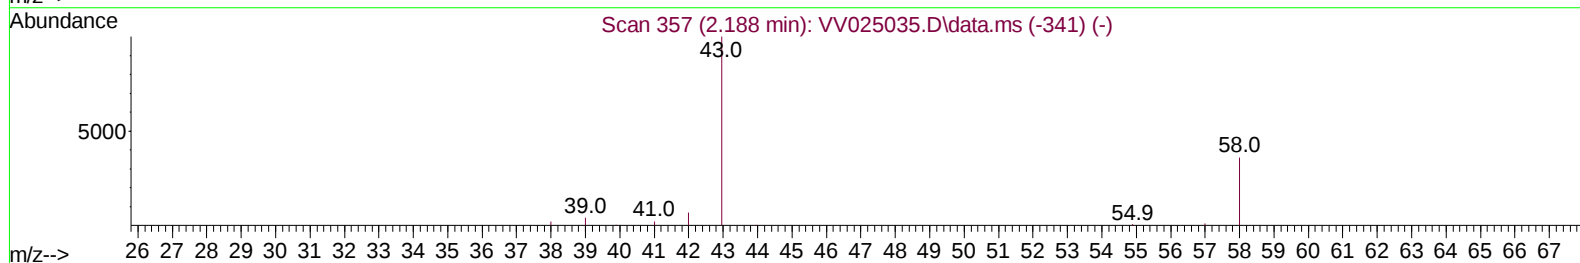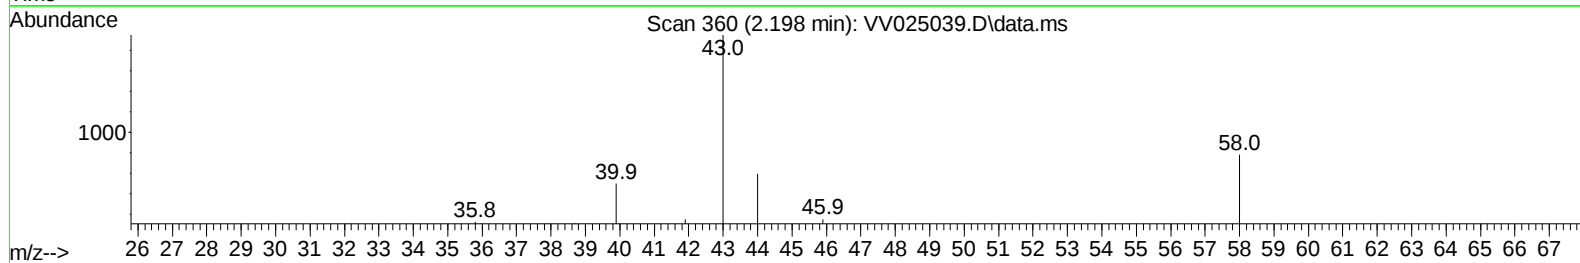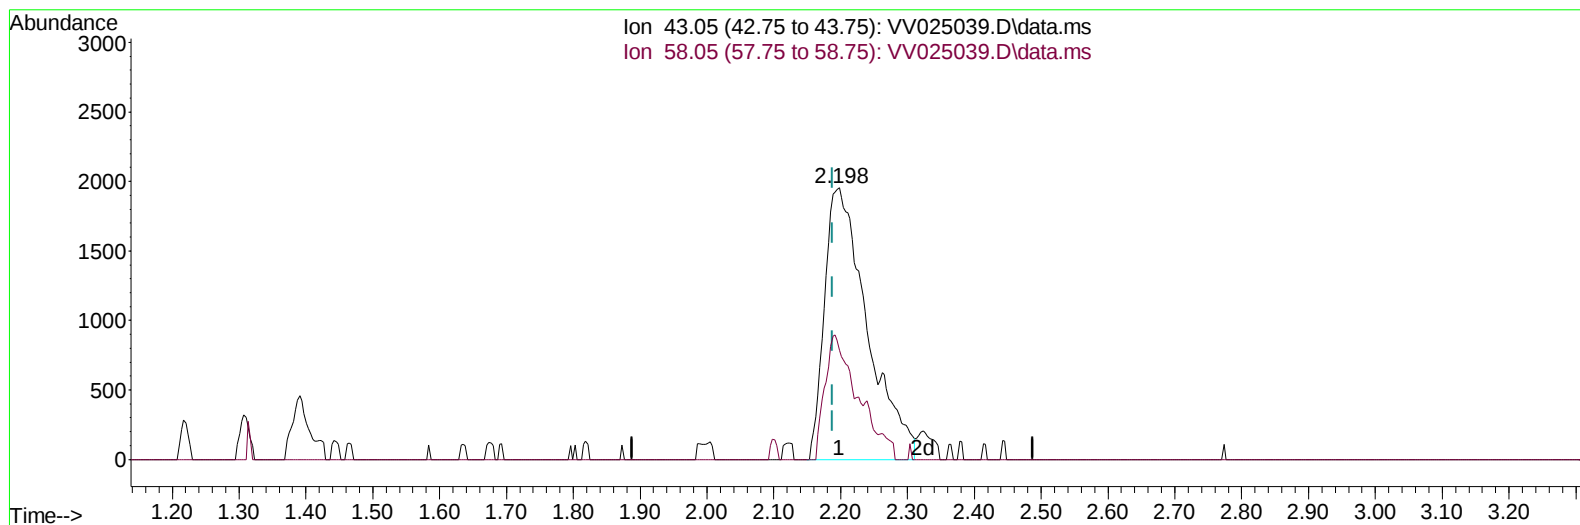

TIC: VV025039.D\data.ms

(13) Acetone (T)

2.198min (+ 0.010) 8.68 ug/L m

response 8627

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.10	29.01
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025039.D
 Acq On : 16 Mar 2022 11:56
 Operator : SY/MD
 Sample : N1934-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDE0

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:01:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 01:58:56 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/17/2022
 Supervised By :Mahesh Dadoda 03/17/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		155673	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117		148193	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		64479	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.307	65		51302	4.174	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	83.400%		
7) Chloroethane-d5	1.568	69		41140	4.571	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	91.400%		
11) 1,1-Dichloroethene-d2	2.108	63		66985	3.372	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	67.400%		
20) 2-Butanone-d5	3.905	46		85268	57.408	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130		Recovery =	114.820%		
24) Chloroform-d	4.349	84		94629	4.642	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	92.800%		
26) 1,2-Dichloroethane-d4	5.034	65		40236	4.721	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	94.400%		
32) Benzene-d6	5.050	84		193279	4.496	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	90.000%		
36) 1,2-Dichloropropane-d6	6.072	67		58996	4.772	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	95.400%		
41) Toluene-d8	7.317	98		166316	4.245	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	84.800%		
43) trans-1,3-Dichloroprop...	7.625	79		18329	4.253	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	85.000%		
46) 2-Hexanone-d5	8.091	63		64735	44.040	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	88.080%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84		32239	4.433	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	88.600%		
66) 1,2-Dichlorobenzene-d4	11.622	152		54663	5.008	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	100.200%		
Target Compounds							
13) Acetone	2.198	43		8627m	8.685	ug/L	
25) Chloroform	4.381	83		36792	1.740	ug/L	96
38) Bromodichloromethane	6.516	83		1934	0.138	ug/L #	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025039.D
Acq On : 16 Mar 2022 11:56
Operator : SY/MD
Sample : N1934-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDE0

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:01:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 01:58:56 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/17/2022
Supervised By :Mahesh Dadoda 03/17/2022

