

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025040.D
 Acq On : 16 Mar 2022 12:19
 Operator : SY/MD
 Sample : N1934-08DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDD8DL

Manual IntegrationsAPPROVED

Reviewed By :John

Carlone




03/17/2022

Supervised By :Mahesh

Dadoda

03/17/2022

Quant Time: Mar 17 02:01:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 01:58:56 2022
 Response via : Initial Calibration

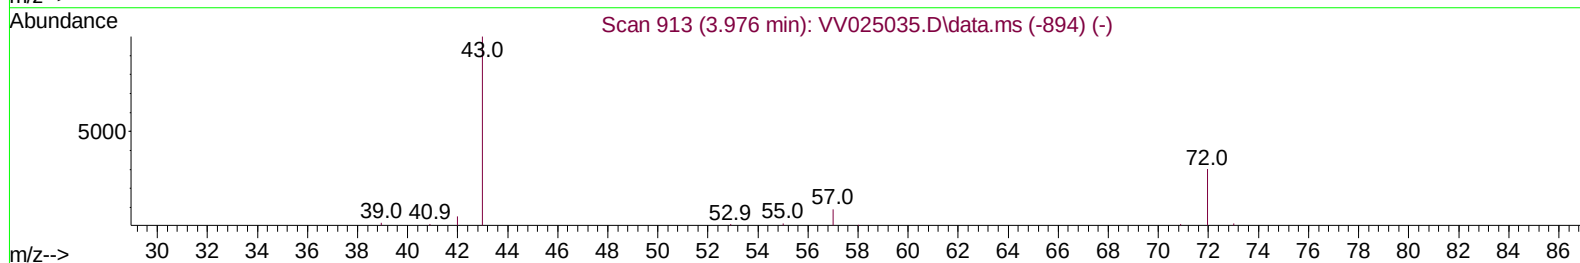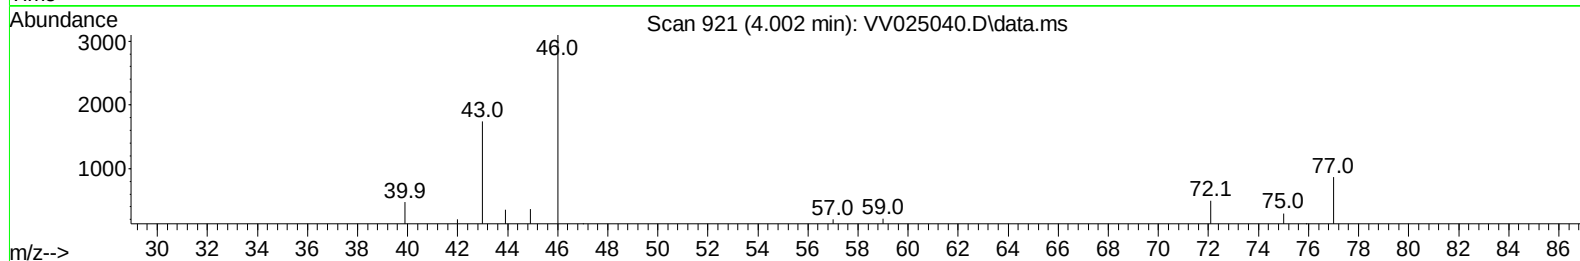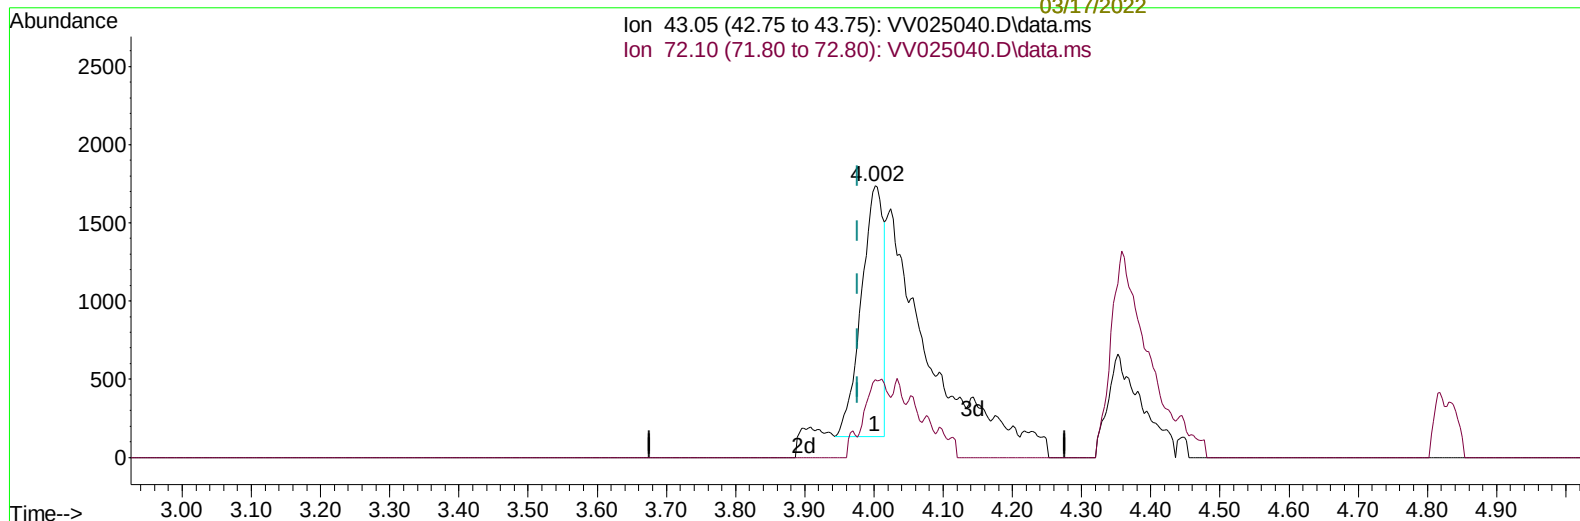

TIC: VV025040.D\data.ms

(21) 2-Butanone (T)

4.002min (+ 0.026) 1.80 ug/L

response 3497

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	20.80	30.17
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025040.D
 Acq On : 16 Mar 2022 12:19
 Operator : SY/MD
 Sample : N1934-08DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDD8DL

Manual IntegrationsAPPROVED

Reviewed By :John

Carlone




03/17/2022

Supervised By :Mahesh

Dadoda

03/17/2022

Quant Time: Mar 17 02:01:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 01:58:56 2022
 Response via : Initial Calibration

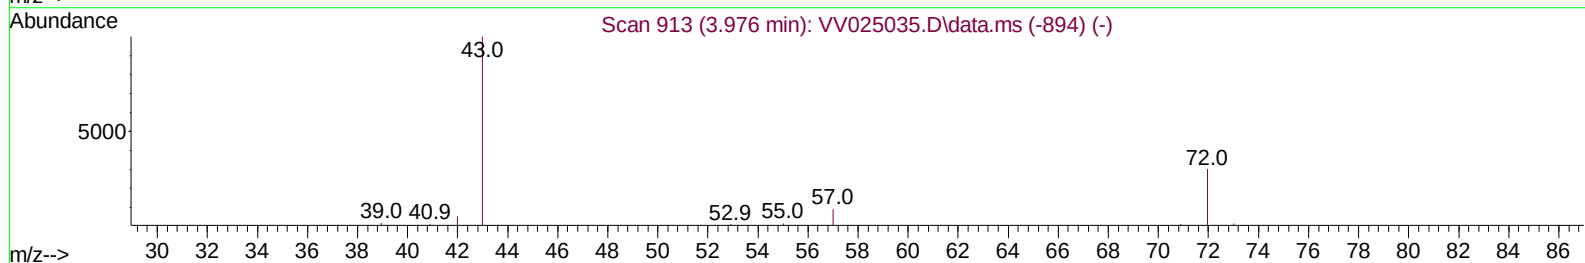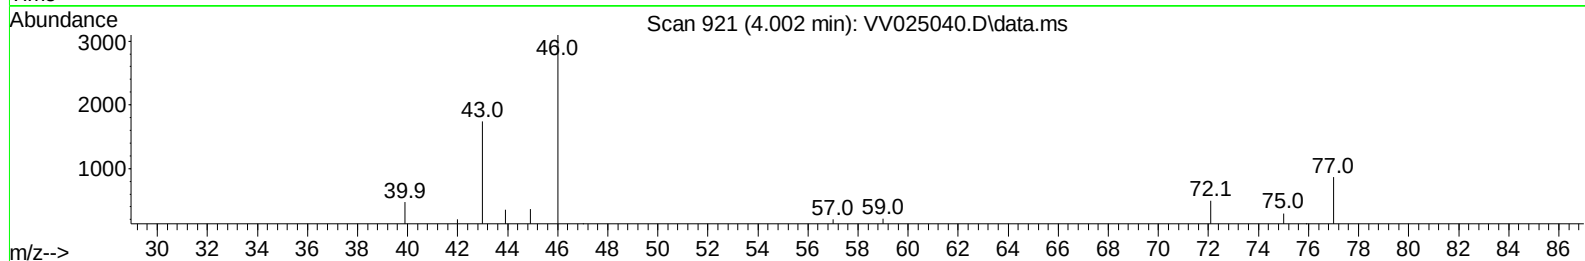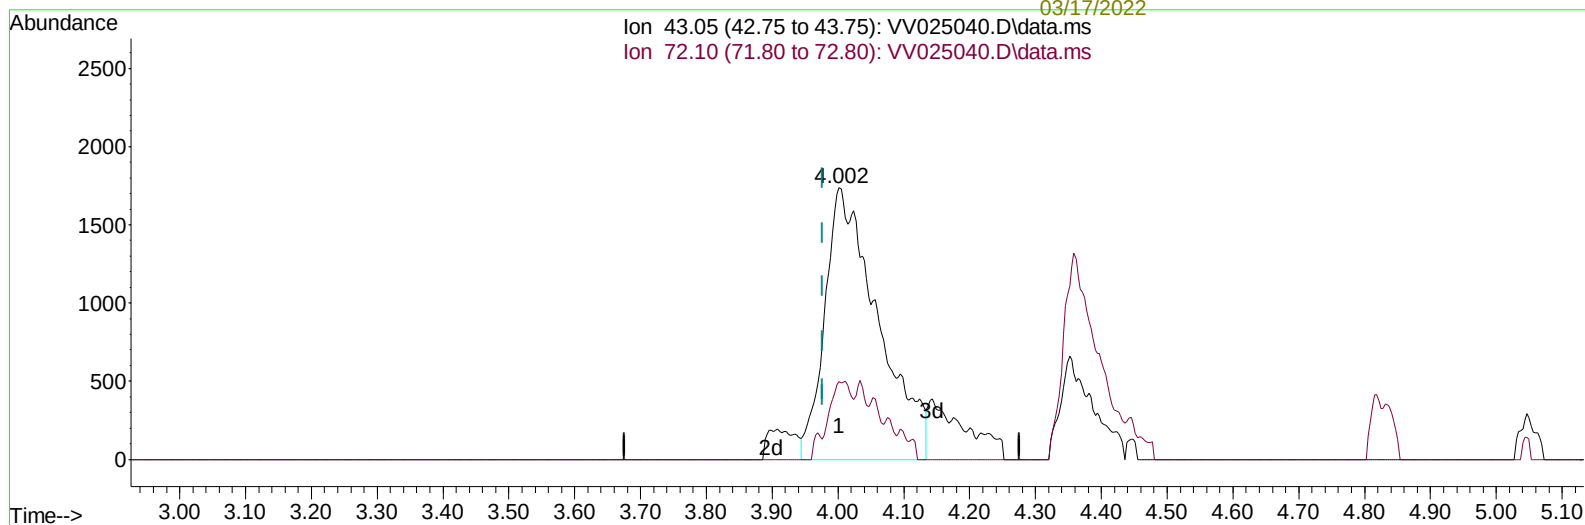

TIC: VV025040.D\data.ms

(21) 2-Butanone (T)

4.002min (+ 0.026) 5.01 ug/L m

response 9725

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	20.80	10.85
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025040.D
 Acq On : 16 Mar 2022 12:19
 Operator : SY/MD
 Sample : N1934-08DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDD8DL

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:01:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 01:58:56 2022
 Response via : Initial Calibration

Reviewed By :John




Carlone

03/17/2022

Supervised By :Mahesh

Dadoda

03/17/2022

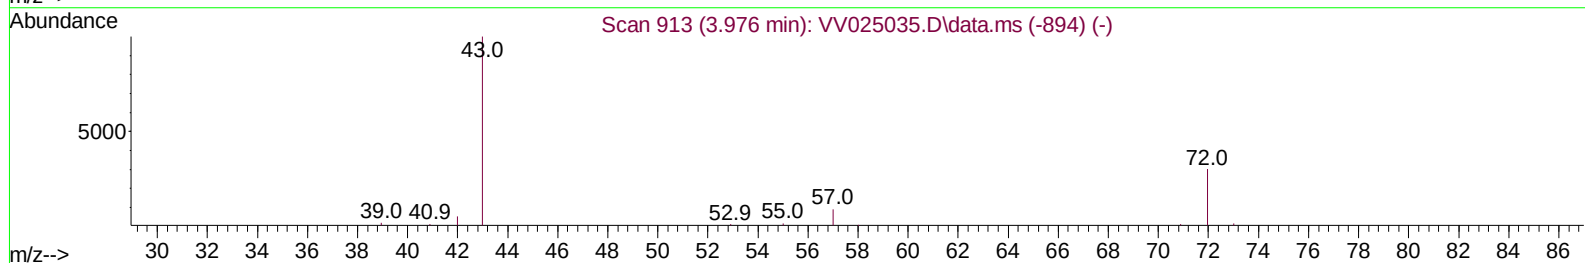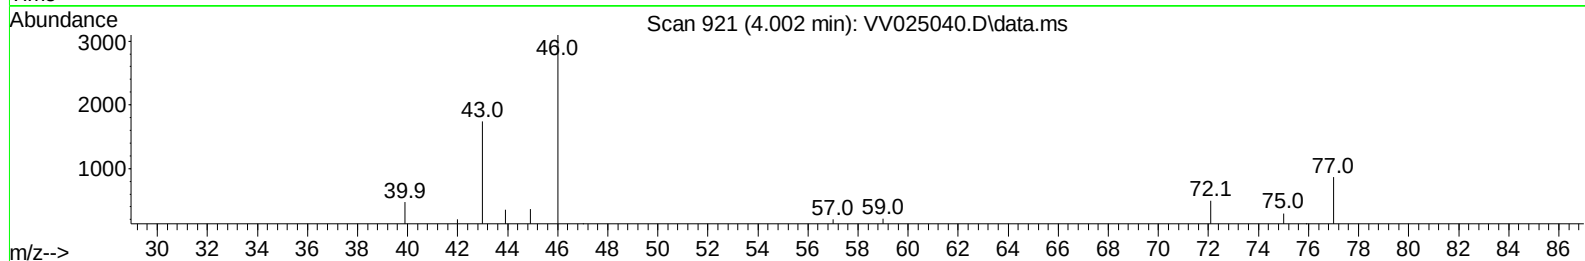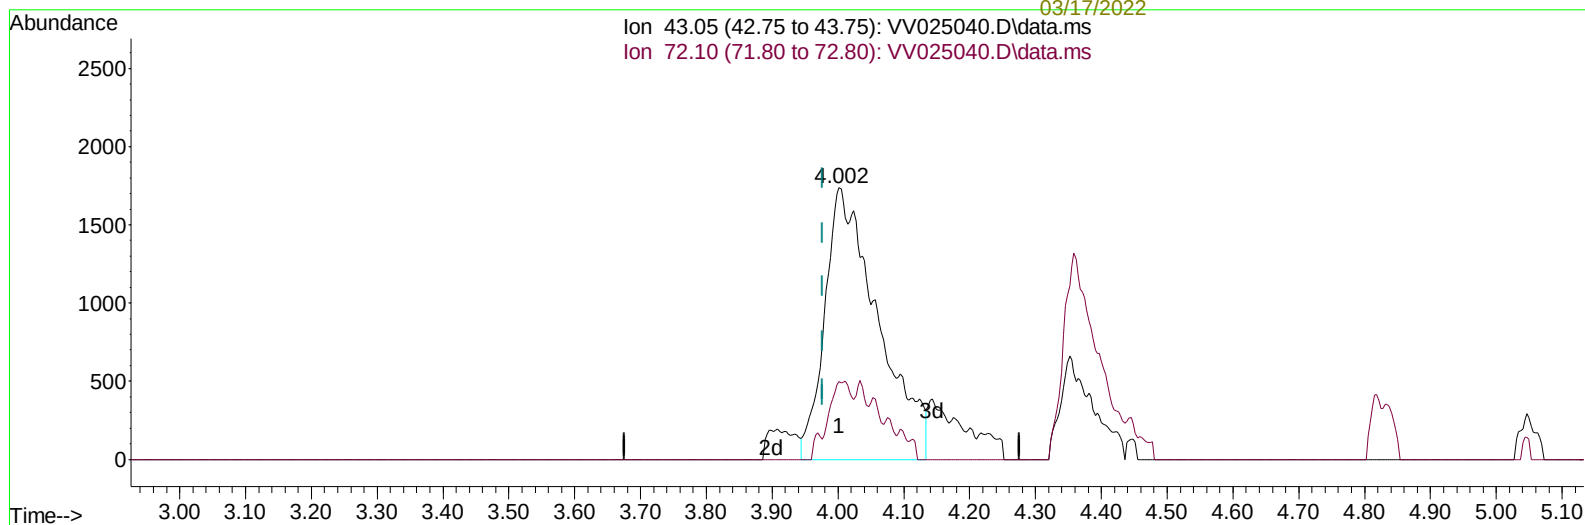

TIC: VV025040.D\data.ms

(21) 2-Butanone (T)

4.002min (+ 0.026) 5.01 ug/L m

response 9725

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	20.80	10.85
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025040.D
 Acq On : 16 Mar 2022 12:19
 Operator : SY/MD
 Sample : N1934-08DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDD8DL

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:01:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 01:58:56 2022
 Response via : Initial Calibration

Reviewed By :John
 Carlone
 03/17/2022
 Supervised By :Mahesh
 Dadoda
 03/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	192881	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	183165	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	78095	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	57834	3.798	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	76.000%	
7) Chloroethane-d5	1.568	69	46621	4.181	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	83.600%	
11) 1,1-Dichloroethene-d2	2.105	63	76380	3.103	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	62.000%	
20) 2-Butanone-d5	3.905	46	102064	55.460	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130	Recovery	=	110.920%	
24) Chloroform-d	4.349	84	107562	4.259	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	85.200%	
26) 1,2-Dichloroethane-d4	5.034	65	47634	4.511	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	90.200%	
32) Benzene-d6	5.050	84	227336	4.279	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	85.600%	
36) 1,2-Dichloropropane-d6	6.069	67	67400	4.411	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	88.200%	
41) Toluene-d8	7.317	98	194404	4.015	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	80.200%	
43) trans-1,3-Dichloroprop...	7.625	79	21157	3.972	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	79.400%	
46) 2-Hexanone-d5	8.091	63	80512	44.315	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	88.620%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	38919	4.330	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	86.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	62001	4.690	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	93.800%	
Target Compounds						
						Qvalue
21) 2-Butanone	4.002	43	9725m	5.006	ug/L	
25) Chloroform	4.378	83	3539	0.135	ug/L	93
31) Carbon tetrachloride	4.828	117	132319	6.603	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025040.D
Acq On : 16 Mar 2022 12:19
Operator : SY/MD
Sample : N1934-08DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD8DL

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:01:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 01:58:56 2022
Response via : Initial Calibration

Reviewed By :John

Carlone

03/17/2022

Supervised By :Mahesh

Dadoda

03/17/2022

