




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025059.D
Acq On : 16 Mar 2022 19:44
Operator : SY/MD
Sample : N1941-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF5

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/17/2022
Supervised By :Mahesh Dadoda 03/18/2022

Quant Time: Mar 17 02:06:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 01:58:56 2022
Response via : Initial Calibration

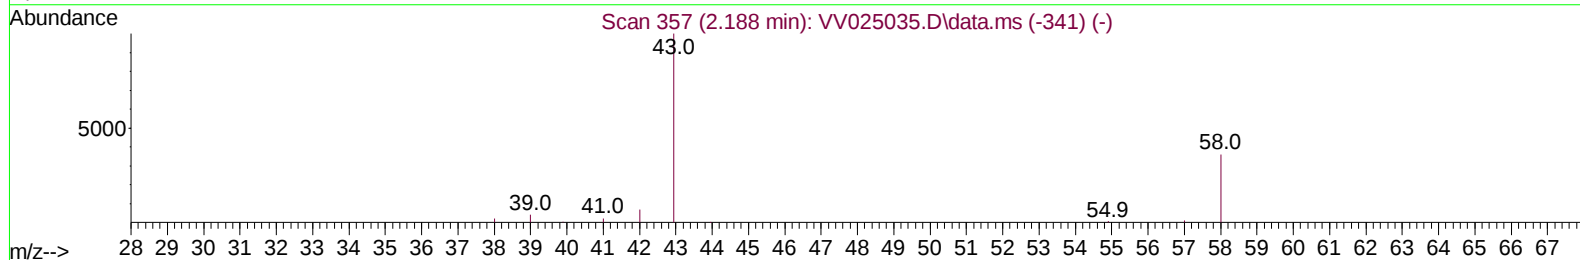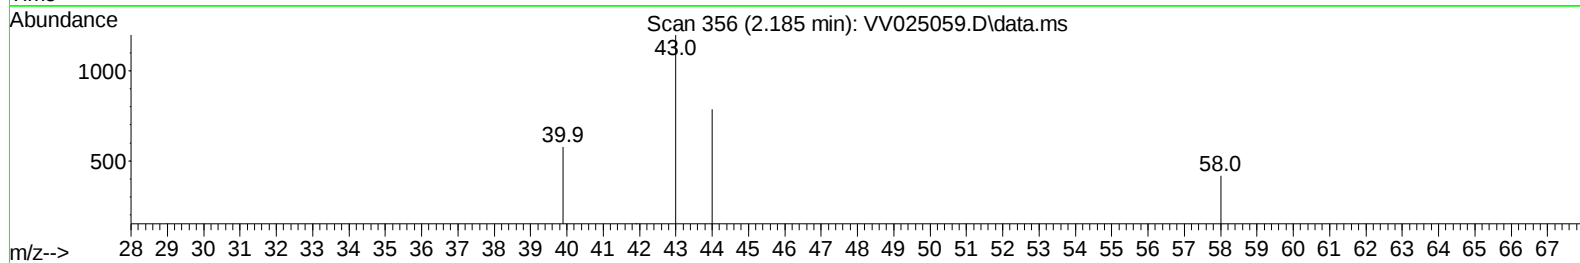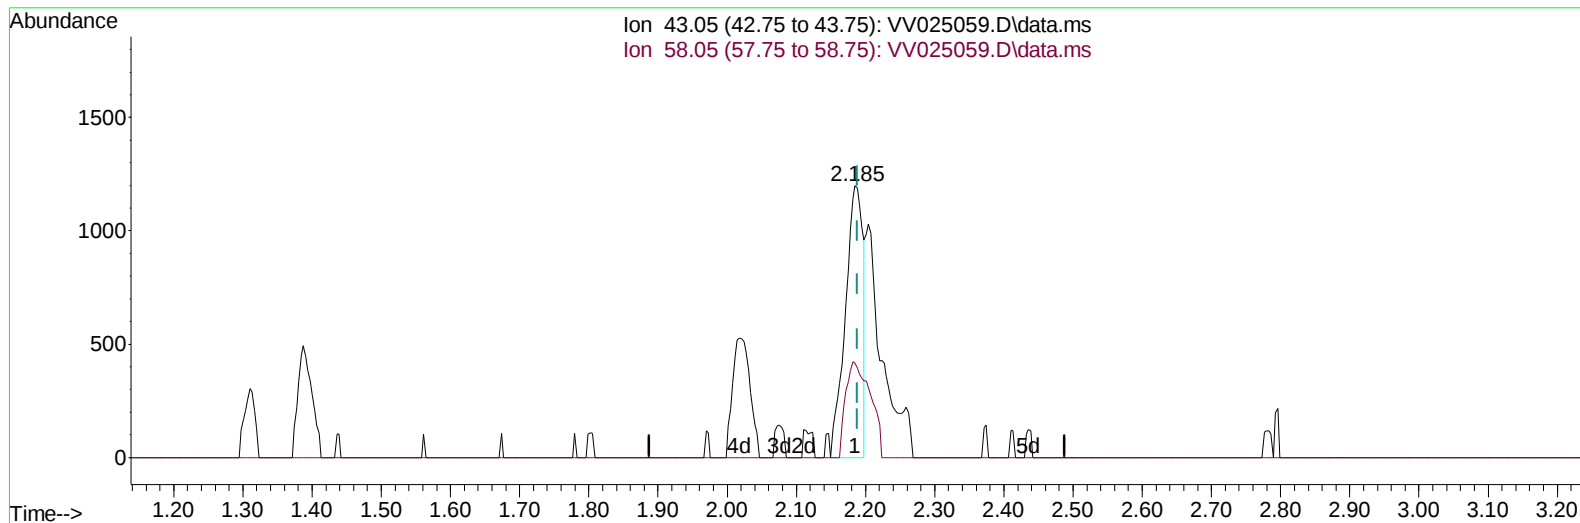

TIC: VV025059.D\data.ms

(13) Acetone (T)

2.185min (-0.003) 2.22 ug/L

response 2118

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.10	49.15
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025059.D
Acq On : 16 Mar 2022 19:44
Operator : SY/MD
Sample : N1941-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF5

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/17/2022
Supervised By :Mahesh Dadoda 03/18/2022

Quant Time: Mar 17 02:06:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 01:58:56 2022
Response via : Initial Calibration

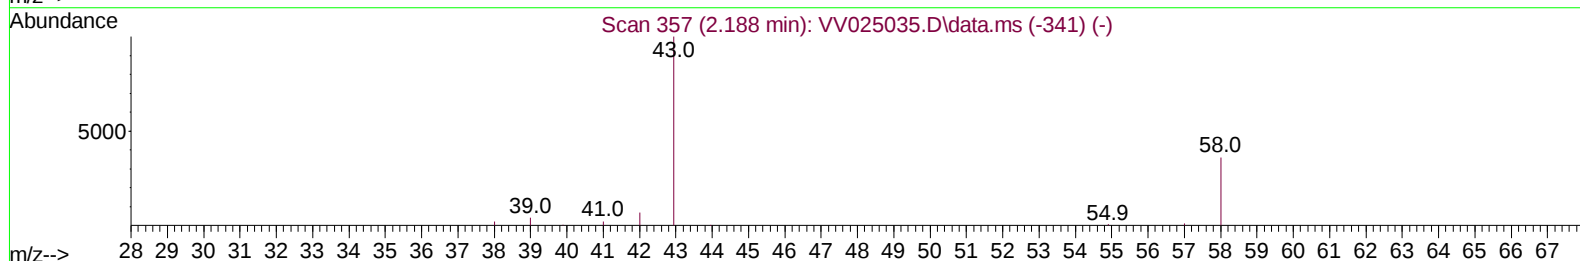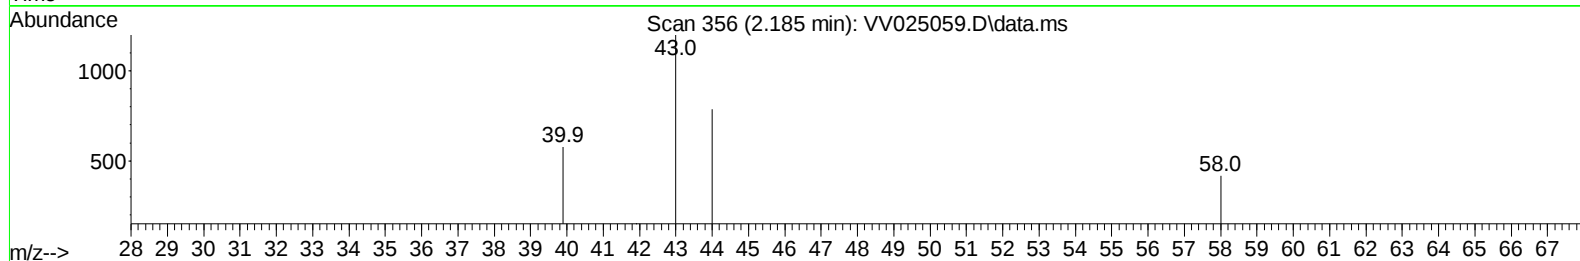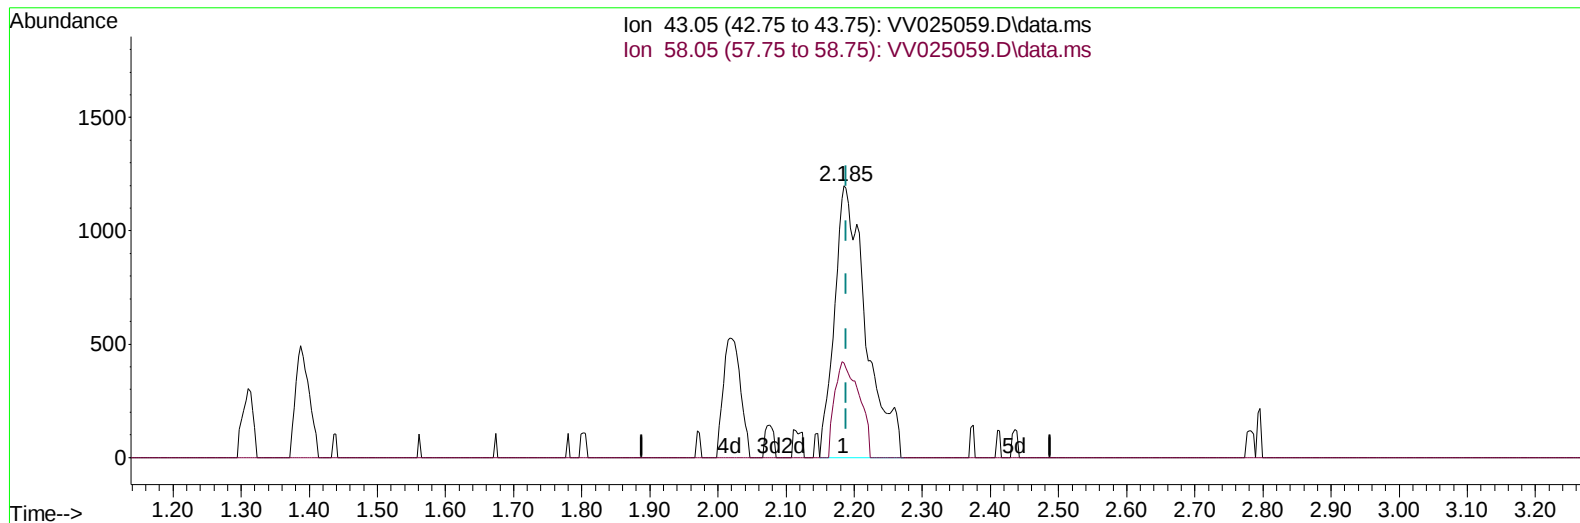

TIC: VV025059.D\data.ms

(13) Acetone (T)

2.185min (-0.003) 4.03 ug/L m

response 3841

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.10	27.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025059.D
 Acq On : 16 Mar 2022 19:44
 Operator : SY/MD
 Sample : N1941-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLF5

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:06:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 01:58:56 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/17/2022
 Supervised By :Mahesh Dadoda 03/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	149359	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	145181	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62712	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	46842	3.972	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	79.400%	
7) Chloroethane-d5	1.571	69	38845	4.499	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	90.000%	
11) 1,1-Dichloroethene-d2	2.111	63	61966	3.251	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	65.000%	
20) 2-Butanone-d5	3.895	46	84926	59.594	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	119.180%	
24) Chloroform-d	4.352	84	89167	4.559	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	91.200%	
26) 1,2-Dichloroethane-d4	5.037	65	39791	4.867	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	97.400%	
32) Benzene-d6	5.053	84	180830	4.294	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	85.800%	
36) 1,2-Dichloropropane-d6	6.072	67	56713	4.683	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	93.600%	
41) Toluene-d8	7.316	98	155087	4.040	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	80.800%	
43) trans-1,3-Dichloroprop...	7.625	79	16408	3.886	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	77.800%	
46) 2-Hexanone-d5	8.088	63	64135	44.537	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	89.080%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	32578	4.573	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	91.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	51616	4.862	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	97.200%	
Target Compounds						
						Qvalue
3) Chloromethane	1.243	50	2065	0.166	ug/L	96
13) Acetone	2.185	43	3841m	4.030	ug/L	
47) Tetrachloroethene	7.979	164	2454	0.277	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025059.D
Acq On : 16 Mar 2022 19:44
Operator : SY/MD
Sample : N1941-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF5

Manual IntegrationsAPPROVED

Quant Time: Mar 17 02:06:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 01:58:56 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/17/2022
Supervised By :Mahesh Dadoda 03/18/2022

