

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031622\
 Data File : VW025062.D
 Acq On : 16 Mar 2022 21:41
 Operator : SY/MD
 Sample : N1941-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLF6

Quant Time: Mar 17 06:27:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 05:44:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	149928	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	143125	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61565	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	45792	3.869	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.400%	
7) Chloroethane-d5	1.568	69	38019	4.386	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	87.800%	
11) 1,1-Dichloroethene-d2	2.108	63	59815	3.127	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	62.600%	
20) 2-Butanone-d5	3.895	46	85374	59.681	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	119.360%	
24) Chloroform-d	4.349	84	88924	4.530	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.600%	
26) 1,2-Dichloroethane-d4	5.034	65	39054	4.758	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.200%	
32) Benzene-d6	5.050	84	179892	4.333	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.600%	
36) 1,2-Dichloropropane-d6	6.072	67	54824	4.592	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	91.800%	
41) Toluene-d8	7.317	98	153203	4.049	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	81.000%	
43) trans-1,3-Dichloroprop...	7.628	79	16970	4.077	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	81.600%	
46) 2-Hexanone-d5	8.088	63	64839	45.672	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.340%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31850	4.535	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	90.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	51562	4.947	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.000%	
Target Compounds						
13) Acetone	2.188	43	4065	4.249	ug/L	Qvalue 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025062.D
Acq On : 16 Mar 2022 21:41
Operator : SY/MD
Sample : N1941-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF6

Quant Time: Mar 17 06:27:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 05:44:36 2022
Response via : Initial Calibration

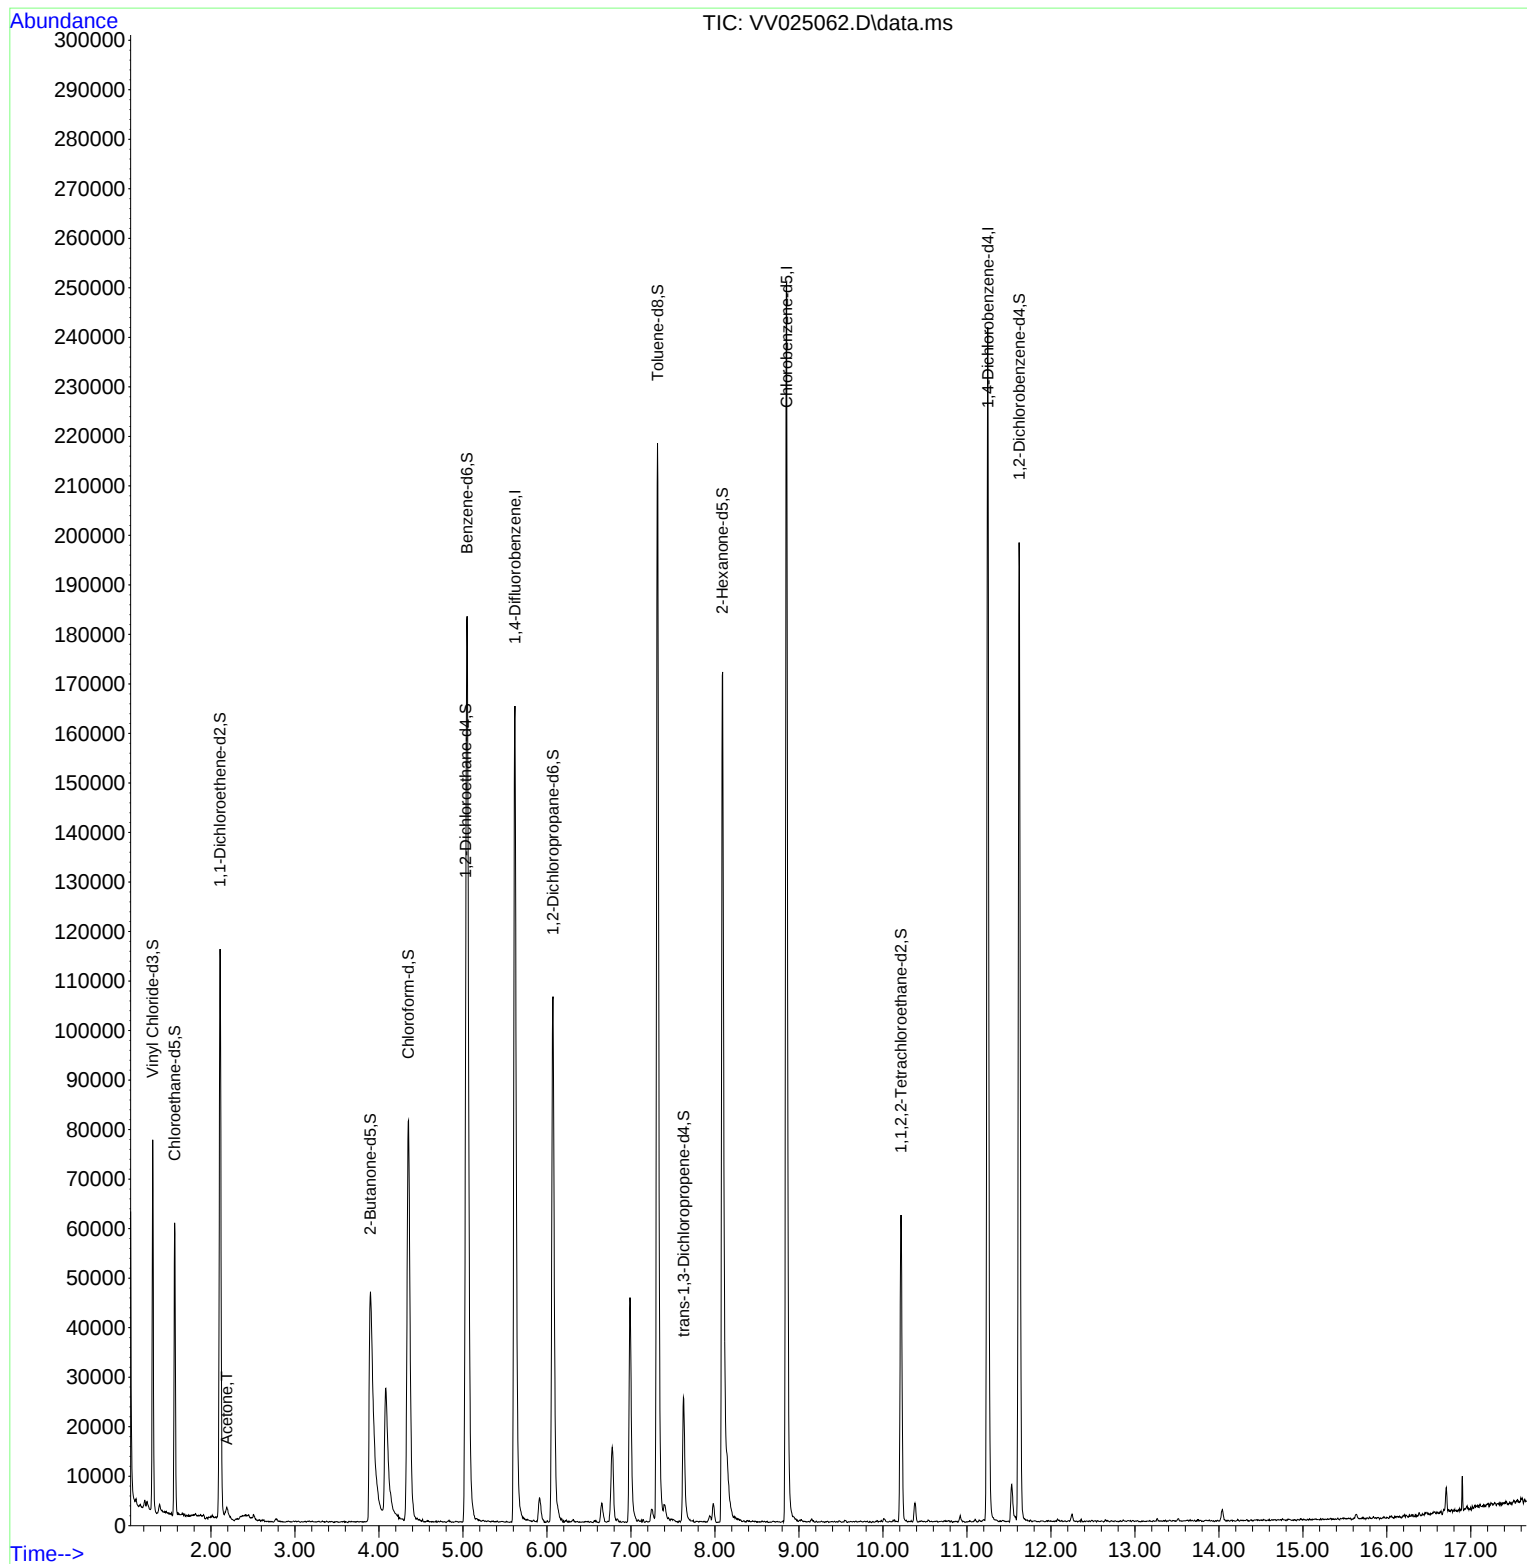

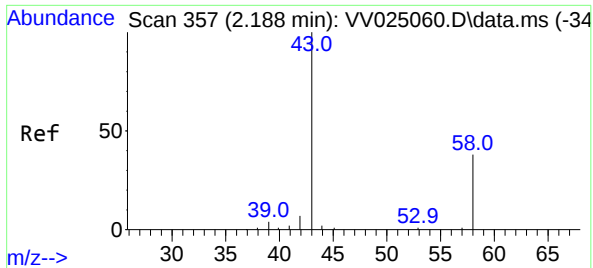

#13
Acetone
Concen: 4.249 ug/L
RT: 2.188 min Scan# 31
Delta R.T. -0.000 min
Lab File: VV025062.D
Acq: 16 Mar 2022 21:41

Instrument :
MSVOA_V
ClientSampleId :
JNLF6

Tgt Ion: 43 Resp: 4065
Ion Ratio Lower Upper
43 100
58 39.8 0.0 54.2

