

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031622\
 Data File : VW025065.D
 Acq On : 16 Mar 2022 22:51
 Operator : SY/MD
 Sample : N1941-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLF9

Quant Time: Mar 17 06:28:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 05:44:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	141385	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	133903	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58452	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	44119	3.953	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.000%
7) Chloroethane-d5	1.568	69	36709	4.491	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.800%
11) 1,1-Dichloroethene-d2	2.108	63	57128	3.167	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.400%
20) 2-Butanone-d5	3.918	46	80108	59.384	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.760%
24) Chloroform-d	4.349	84	87133	4.707	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.200%
26) 1,2-Dichloroethane-d4	5.037	65	38734	5.004	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.000%
32) Benzene-d6	5.053	84	173703	4.472	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%
36) 1,2-Dichloropropane-d6	6.069	67	54419	4.872	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.400%
41) Toluene-d8	7.317	98	149606	4.226	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.600%
43) trans-1,3-Dichloroprop...	7.628	79	15271	3.922	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.400%
46) 2-Hexanone-d5	8.091	63	62355	46.948	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.900%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31950	4.862	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	48496	4.901	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.000%
Target Compounds						
25) Chloroform	4.375	83	2179	0.113	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025065.D
Acq On : 16 Mar 2022 22:51
Operator : SY/MD
Sample : N1941-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF9

Quant Time: Mar 17 06:28:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 05:44:36 2022
Response via : Initial Calibration

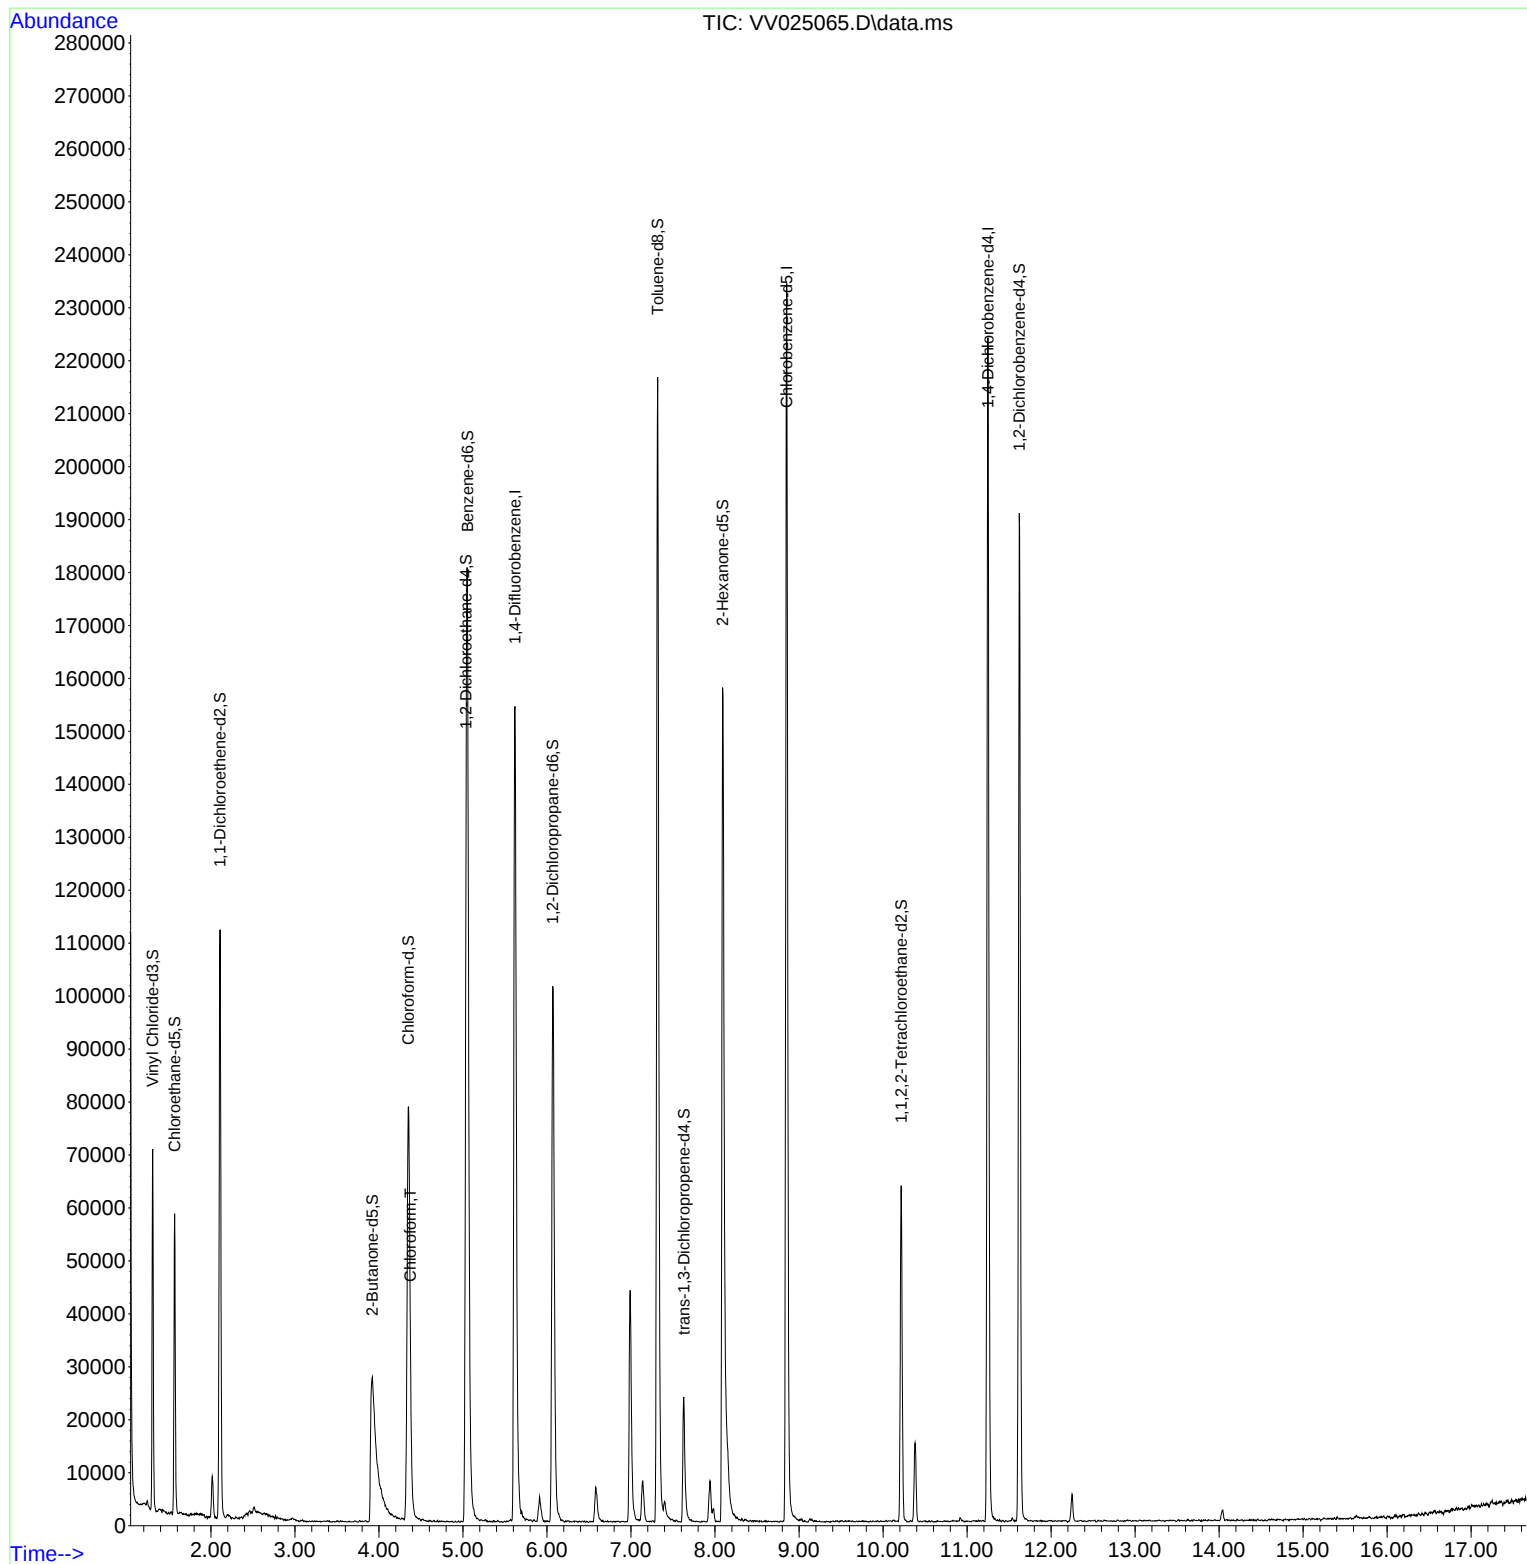

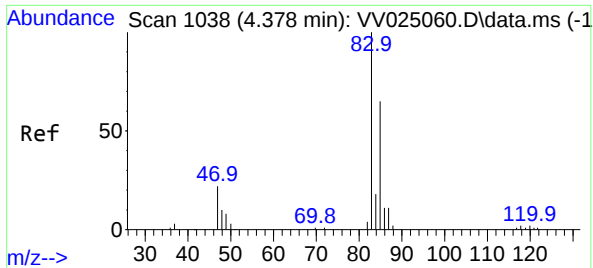

#25
 Chloroform
 Concen: 0.113 ug/L
 RT: 4.375 min Scan# 10
 Delta R.T. -0.003 min
 Lab File: VV025065.D
 Acq: 16 Mar 2022 22:51

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLF9

Tgt Ion: 83 Resp: 2179

Ion	Ratio	Lower	Upper
83	100		
85	62.5	44.5	82.7

