

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031622\
 Data File : VW025066.D
 Acq On : 16 Mar 2022 23:15
 Operator : SY/MD
 Sample : N1941-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLG0

Quant Time: Mar 17 06:28:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 05:44:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	145181	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	140126	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61272	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	43834	3.824	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	76.400%	
7) Chloroethane-d5	1.568	69	35551	4.236	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	84.800%	
11) 1,1-Dichloroethene-d2	2.108	63	56792	3.066	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.400%	
20) 2-Butanone-d5	3.908	46	83801	60.497	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	121.000%	
24) Chloroform-d	4.352	84	86859	4.569	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.400%	
26) 1,2-Dichloroethane-d4	5.034	65	39982	5.031	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.600%	
32) Benzene-d6	5.053	84	174628	4.296	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.000%	
36) 1,2-Dichloropropane-d6	6.072	67	54329	4.648	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.000%	
41) Toluene-d8	7.317	98	146746	3.961	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.200%	
43) trans-1,3-Dichloroprop...	7.625	79	16818	4.127	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.600%	
46) 2-Hexanone-d5	8.092	63	72167	51.922	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.840%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34789	5.059	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	50081	4.828	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.600%	
Target Compounds						Qvalue
3) Chloromethane	1.243	50	1383	0.114	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025066.D
Acq On : 16 Mar 2022 23:15
Operator : SY/MD
Sample : N1941-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLG0

Quant Time: Mar 17 06:28:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 05:44:36 2022
Response via : Initial Calibration

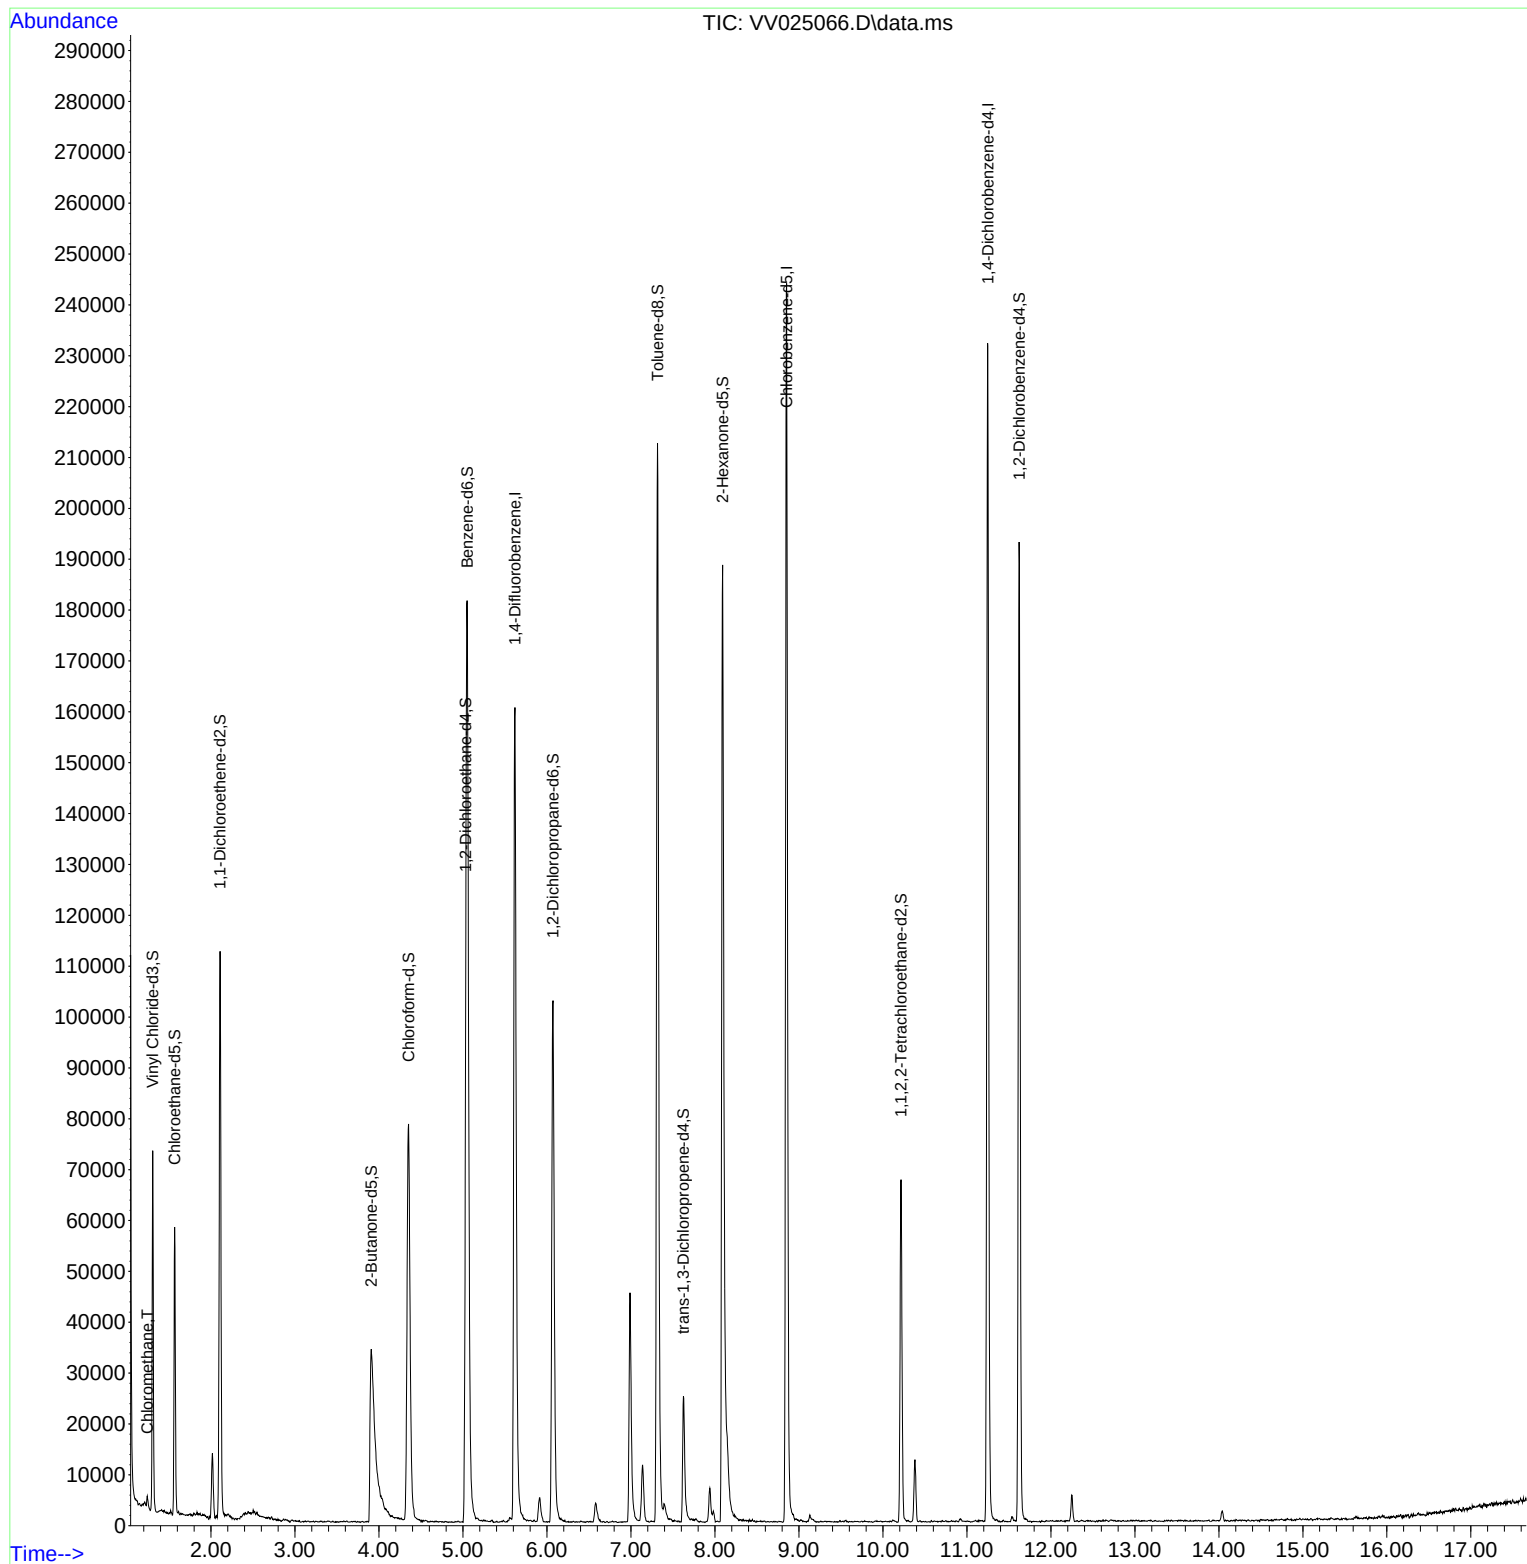

Abundance Scan 63 (1.243 min): VV025060.D\data.ms (-55)

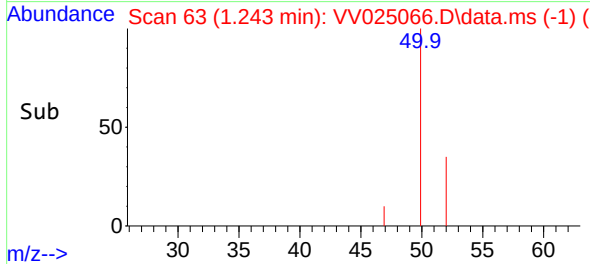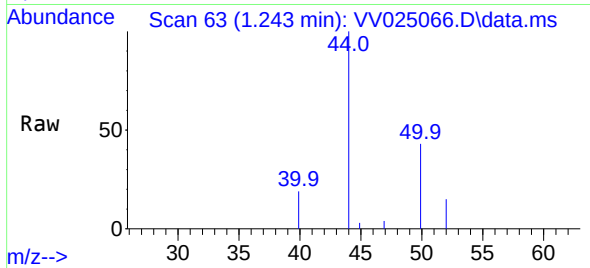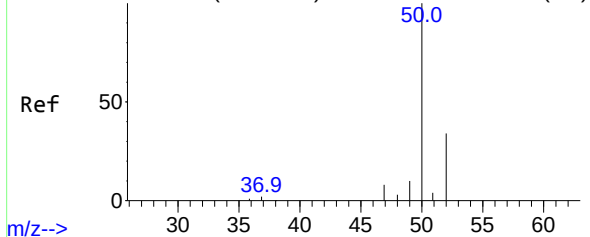

#3
Chloromethane
Concen: 0.114 ug/L
RT: 1.243 min Scan# 61
Delta R.T. 0.000 min
Lab File: VV025066.D
Acq: 16 Mar 2022 23:15

Instrument :
MSVOA_V
ClientSampleId :
JNLG0

Tgt Ion: 50 Resp: 1383
Ion Ratio Lower Upper
50 100
52 35.1 23.2 43.2

