

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025037.D
 Acq On : 16 Mar 2022 11:02
 Operator : SY/MD
 Sample : N1934-04DL 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDD6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	100	rVB	101475	104261	17.19%	1.989%
2	1.568	156	164	177	rBV	81470	89611	14.77%	1.709%
3	2.105	317	331	345	rBV	157587	224137	36.95%	4.275%
4	2.507	447	456	467	rVB2	5435	8667	1.43%	0.165%
5	3.905	880	891	928	rBV	34344	153144	25.25%	2.921%
6	4.343	1011	1027	1056	rBV	106770	271847	44.82%	5.185%
7	4.822	1158	1176	1199	rBV2	124163	298068	49.14%	5.686%
8	5.044	1228	1245	1276	rBV2	243143	606570	100.00%	11.570%
9	5.613	1410	1422	1453	rBV	226557	462421	76.24%	8.821%
10	5.905	1504	1513	1527	rVB3	5583	11328	1.87%	0.216%
11	6.066	1550	1563	1596	rBV	136982	282792	46.62%	5.394%
12	6.982	1838	1848	1873	rBV	64041	118712	19.57%	2.264%
13	7.314	1939	1951	1971	rBV	298127	525377	86.61%	10.022%
14	7.391	1971	1975	1992	rVB4	4154	8564	1.41%	0.163%
15	7.622	2037	2047	2067	rBV	34728	62349	10.28%	1.189%
16	8.088	2182	2192	2228	rBV	207978	435369	71.78%	8.305%
17	8.847	2417	2428	2461	rBV	334259	554198	91.37%	10.571%
18	10.214	2842	2853	2868	rBV	81466	128337	21.16%	2.448%
19	11.246	3163	3174	3199	rBV	318746	493820	81.41%	9.420%
20	11.622	3278	3291	3310	rBV	255762	402918	66.43%	7.686%




Sum of corrected areas: 5242490

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025037.D
Acq On : 16 Mar 2022 11:02
Operator : SY/MD
Sample : N1934-04DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

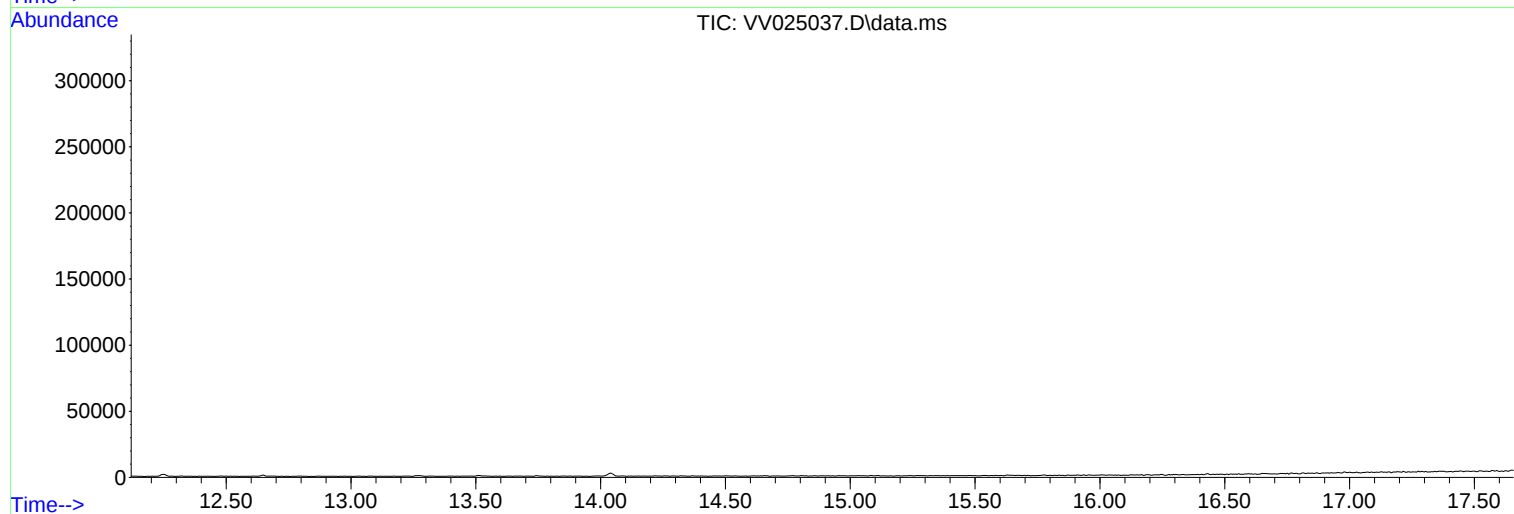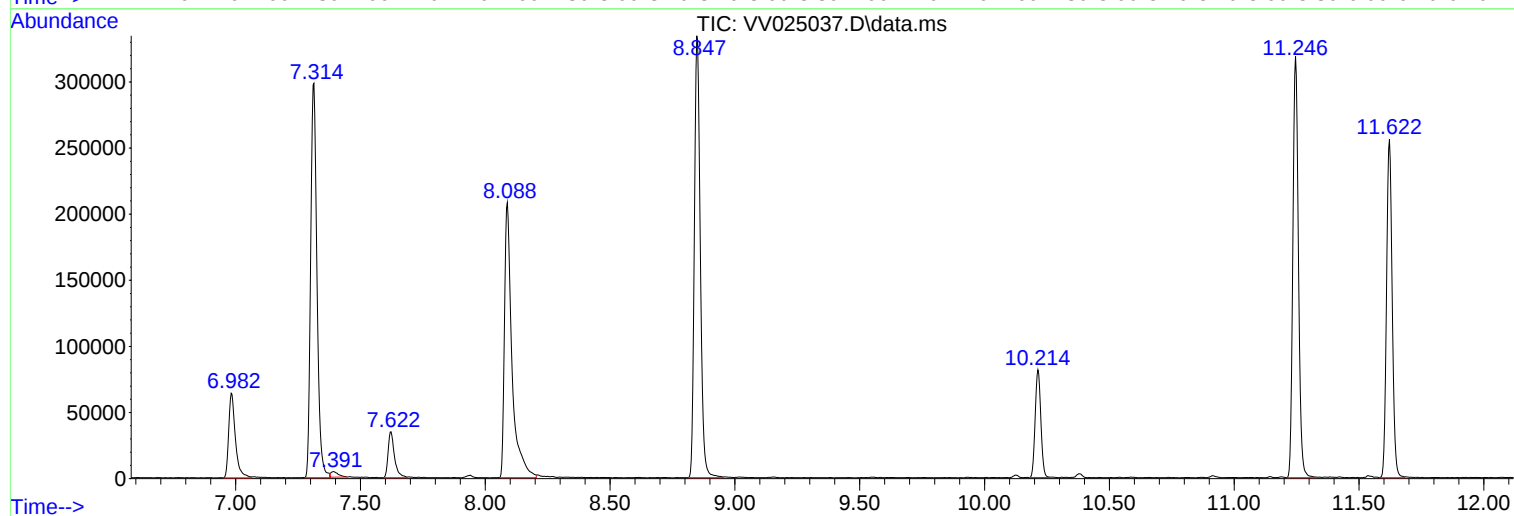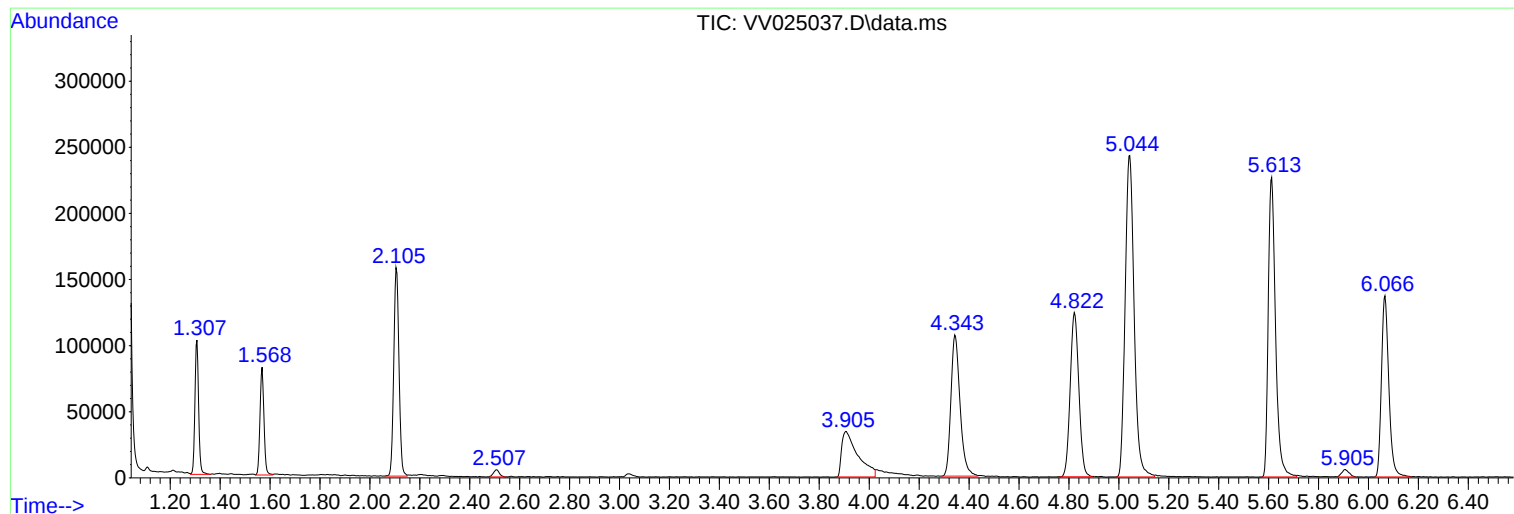

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025037.D
Acq On : 16 Mar 2022 11:02
Operator : SY/MD
Sample : N1934-04DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025037.D
Acq On : 16 Mar 2022 11:02
Operator : SY/MD
Sample : N1934-04DL 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc