

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025039.D
 Acq On : 16 Mar 2022 11:56
 Operator : SY/MD
 Sample : N1934-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	98	rVB	84852	96083	19.60%	2.367%
2	1.568	156	164	175	rBV	64041	73296	14.96%	1.806%
3	2.108	322	332	346	rBV	126093	182307	37.20%	4.491%
4	3.905	881	891	933	rBV2	33148	136049	27.76%	3.352%
5	4.352	1014	1030	1061	rBV4	95531	296266	60.45%	7.299%
6	5.050	1232	1247	1276	rBV2	198736	490106	100.00%	12.075%
7	5.616	1410	1423	1450	rBV	170543	350273	71.47%	8.630%
8	5.911	1505	1515	1533	rVB3	6018	12097	2.47%	0.298%
9	6.069	1548	1564	1582	rBV	110111	226281	46.17%	5.575%
10	6.989	1840	1850	1875	rBV	49355	93190	19.01%	2.296%
11	7.317	1937	1952	1970	rBV	241395	420131	85.72%	10.351%
12	7.625	2039	2048	2075	rBV	26606	48894	9.98%	1.205%
13	7.944	2134	2147	2157	rVB2	6299	11195	2.28%	0.276%
14	8.091	2183	2193	2236	rBV	171061	348609	71.13%	8.589%
15	8.850	2419	2429	2456	rBV	262679	422339	86.17%	10.405%
16	10.214	2843	2853	2868	rBV	63246	98758	20.15%	2.433%
17	10.381	2895	2905	2916	rBV2	11248	16735	3.41%	0.412%
18	11.246	3164	3174	3197	rBV	247184	385009	78.56%	9.485%
19	11.532	3255	3263	3280	rBV4	8296	16790	3.43%	0.414%
20	11.622	3280	3291	3312	rVB	209741	328790	67.09%	8.100%
21	12.249	3477	3486	3496	rVB2	3616	5752	1.17%	0.142%




Sum of corrected areas: 4058950

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025039.D
Acq On : 16 Mar 2022 11:56
Operator : SY/MD
Sample : N1934-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

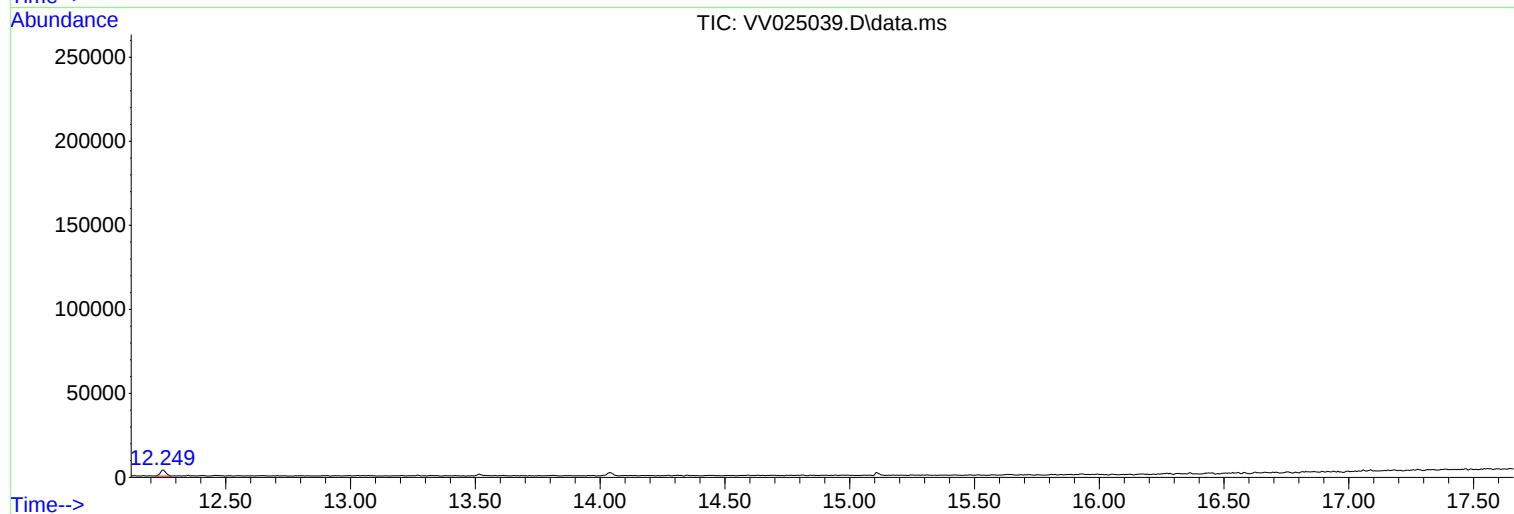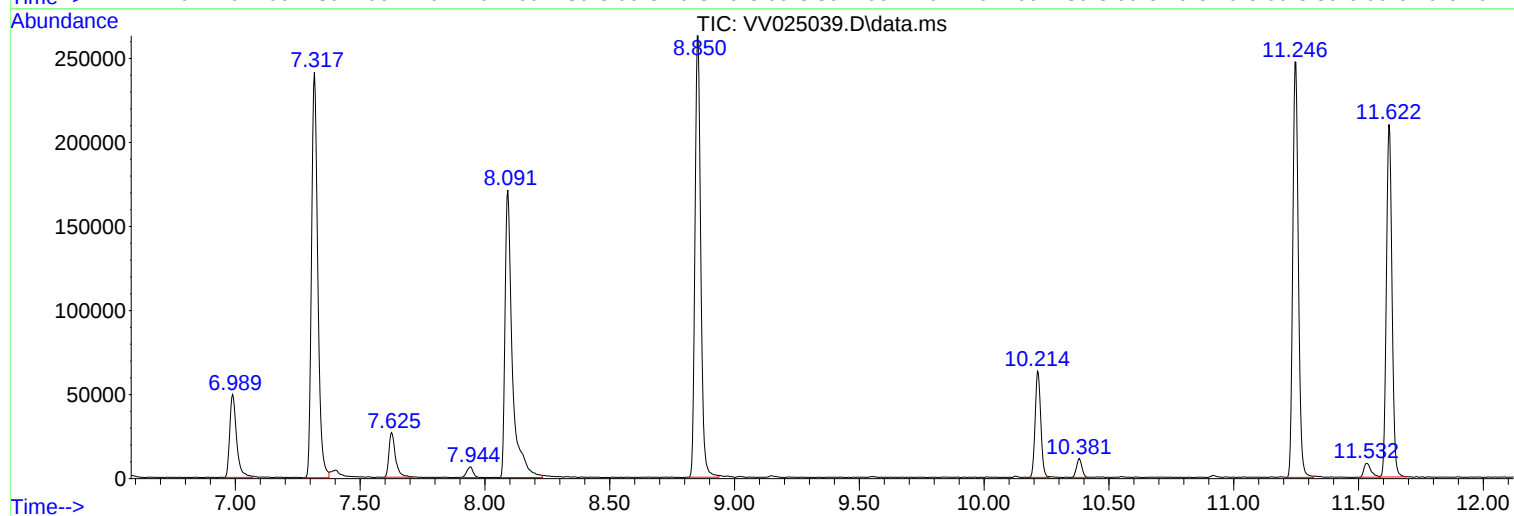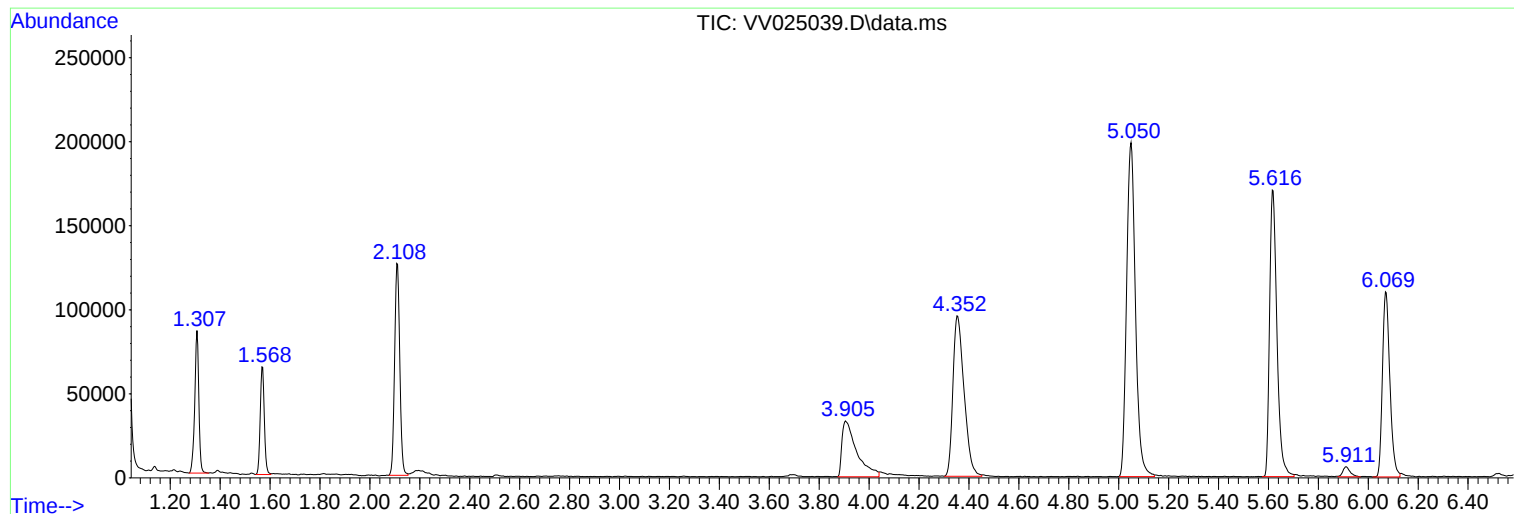

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025039.D
Acq On : 16 Mar 2022 11:56
Operator : SY/MD
Sample : N1934-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025039.D
Acq On : 16 Mar 2022 11:56
Operator : SY/MD
Sample : N1934-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc