

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025041.D
 Acq On : 16 Mar 2022 12:42
 Operator : SY/MD
 Sample : N1934-09DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDD9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	83214	81288	16.63%	1.920%
2	1.568	156	164	178	rBV	64599	72689	14.87%	1.717%
3	2.108	322	332	349	rBV	126523	181538	37.14%	4.288%
4	3.918	883	895	926	rBV2	25940	120620	24.68%	2.849%
5	4.352	1013	1030	1067	rBV2	88643	237636	48.62%	5.614%
6	4.828	1161	1178	1201	rBV2	152787	363386	74.35%	8.584%
7	5.050	1231	1247	1275	rBV2	197445	488730	100.00%	11.545%
8	5.619	1412	1424	1452	rBV	163960	336623	68.88%	7.952%
9	5.911	1502	1515	1532	rVB6	4590	10085	2.06%	0.238%
10	6.069	1552	1564	1592	rBV	106461	224309	45.90%	5.299%
11	6.989	1839	1850	1878	rBV	49970	95609	19.56%	2.259%
12	7.317	1941	1952	1972	rBV	235953	412876	84.48%	9.753%
13	7.625	2039	2048	2068	rBV2	27562	48992	10.02%	1.157%
14	7.937	2135	2145	2157	rBV3	2852	4939	1.01%	0.117%
15	8.091	2182	2193	2233	rBV	163537	353018	72.23%	8.339%
16	8.850	2419	2429	2460	rBV	249011	408119	83.51%	9.641%
17	10.217	2842	2854	2868	rBV2	66308	104346	21.35%	2.465%
18	10.381	2894	2905	2915	rBV4	4036	6218	1.27%	0.147%
19	11.246	3164	3174	3197	rBV	232523	362547	74.18%	8.564%
20	11.622	3280	3291	3312	rBV	204108	319689	65.41%	7.552%




Sum of corrected areas: 4233257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025041.D
Acq On : 16 Mar 2022 12:42
Operator : SY/MD
Sample : N1934-09DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

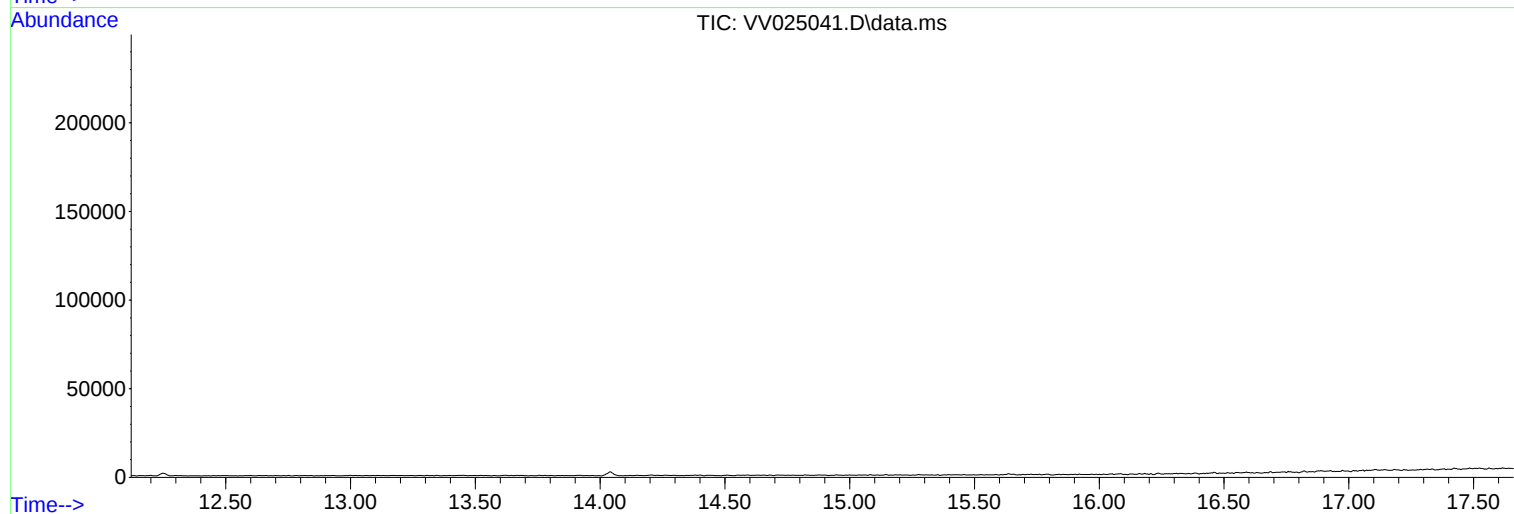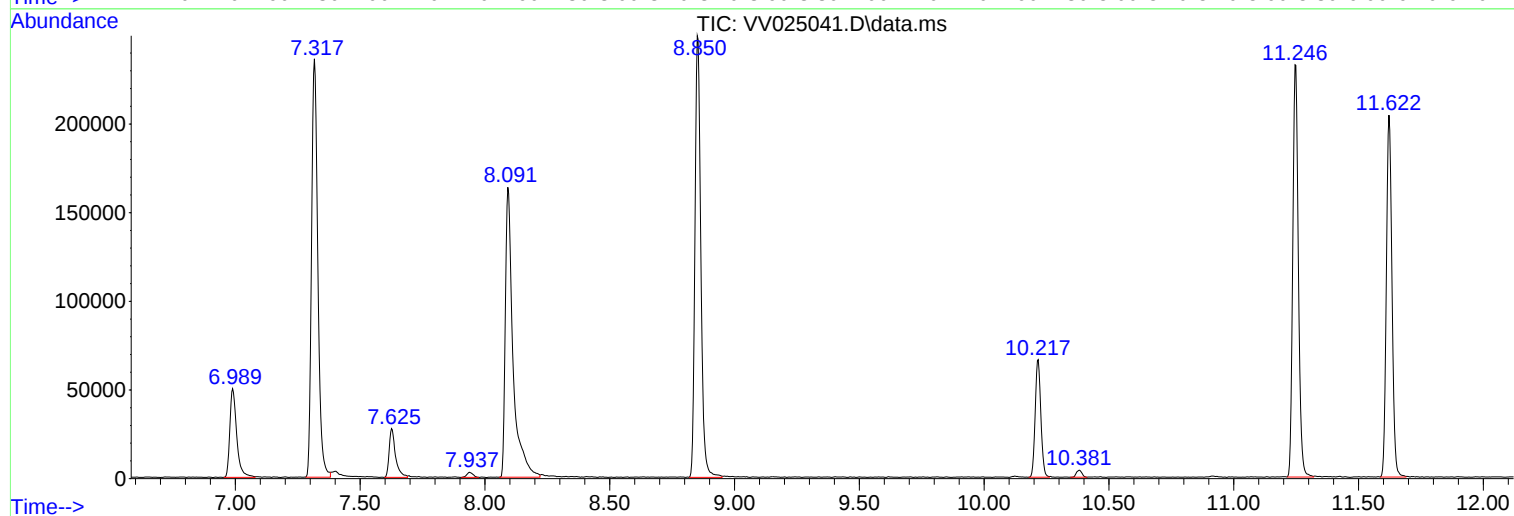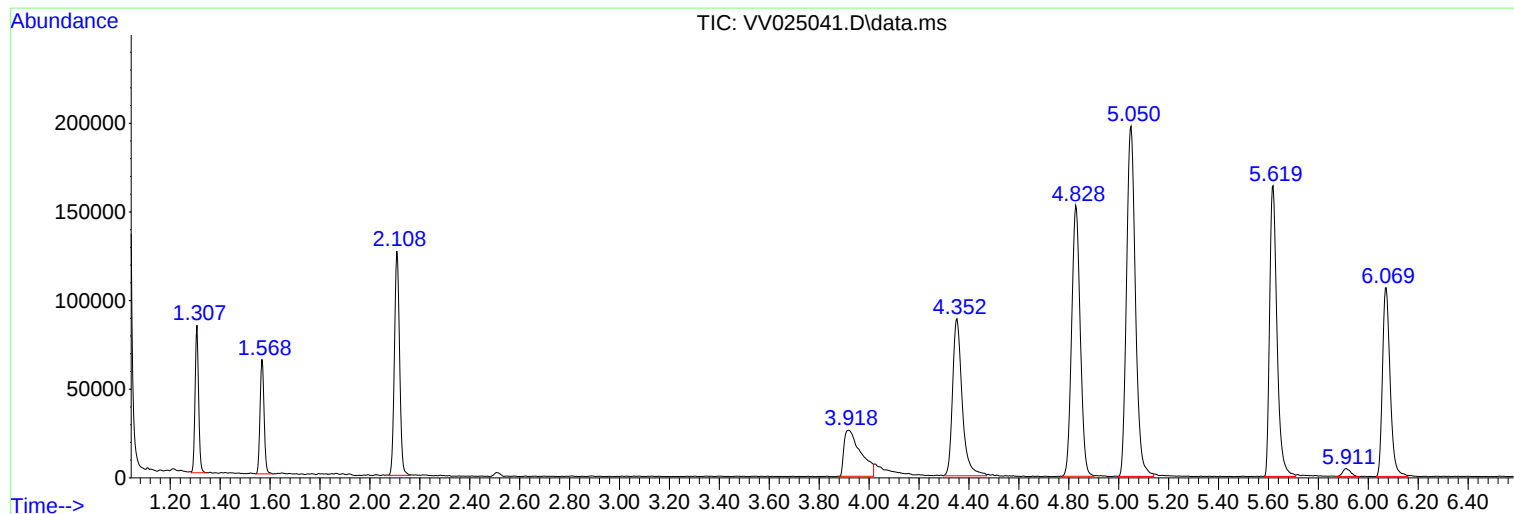

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025041.D
Acq On : 16 Mar 2022 12:42
Operator : SY/MD
Sample : N1934-09DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025041.D
Acq On : 16 Mar 2022 12:42
Operator : SY/MD
Sample : N1934-09DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc