

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025042.D
 Acq On : 16 Mar 2022 13:06
 Operator : SY/MD
 Sample : N1933-05DL 4X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDB6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	75594	79066	16.30%	1.920%
2	1.568	156	164	178	rVB	59505	69844	14.40%	1.696%
3	2.101	318	330	342	rBV	125196	178649	36.84%	4.339%
4	2.506	446	456	466	rVB	9256	14846	3.06%	0.361%
5	3.905	881	891	925	rBV2	34076	137373	28.33%	3.336%
6	4.349	1013	1029	1063	rBV	81875	208158	42.93%	5.055%
7	4.825	1158	1177	1198	rBV	96755	230005	47.43%	5.586%
8	5.046	1231	1246	1279	rBV2	198786	484928	100.00%	11.777%
9	5.616	1411	1423	1452	rBV	167851	341442	70.41%	8.292%
10	5.908	1506	1514	1529	rVB7	4375	9264	1.91%	0.225%
11	6.069	1552	1564	1592	rBV	106240	218099	44.98%	5.297%
12	6.989	1839	1850	1876	rBV	49675	92248	19.02%	2.240%
13	7.316	1939	1952	1972	rBV	233198	414339	85.44%	10.063%
14	7.625	2039	2048	2068	rBV2	26374	47818	9.86%	1.161%
15	8.095	2183	2194	2239	rBV	156577	362404	74.73%	8.801%
16	8.850	2418	2429	2454	rBV	246006	406771	83.88%	9.879%
17	10.217	2843	2854	2875	rVB	66637	107181	22.10%	2.603%
18	11.249	3164	3175	3199	rBV	248173	380230	78.41%	9.234%
19	11.622	3280	3291	3308	rBV	208763	328600	67.76%	7.980%
20	14.040	4032	4043	4052	rBV	4270	6292	1.30%	0.153%




Sum of corrected areas: 4117557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025042.D
Acq On : 16 Mar 2022 13:06
Operator : SY/MD
Sample : N1933-05DL 4X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

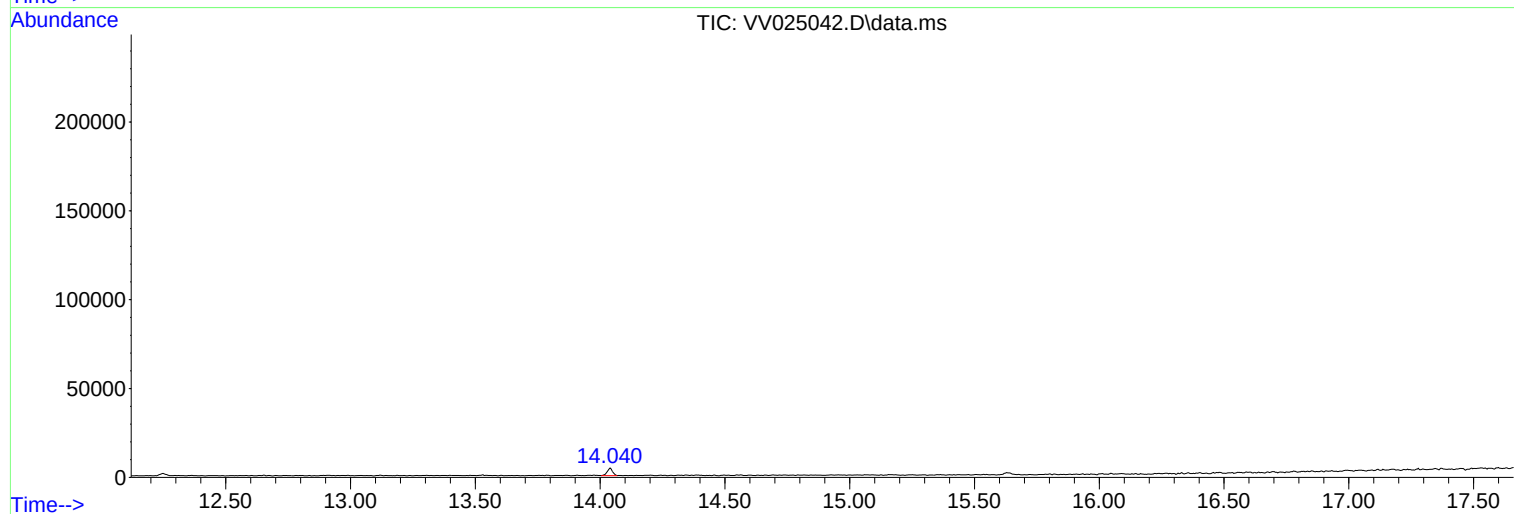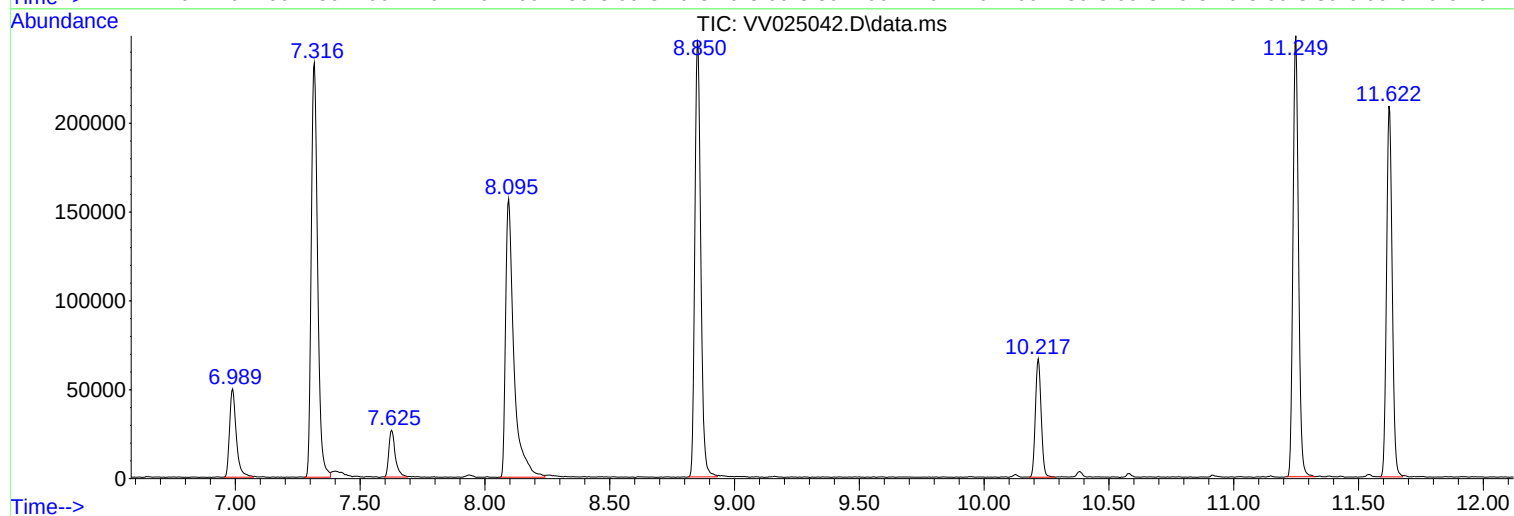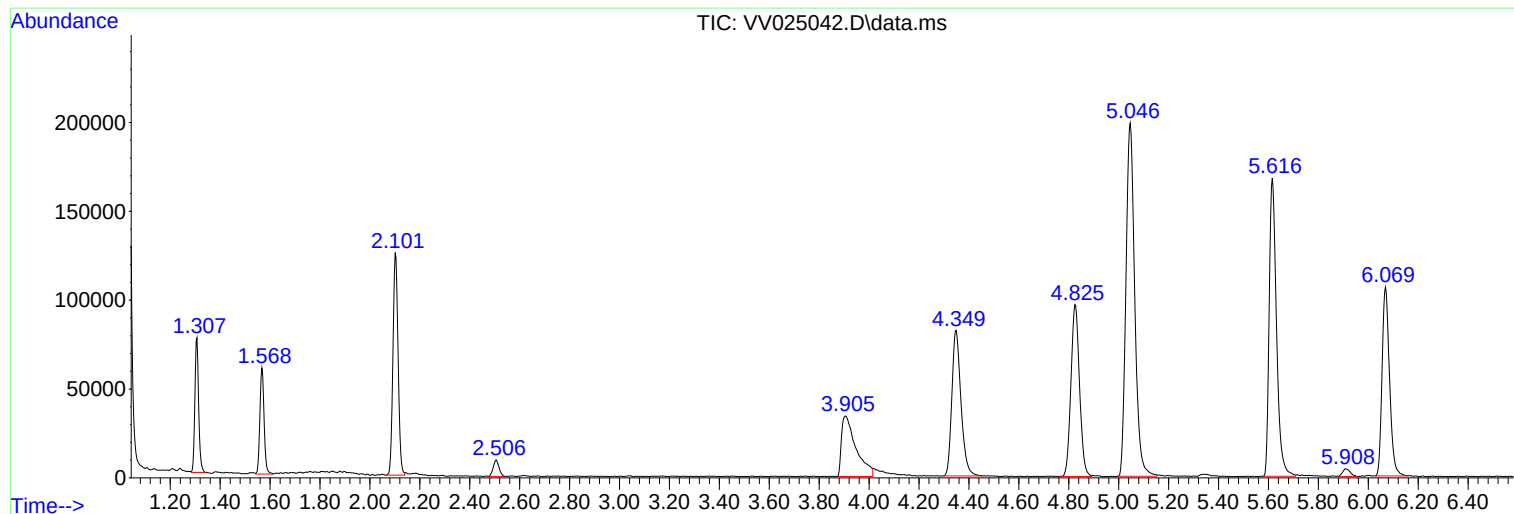

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025042.D
Acq On : 16 Mar 2022 13:06
Operator : SY/MD
Sample : N1933-05DL 4X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025042.D
Acq On : 16 Mar 2022 13:06
Operator : SY/MD
Sample : N1933-05DL 4X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc