

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025044.D
 Acq On : 16 Mar 2022 13:52
 Operator : SY/MD
 Sample : N1933-15DL 50X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDC6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	85982	83953	16.71%	1.969%
2	1.568	156	164	181	rBV	64698	74174	14.77%	1.740%
3	2.111	322	333	347	rBV	127169	182387	36.31%	4.278%
4	3.912	883	893	942	rBV2	26851	136522	27.18%	3.202%
5	4.352	1012	1030	1069	rBV2	88260	234892	46.76%	5.509%
6	4.831	1162	1179	1204	rBV	121352	291934	58.11%	6.847%
7	5.050	1231	1247	1280	rBV2	200656	502344	100.00%	11.782%
8	5.619	1408	1424	1456	rBV	169289	349173	69.51%	8.189%
9	5.915	1505	1516	1527	rBV4	4781	8763	1.74%	0.206%
10	6.069	1552	1564	1593	rBV	109306	227733	45.33%	5.341%
11	6.989	1840	1850	1879	rBV	49644	94359	18.78%	2.213%
12	7.317	1940	1952	1971	rBV	241661	422473	84.10%	9.908%
13	7.625	2039	2048	2068	rBV	27334	49218	9.80%	1.154%
14	7.944	2135	2147	2155	rBV2	3104	5556	1.11%	0.130%
15	8.092	2183	2193	2236	rBV	166518	361945	72.05%	8.489%
16	8.850	2418	2429	2456	rBV	255834	419157	83.44%	9.831%
17	10.217	2842	2854	2874	rBV	67421	106672	21.23%	2.502%
18	10.381	2894	2905	2914	rVB3	4295	6282	1.25%	0.147%
19	11.249	3164	3175	3198	rBV	244579	377414	75.13%	8.852%
20	11.622	3280	3291	3317	rBV	206740	328798	65.45%	7.711%




Sum of corrected areas: 4263749

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025044.D
Acq On : 16 Mar 2022 13:52
Operator : SY/MD
Sample : N1933-15DL 50X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

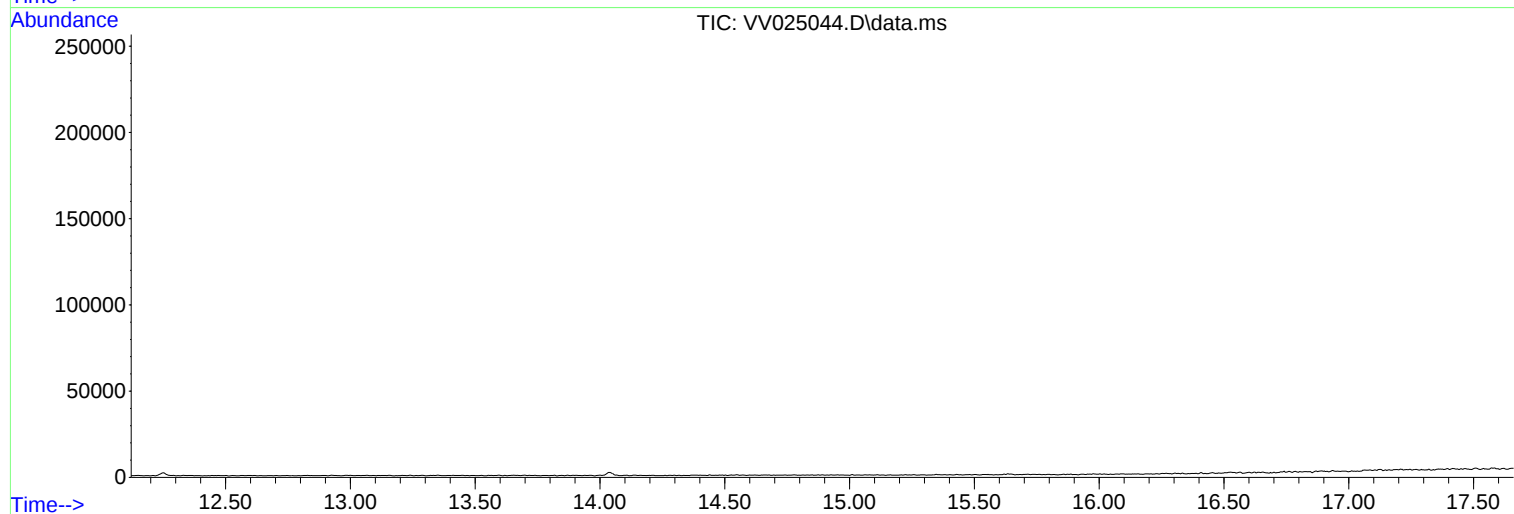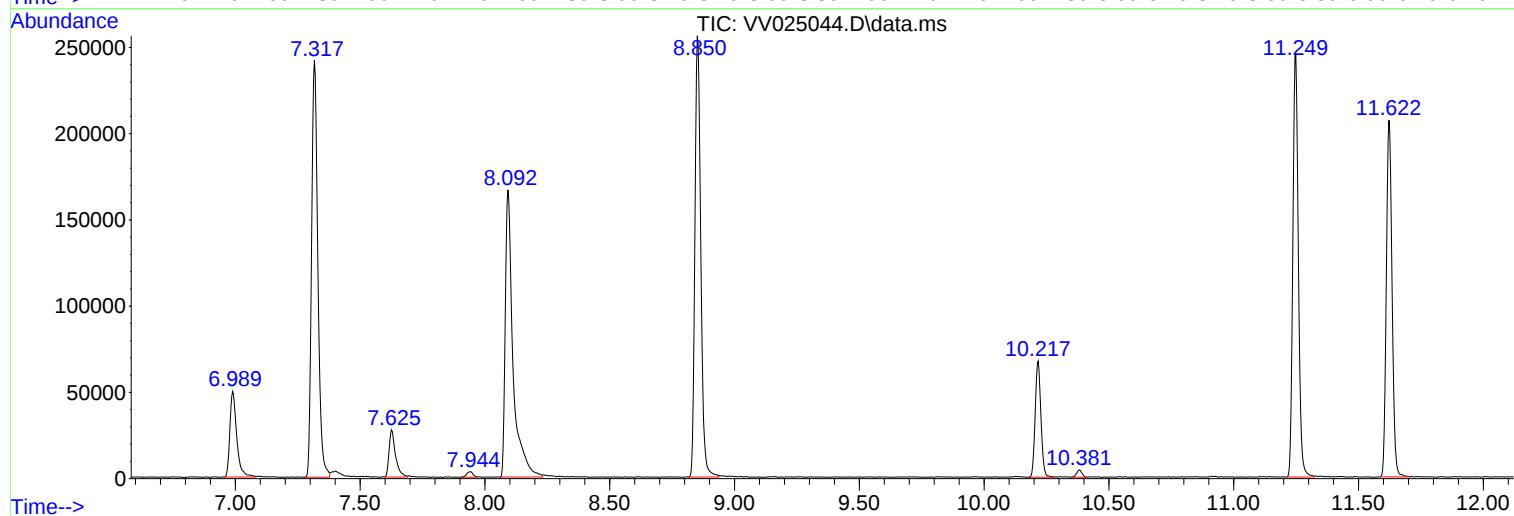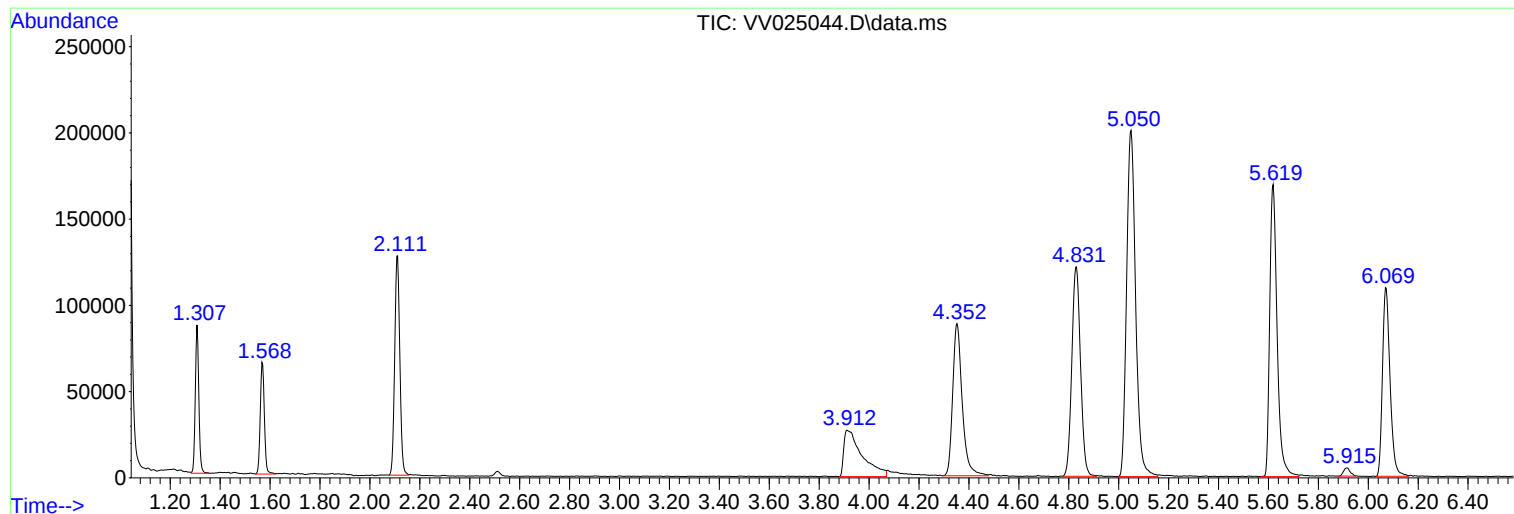

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025044.D
Acq On : 16 Mar 2022 13:52
Operator : SY/MD
Sample : N1933-15DL 50X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025044.D
Acq On : 16 Mar 2022 13:52
Operator : SY/MD
Sample : N1933-15DL 50X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------