

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025045.D
 Acq On : 16 Mar 2022 14:16
 Operator : SY/MD
 Sample : N1933-16DL 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDC7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	80825	82340	16.72%	1.922%
2	1.571	157	165	175	rBV	66385	72619	14.75%	1.695%
3	2.111	322	333	350	rBV	125972	181430	36.84%	4.235%
4	2.513	447	458	470	rVB3	4776	8153	1.66%	0.190%
5	3.909	881	892	940	rBV2	33774	143126	29.06%	3.341%
6	4.352	1014	1030	1058	rBV2	86833	220020	44.68%	5.136%
7	4.831	1161	1179	1202	rBV	143260	344071	69.87%	8.031%
8	5.050	1230	1247	1273	rBV2	198277	492468	100.00%	11.495%
9	5.619	1412	1424	1448	rBV	169623	342773	69.60%	8.001%
10	5.915	1506	1516	1531	rBV4	4318	9232	1.87%	0.215%
11	6.072	1552	1565	1593	rBV	112755	230967	46.90%	5.391%
12	6.989	1840	1850	1879	rBV	50305	93285	18.94%	2.177%
13	7.317	1941	1952	1972	rBV	242028	419377	85.16%	9.789%
14	7.625	2039	2048	2075	rBV2	28078	50669	10.29%	1.183%
15	8.092	2179	2193	2231	rBV	171701	360744	73.25%	8.420%
16	8.850	2419	2429	2455	rBV	250034	416527	84.58%	9.722%
17	10.217	2838	2854	2876	rVB	67382	108518	22.04%	2.533%
18	11.249	3163	3175	3199	rBV	244039	376425	76.44%	8.786%
19	11.622	3277	3291	3315	rBV	212043	331420	67.30%	7.736%




Sum of corrected areas: 4284164

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025045.D
Acq On : 16 Mar 2022 14:16
Operator : SY/MD
Sample : N1933-16DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

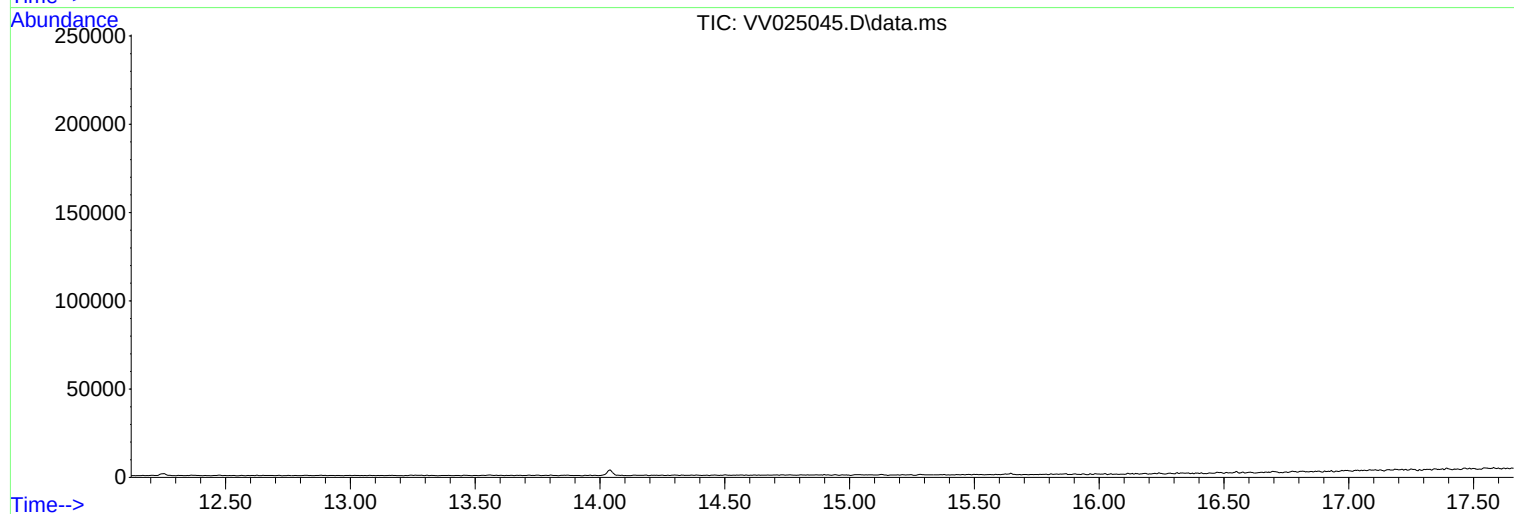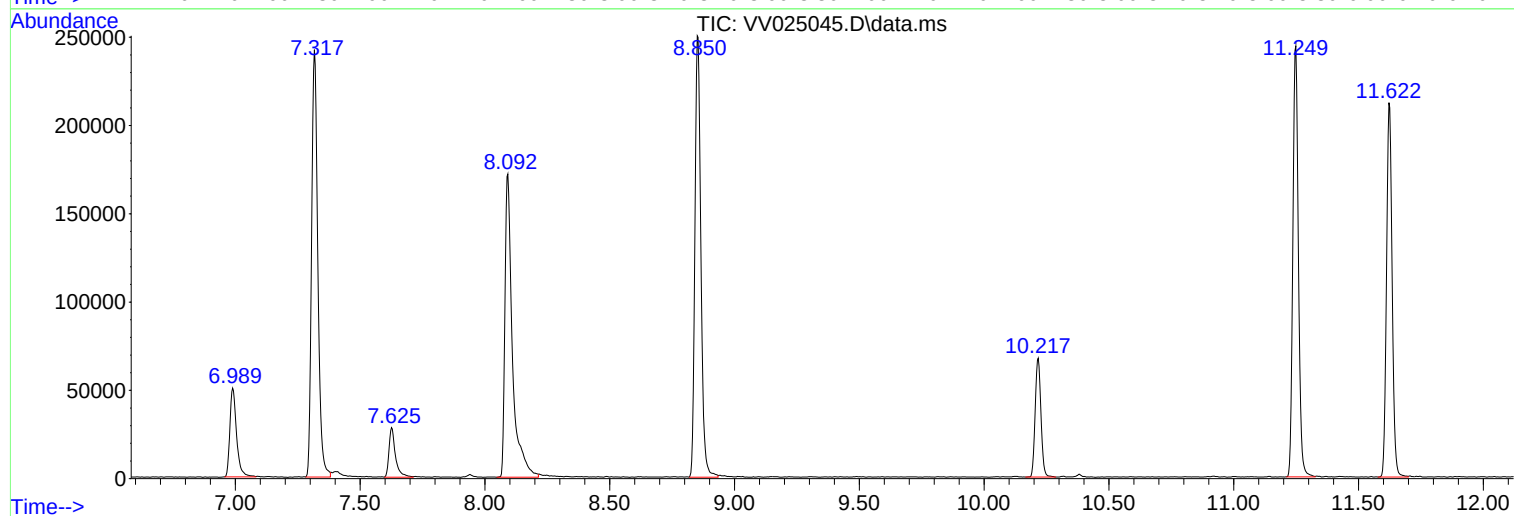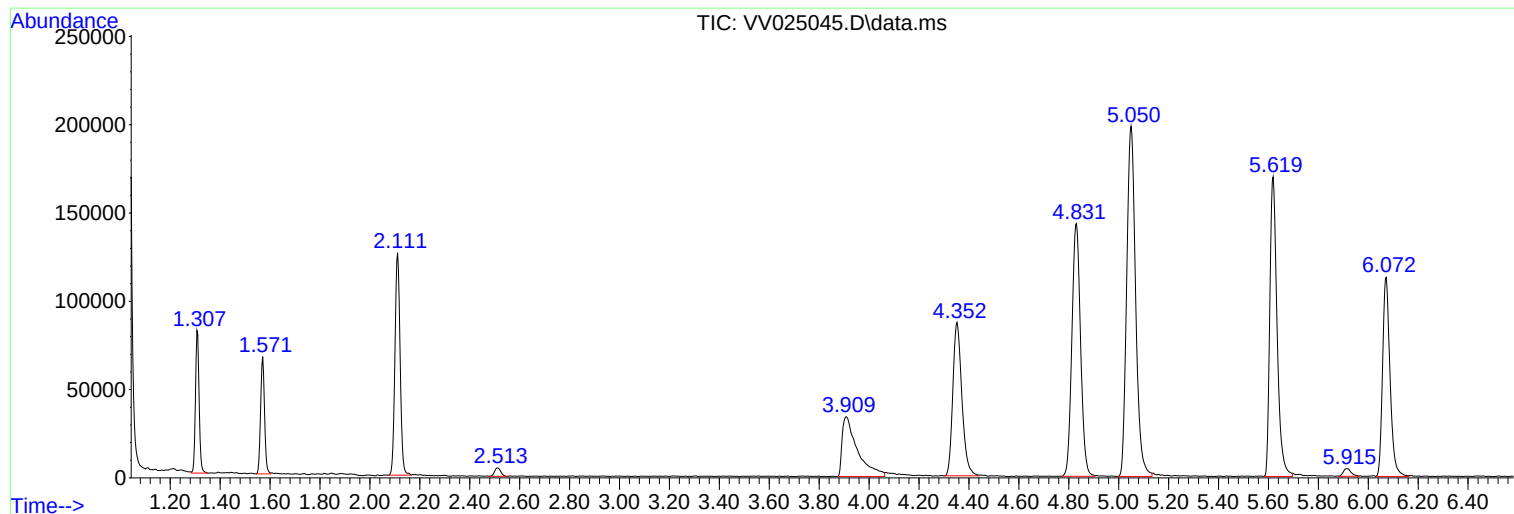

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025045.D
Acq On : 16 Mar 2022 14:16
Operator : SY/MD
Sample : N1933-16DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025045.D
Acq On : 16 Mar 2022 14:16
Operator : SY/MD
Sample : N1933-16DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------