

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025056.D
Acq On : 16 Mar 2022 18:34
Operator : SY/MD
Sample : N1941-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.050	1231	1247	1270	rBV2	188436	470195	1.20%	1.166%
2	7.317	1941	1952	1973	rBV	229099	398629	1.02%	0.989%
3	7.982	2137	2159	2183	rBV	22807279	39045332	100.00%	96.854%
4	8.854	2418	2430	2458	rBV	242445	399588	1.02%	0.991%




Sum of corrected areas: 40313744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025056.D
Acq On : 16 Mar 2022 18:34
Operator : SY/MD
Sample : N1941-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

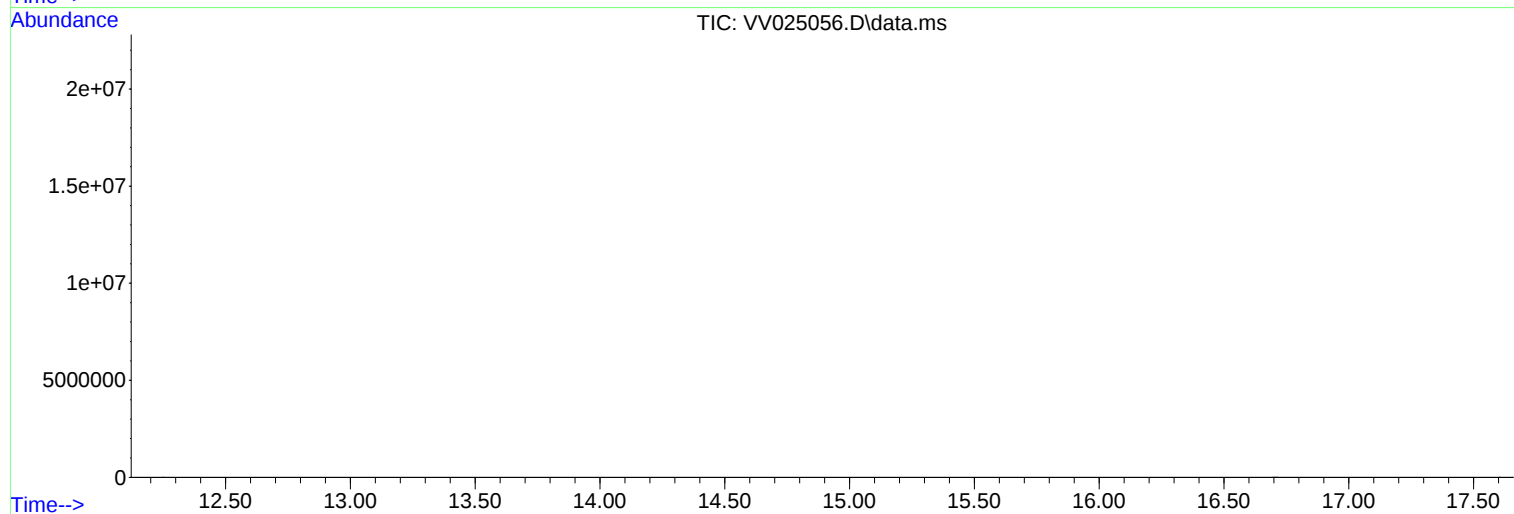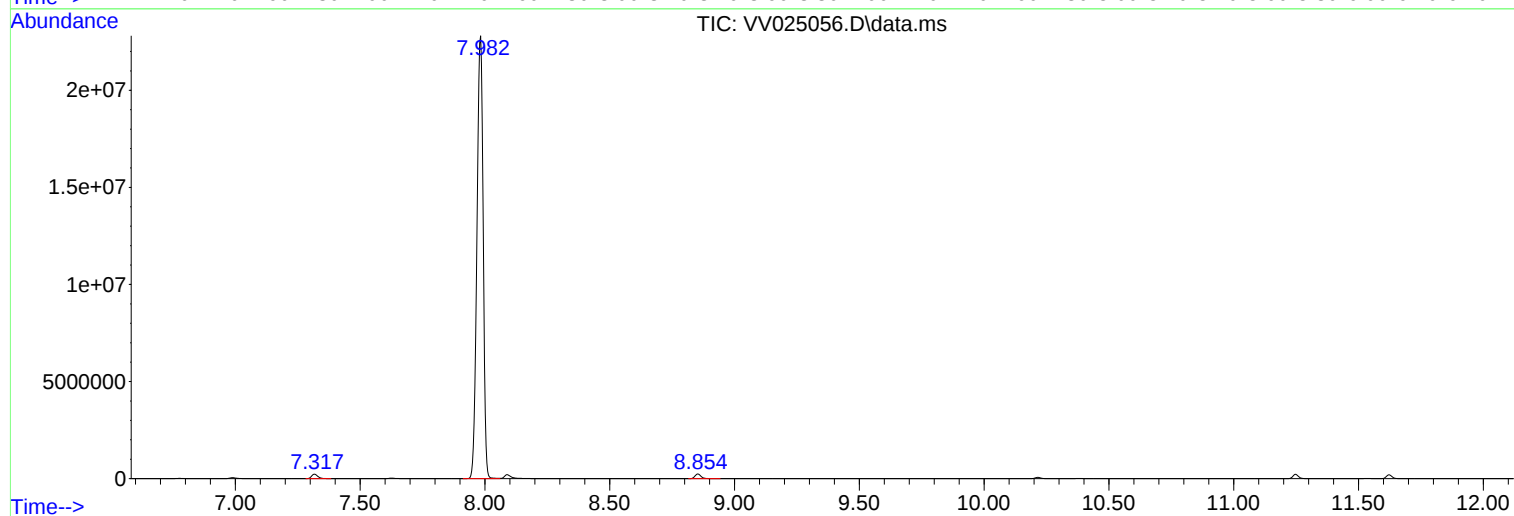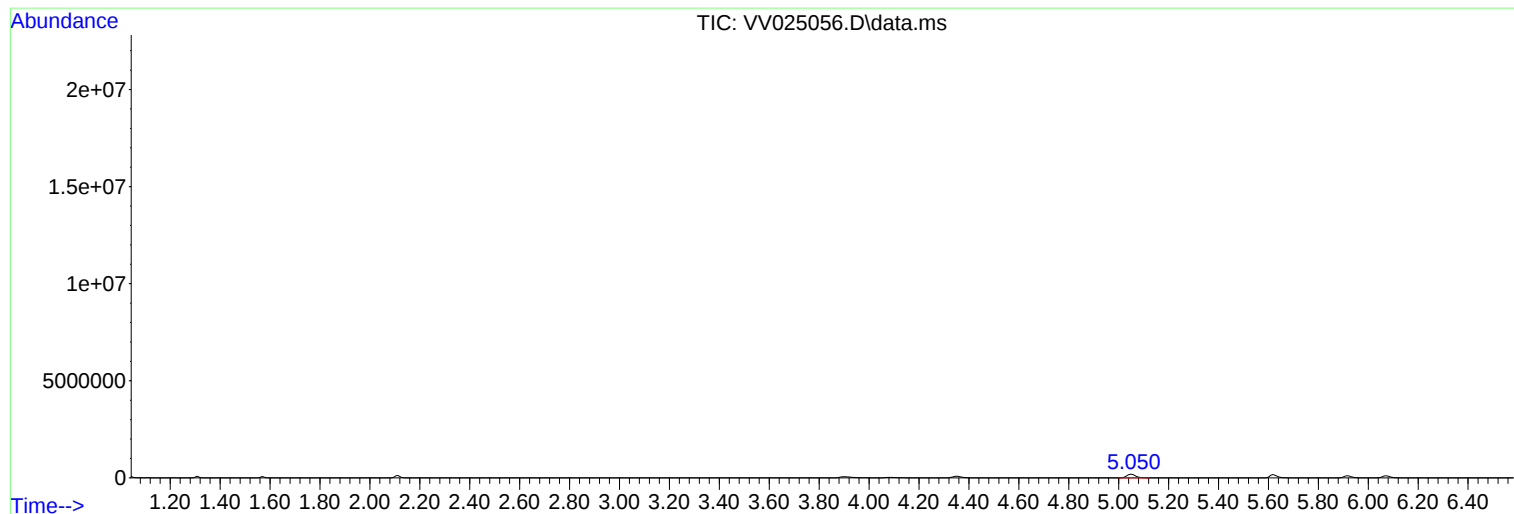

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025056.D
Acq On : 16 Mar 2022 18:34
Operator : SY/MD
Sample : N1941-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025056.D
Acq On : 16 Mar 2022 18:34
Operator : SY/MD
Sample : N1941-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
