

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025061.D
 Acq On : 16 Mar 2022 21:17
 Operator : SY/MD
 Sample : VV0316WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK317

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	71803	70282	15.53%	1.917%
2	1.568	156	164	175	rBV	58517	64819	14.33%	1.768%
3	2.108	321	332	348	rBV	113625	161589	35.72%	4.407%
4	2.510	448	457	467	rVB	5451	8442	1.87%	0.230%
5	3.915	884	894	931	rBV2	26550	117002	25.86%	3.191%
6	4.352	1013	1030	1056	rBV	77833	198120	43.79%	5.403%
7	5.050	1231	1247	1278	rBV2	183908	452435	100.00%	12.339%
8	5.619	1412	1424	1451	rBV	165195	334970	74.04%	9.135%
9	5.912	1505	1515	1530	rVB2	4695	9322	2.06%	0.254%
10	6.072	1552	1565	1593	rBV	100879	210669	46.56%	5.745%
11	6.989	1840	1850	1870	rBV	43759	81258	17.96%	2.216%
12	7.317	1941	1952	1973	rBV	216601	380275	84.05%	10.371%
13	7.625	2038	2048	2064	rBV2	24155	43262	9.56%	1.180%
14	7.979	2151	2158	2168	rVB5	3887	6624	1.46%	0.181%
15	8.092	2184	2193	2225	rBV	158892	340291	75.21%	9.280%
16	8.854	2415	2430	2466	rBV	246902	408022	90.18%	11.127%
17	10.217	2840	2854	2870	rBV	63096	100858	22.29%	2.751%
18	11.249	3164	3175	3198	rBV	239012	369945	81.77%	10.089%
19	11.622	3278	3291	3311	rBV	192702	303619	67.11%	8.280%
20	14.040	4033	4043	4053	rVB	2962	5000	1.11%	0.136%




Sum of corrected areas: 3666804

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025061.D
Acq On : 16 Mar 2022 21:17
Operator : SY/MD
Sample : VV0316WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

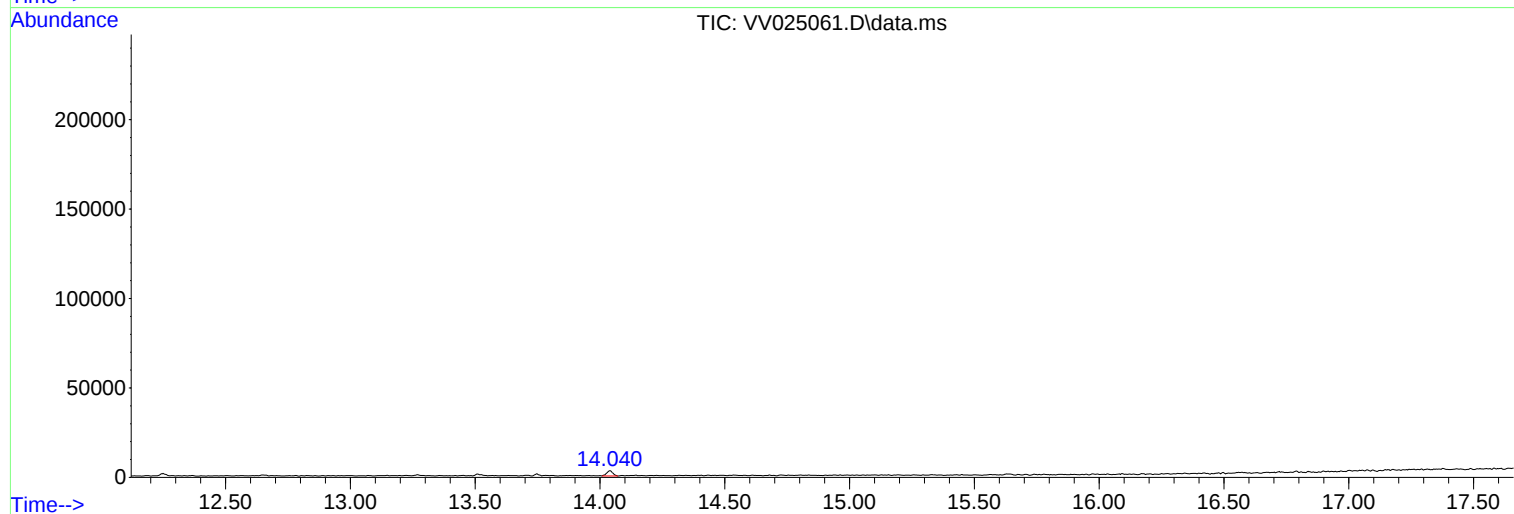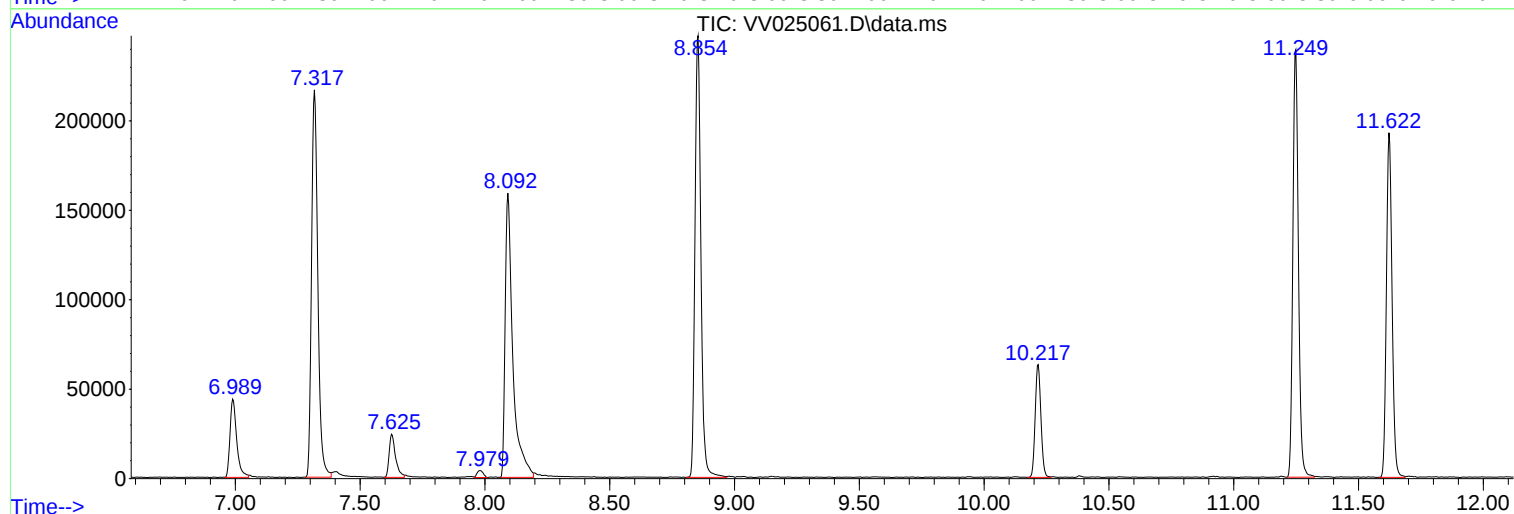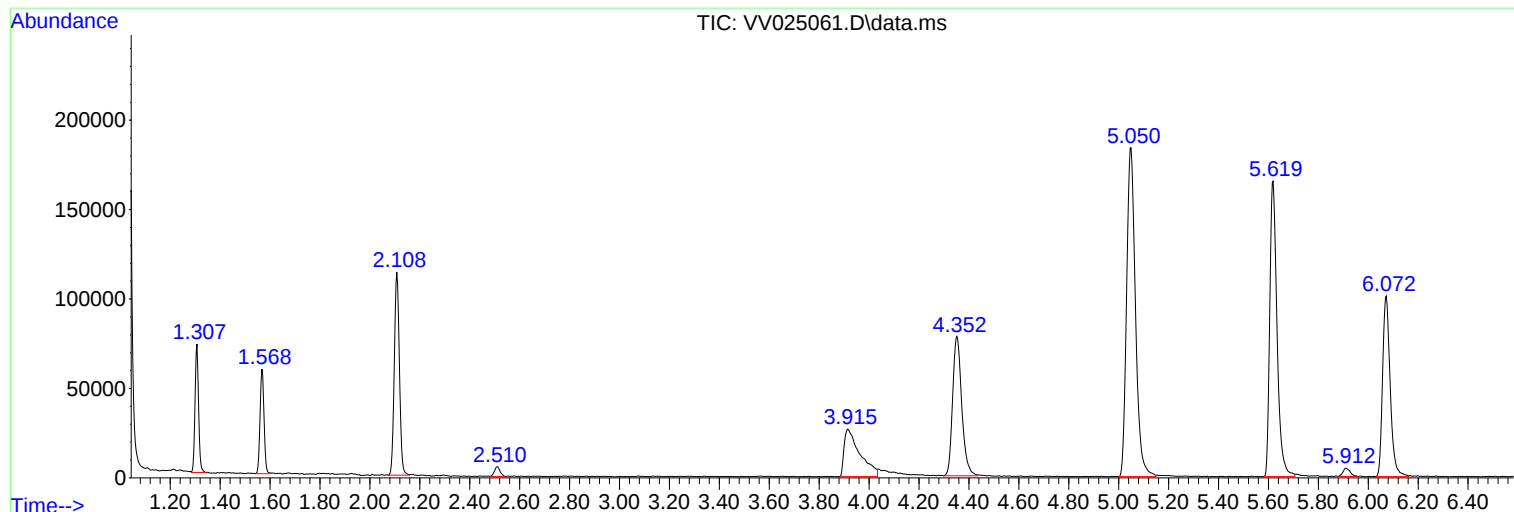

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025061.D
Acq On : 16 Mar 2022 21:17
Operator : SY/MD
Sample : VV0316WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025061.D
Acq On : 16 Mar 2022 21:17
Operator : SY/MD
Sample : VV0316WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK317

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc