

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025063.D
 Acq On : 16 Mar 2022 22:05
 Operator : SY/MD
 Sample : N1941-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLF7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	93	rBV	68343	68889	15.92%	1.920%
2	1.568	156	164	176	rVB	56204	62014	14.33%	1.728%
3	2.108	322	332	348	rBV	109218	154362	35.67%	4.301%
4	3.902	877	890	923	rBV3	41086	157394	36.37%	4.386%
5	4.349	1013	1029	1054	rBV	75682	190517	44.02%	5.309%
6	5.047	1230	1246	1278	rBV2	174922	432809	100.00%	12.060%
7	5.616	1411	1423	1458	rBV	157682	324877	75.06%	9.053%
8	5.911	1507	1515	1530	rVB5	4329	8753	2.02%	0.244%
9	6.069	1552	1564	1595	rBV	99407	211295	48.82%	5.888%
10	6.989	1836	1850	1871	rBV2	43158	80052	18.50%	2.231%
11	7.317	1939	1952	1970	rBV	206353	361927	83.62%	10.085%
12	7.625	2039	2048	2071	rBV	23345	41670	9.63%	1.161%
13	7.940	2135	2146	2153	rBV2	7099	12392	2.86%	0.345%
14	7.982	2153	2159	2169	rVB5	3136	4980	1.15%	0.139%
15	8.091	2182	2193	2228	rBV	157084	321907	74.38%	8.970%
16	8.853	2418	2430	2447	rBV	240999	391209	90.39%	10.901%
17	10.217	2843	2854	2867	rBV	60899	93462	21.59%	2.604%
18	10.381	2893	2905	2916	rBV2	12587	19593	4.53%	0.546%
19	11.249	3164	3175	3195	rBV	227337	347721	80.34%	9.689%
20	11.535	3256	3264	3274	rBV3	3954	6250	1.44%	0.174%
21	11.622	3280	3291	3311	rVB	182408	285274	65.91%	7.949%
22	12.249	3475	3486	3499	rVB2	4613	6885	1.59%	0.192%
23	14.040	4034	4043	4056	rVB	2956	4482	1.04%	0.125%




Sum of corrected areas: 3588714

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025063.D
Acq On : 16 Mar 2022 22:05
Operator : SY/MD
Sample : N1941-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

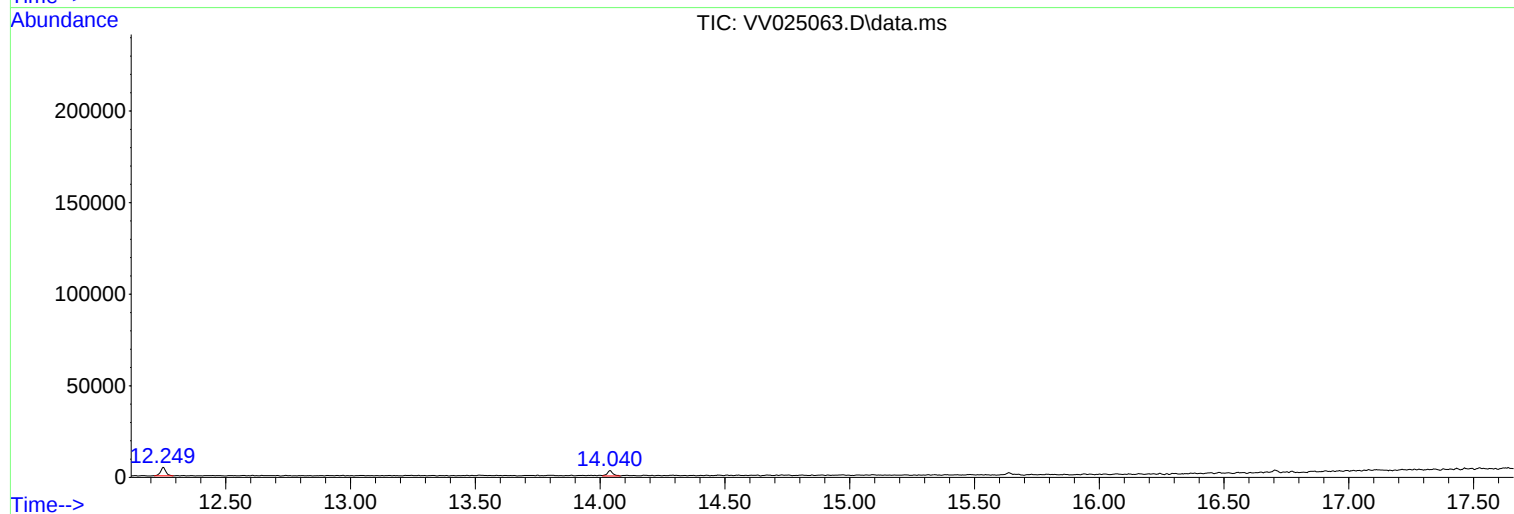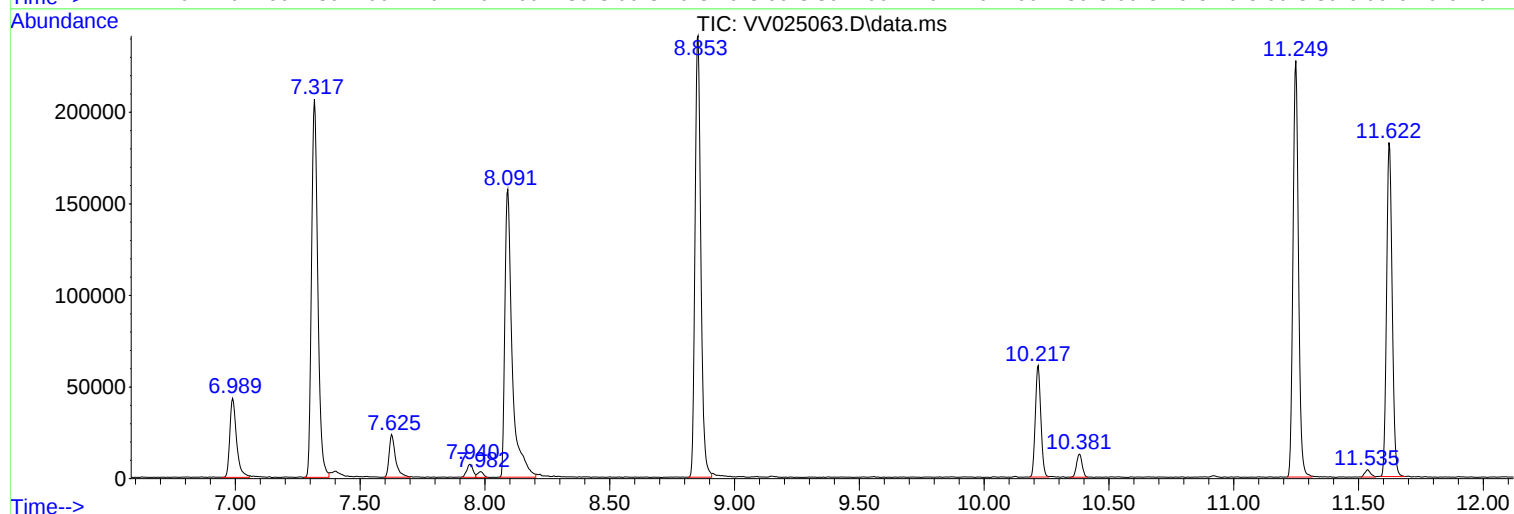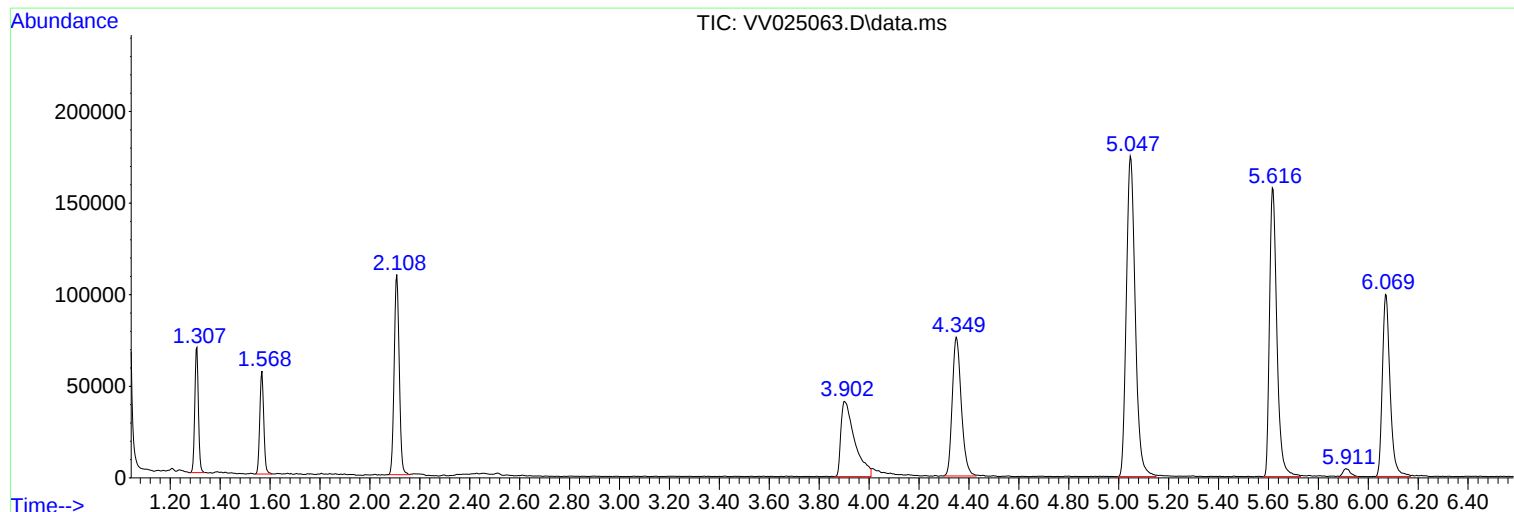

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025063.D
Acq On : 16 Mar 2022 22:05
Operator : SY/MD
Sample : N1941-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025063.D
Acq On : 16 Mar 2022 22:05
Operator : SY/MD
Sample : N1941-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc