

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
 Data File : VV025069.D
 Acq On : 17 Mar 2022 00:25
 Operator : SY/MD
 Sample : N1941-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLG3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025069.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	71919	71958	15.64%	1.903%
2	1.568	156	164	174	rBV	57698	64611	14.05%	1.709%
3	2.018	296	304	319	rVB3	5457	8942	1.94%	0.236%
4	2.108	321	332	344	rBV	112064	162473	35.32%	4.297%
5	3.892	877	887	915	rBV	47606	145670	31.67%	3.852%
6	4.352	1015	1030	1057	rBV	80150	198666	43.19%	5.254%
7	5.050	1231	1247	1277	rBV2	185284	459975	100.00%	12.165%
8	5.619	1412	1424	1447	rBV	163922	328218	71.36%	8.680%
9	5.912	1506	1515	1529	rVB3	4692	9056	1.97%	0.239%
10	6.069	1552	1564	1590	rBV	104230	215118	46.77%	5.689%
11	6.989	1839	1850	1876	rBV	45914	84832	18.44%	2.244%
12	7.137	1886	1896	1913	rVB3	7610	14867	3.23%	0.393%
13	7.317	1941	1952	1970	rBV	216021	375484	81.63%	9.930%
14	7.397	1974	1977	1991	rVB4	3190	5389	1.17%	0.143%
15	7.625	2035	2048	2065	rBV2	24389	44891	9.76%	1.187%
16	8.088	2182	2192	2227	rBV	195624	381237	82.88%	10.082%
17	8.854	2419	2430	2463	rBV	246737	405088	88.07%	10.713%
18	9.571	2646	2653	2667	rBV4	3959	6897	1.50%	0.182%
19	10.217	2840	2854	2870	rBV	69343	109406	23.79%	2.893%
20	10.381	2896	2905	2918	rVB2	5065	7471	1.62%	0.198%
21	11.249	3164	3175	3201	rBV	230860	363038	78.93%	9.601%
22	11.535	3256	3264	3279	rVB2	3489	5939	1.29%	0.157%
23	11.622	3280	3291	3309	rBV	202628	312002	67.83%	8.251%




Sum of corrected areas: 3781228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025069.D
Acq On : 17 Mar 2022 00:25
Operator : SY/MD
Sample : N1941-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

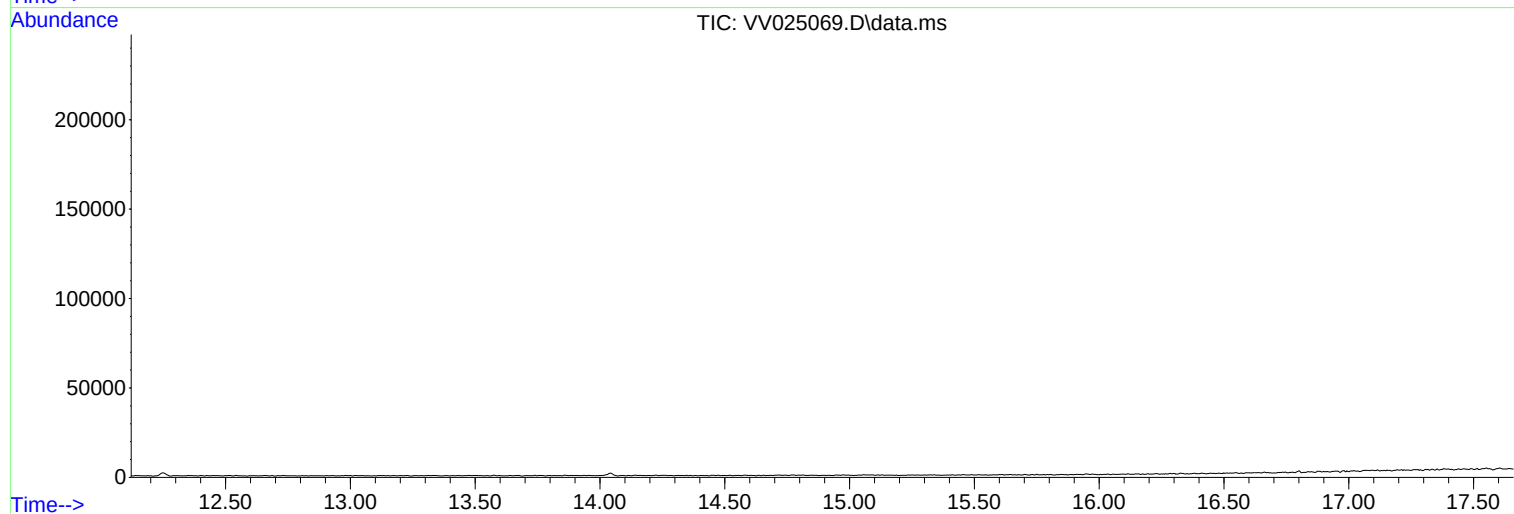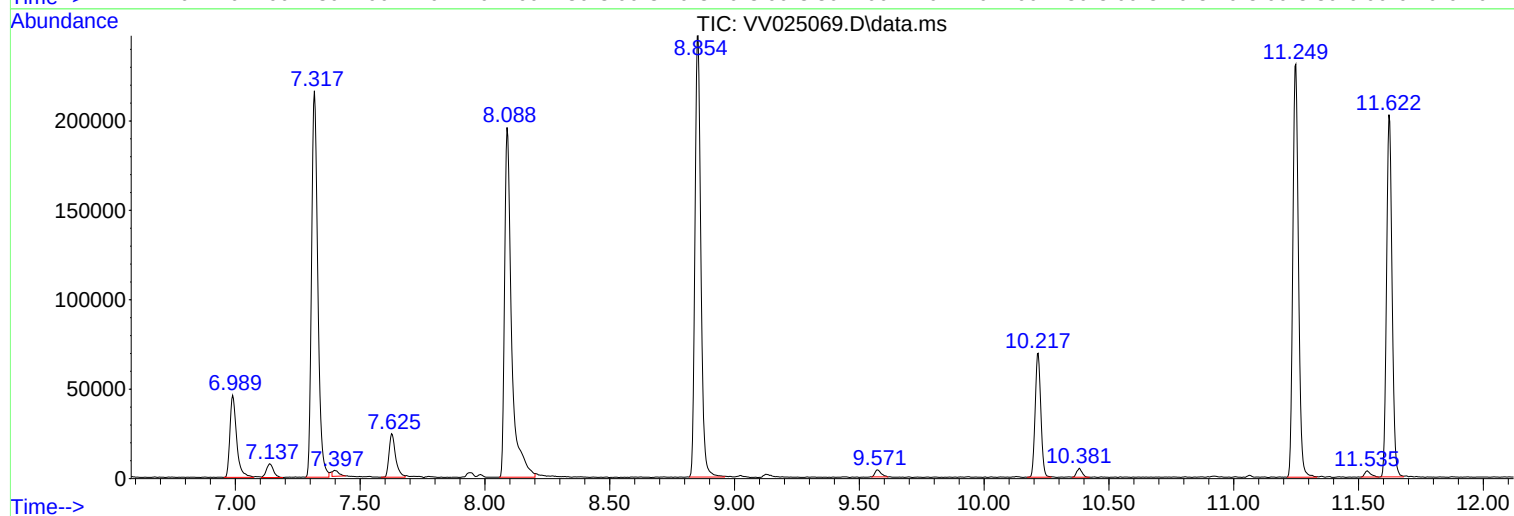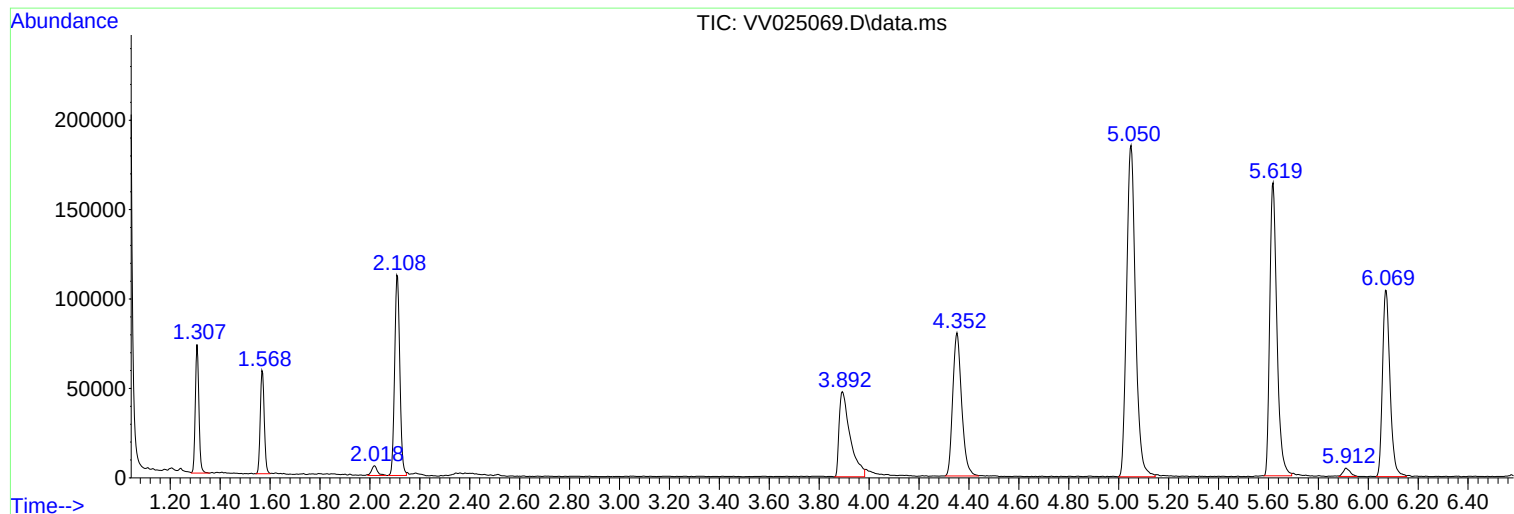

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025069.D
Acq On : 17 Mar 2022 00:25
Operator : SY/MD
Sample : N1941-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031622\
Data File : VV025069.D
Acq On : 17 Mar 2022 00:25
Operator : SY/MD
Sample : N1941-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc