

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031722\
 Data File : VW025085.D
 Acq On : 17 Mar 2022 16:20
 Operator : SY/MD
 Sample : N1941-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Mar 18 02:22:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 18 02:20:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	140581	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	133236	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58882	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	54364	4.898	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.000%
7) Chloroethane-d5	1.568	69	41106	5.058	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.200%
11) 1,1-Dichloroethene-d2	2.108	63	67029	3.737	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.800%
20) 2-Butanone-d5	3.912	46	60787	45.319	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.640%
24) Chloroform-d	4.352	84	85490	4.644	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.800%
26) 1,2-Dichloroethane-d4	5.037	65	36500	4.743	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
32) Benzene-d6	5.053	84	181724	4.702	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
36) 1,2-Dichloropropane-d6	6.072	67	52519	4.725	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.600%
41) Toluene-d8	7.317	98	155279	4.408	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.200%
43) trans-1,3-Dichloroprop...	7.625	79	16410	4.235	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.800%
46) 2-Hexanone-d5	8.092	63	55223	41.786	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.580%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	29907	4.574	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	48219	4.837	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.800%
Target Compounds						
25) Chloroform	4.384	83	2493	0.131	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025085.D
Acq On : 17 Mar 2022 16:20
Operator : SY/MD
Sample : N1941-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Mar 18 02:22:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 18 02:20:05 2022
Response via : Initial Calibration

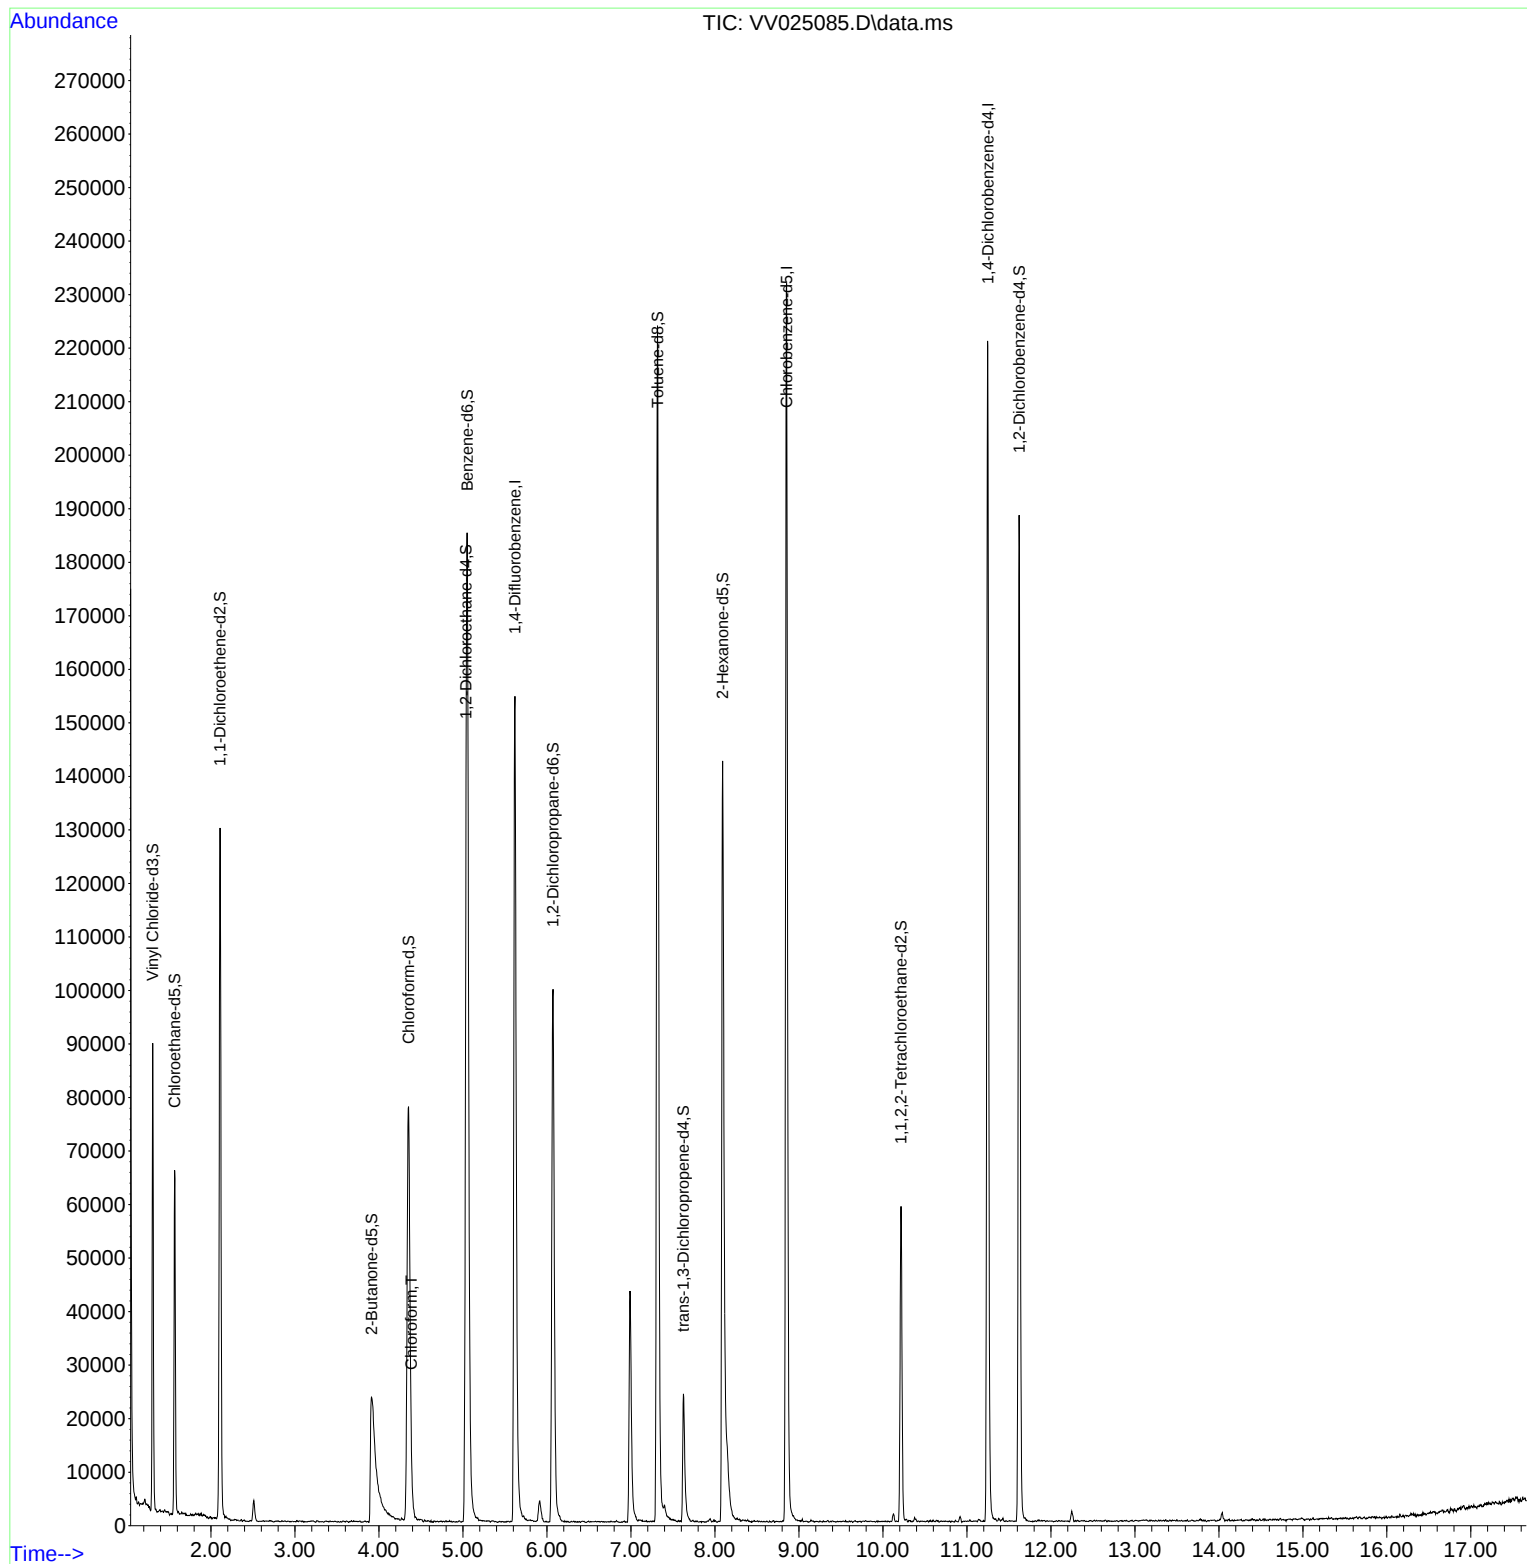

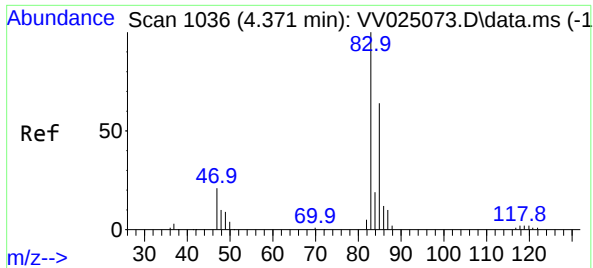

#25
 Chloroform
 Concen: 0.131 ug/L
 RT: 4.384 min Scan# 10
 Delta R.T. 0.013 min
 Lab File: VV025085.D
 Acq: 17 Mar 2022 16:20

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion:	83	Resp:	2493
Ion	Ratio	Lower	Upper
83	100		
85	67.0	44.5	82.7

