

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
 Data File : VV025074.D
 Acq On : 17 Mar 2022 11:33
 Operator : SY/MD
 Sample : VV0317WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK318

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	102	rVB	95828	99433	19.80%	2.558%
2	1.568	155	164	175	rBV	70565	79813	15.90%	2.053%
3	2.105	320	331	352	rBV	147539	211120	42.05%	5.431%
4	2.507	447	456	469	rVB	8984	13806	2.75%	0.355%
5	3.040	613	622	633	rBV3	3516	5971	1.19%	0.154%
6	3.921	885	896	944	rBV2	18187	103855	20.68%	2.672%
7	4.346	1011	1028	1055	rBV2	84972	214641	42.75%	5.522%
8	5.043	1230	1245	1277	rBV2	205422	502104	100.00%	12.917%
9	5.613	1407	1422	1450	rBV	161044	330835	65.89%	8.511%
10	5.905	1505	1513	1531	rVB5	4537	9410	1.87%	0.242%
11	6.066	1549	1563	1591	rBV2	108695	229113	45.63%	5.894%
12	6.986	1839	1849	1877	rBV	49332	92468	18.42%	2.379%
13	7.313	1940	1951	1971	rBV	248219	435246	86.68%	11.197%
14	7.394	1971	1976	1987	rVB3	3380	6282	1.25%	0.162%
15	7.622	2038	2047	2070	rBV	26497	47918	9.54%	1.233%
16	8.092	2183	2193	2234	rBV	140496	316955	63.13%	8.154%
17	8.850	2418	2429	2451	rBV	241311	400742	79.81%	10.309%
18	10.214	2843	2853	2867	rBV2	62051	99321	19.78%	2.555%
19	11.246	3164	3174	3194	rBV	233149	361568	72.01%	9.301%
20	11.622	3279	3291	3308	rBV	207342	326624	65.05%	8.402%




Sum of corrected areas: 3887225

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025074.D
Acq On : 17 Mar 2022 11:33
Operator : SY/MD
Sample : VV0317WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

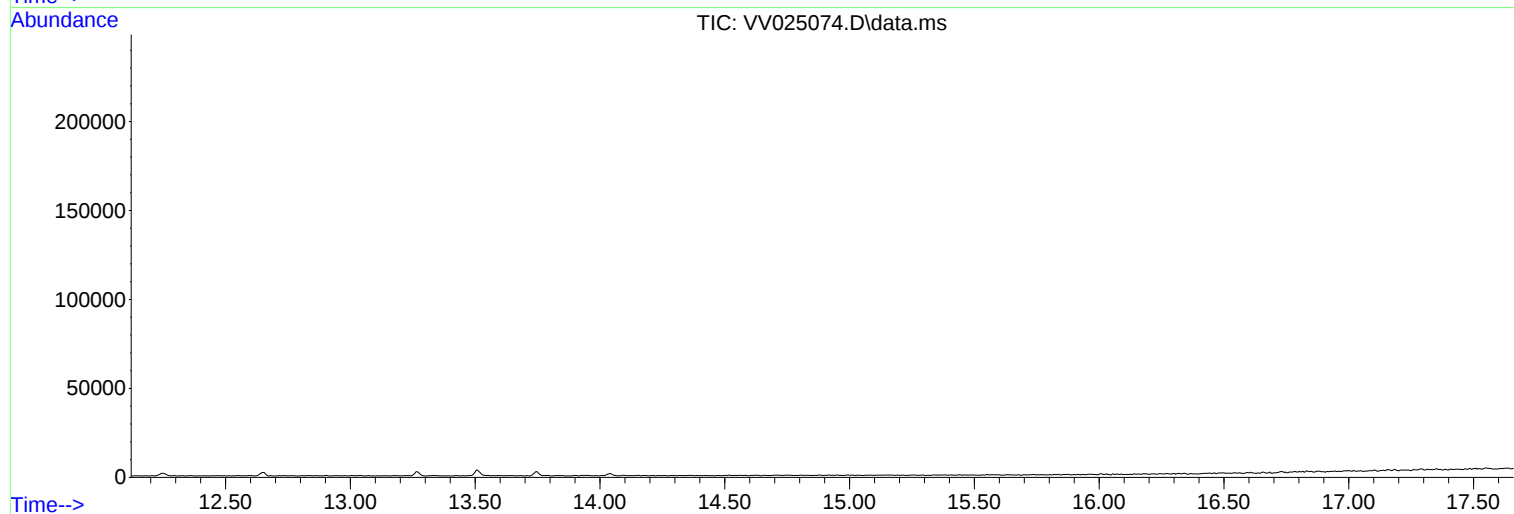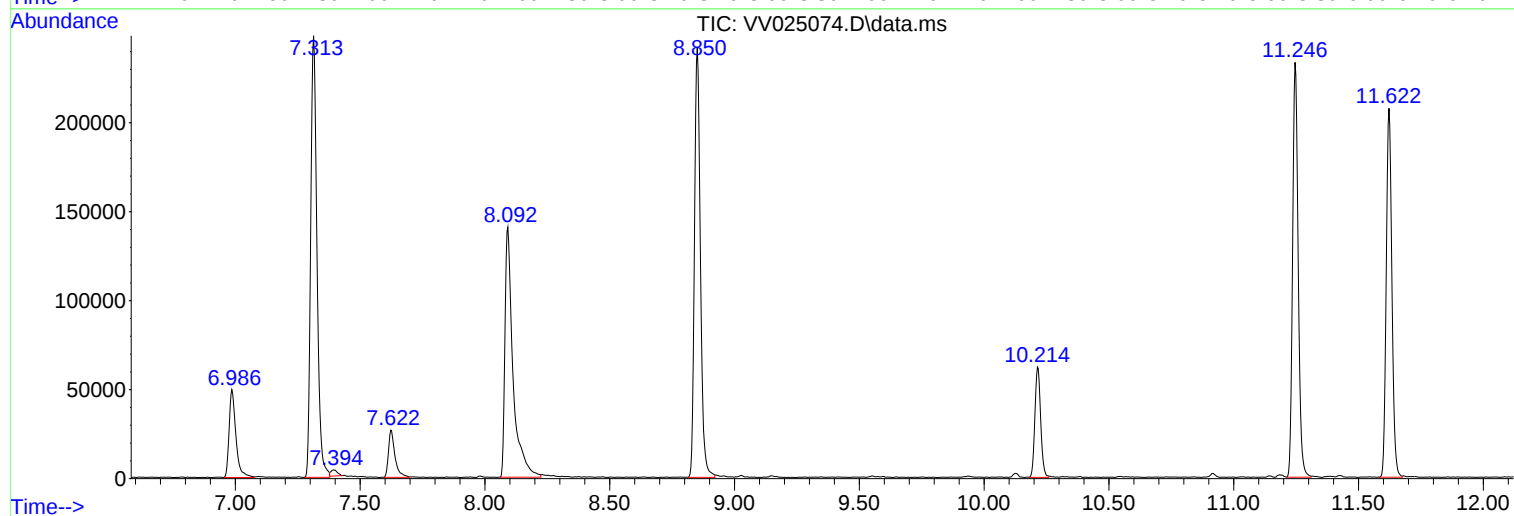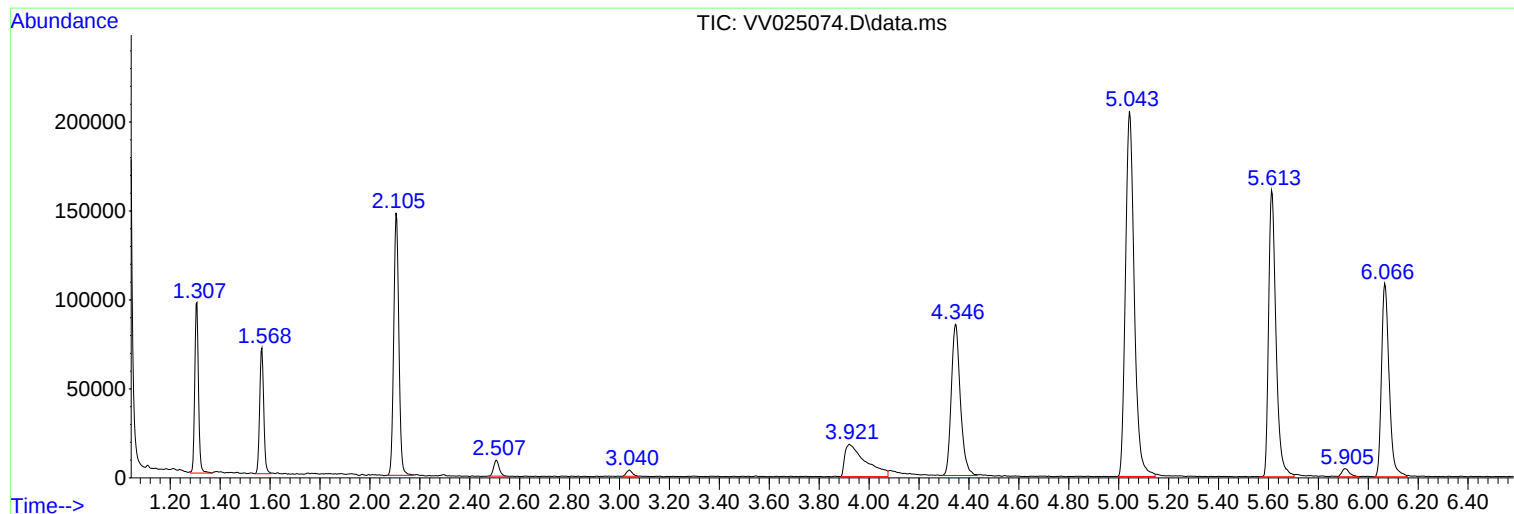

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025074.D
Acq On : 17 Mar 2022 11:33
Operator : SY/MD
Sample : VV0317WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025074.D
Acq On : 17 Mar 2022 11:33
Operator : SY/MD
Sample : VV0317WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK318

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------