

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
 Data File : VV025076.D
 Acq On : 17 Mar 2022 12:41
 Operator : SY/MD
 Sample : VIBLK262
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK262

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	99	rVB	93760	94383	19.16%	2.475%
2	1.568	156	164	183	rVB	70167	79528	16.15%	2.085%
3	2.108	320	332	352	rBV	140551	203303	41.28%	5.330%
4	2.510	447	457	470	rBV	19586	31640	6.42%	0.830%
5	3.915	883	894	937	rBV2	25199	113757	23.10%	2.983%
6	4.352	1014	1030	1057	rBV2	82257	209183	42.47%	5.485%
7	5.050	1232	1247	1279	rBV2	201043	492536	100.00%	12.914%
8	5.619	1412	1424	1454	rBV	154230	319473	64.86%	8.376%
9	5.915	1507	1516	1530	rVB4	3814	7717	1.57%	0.202%
10	6.072	1552	1565	1587	rBV	105468	218849	44.43%	5.738%
11	6.989	1839	1850	1873	rBV	47394	88716	18.01%	2.326%
12	7.317	1941	1952	1971	rBV	243622	423195	85.92%	11.096%
13	7.625	2038	2048	2071	rBV	25153	46279	9.40%	1.213%
14	7.940	2135	2146	2155	rBV2	4478	7723	1.57%	0.202%
15	8.091	2183	2193	2230	rBV	148979	313103	63.57%	8.209%
16	8.853	2419	2430	2461	rBV	237838	390350	79.25%	10.235%
17	10.214	2840	2853	2870	rBV	63128	98065	19.91%	2.571%
18	10.381	2893	2905	2916	rBV4	5505	9215	1.87%	0.242%
19	11.249	3163	3175	3201	rBV	224653	349484	70.96%	9.163%
20	11.622	3280	3291	3312	rBV	202016	317517	64.47%	8.325%




Sum of corrected areas: 3814016

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025076.D
Acq On : 17 Mar 2022 12:41
Operator : SY/MD
Sample : VIBLK262
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

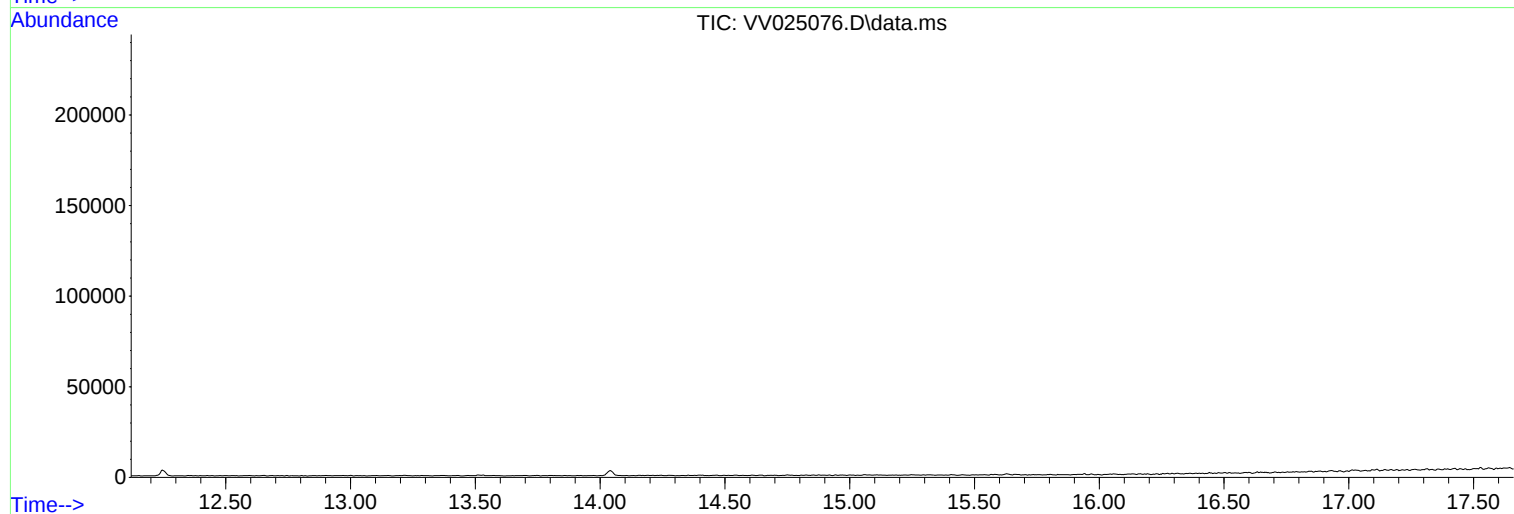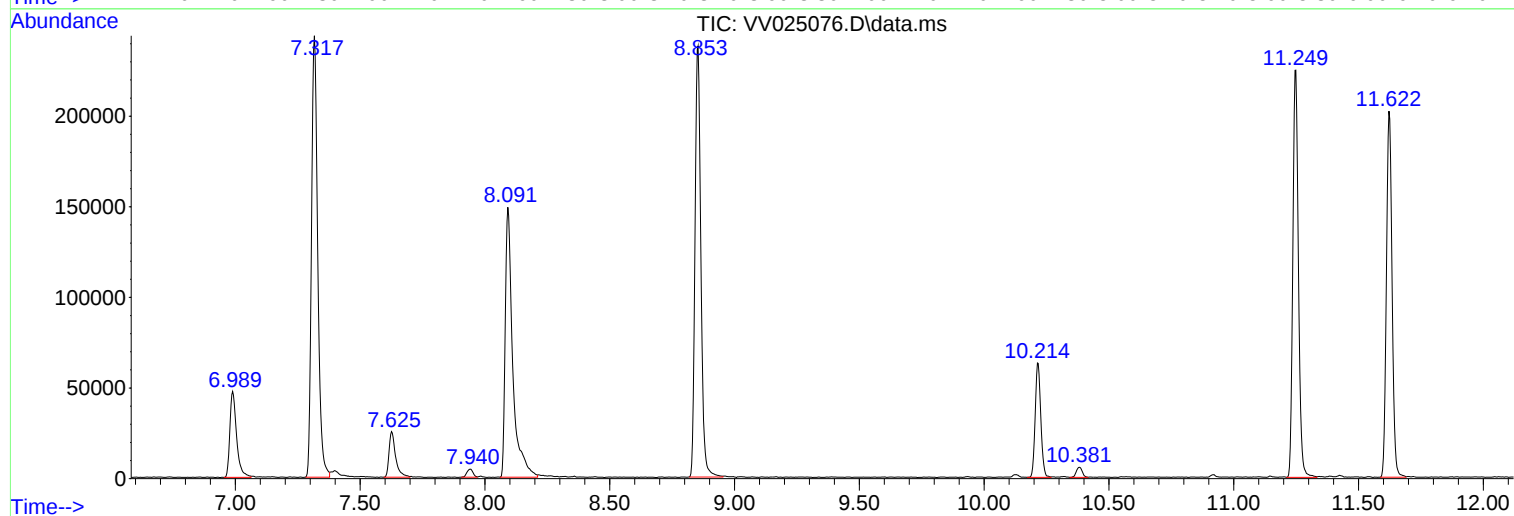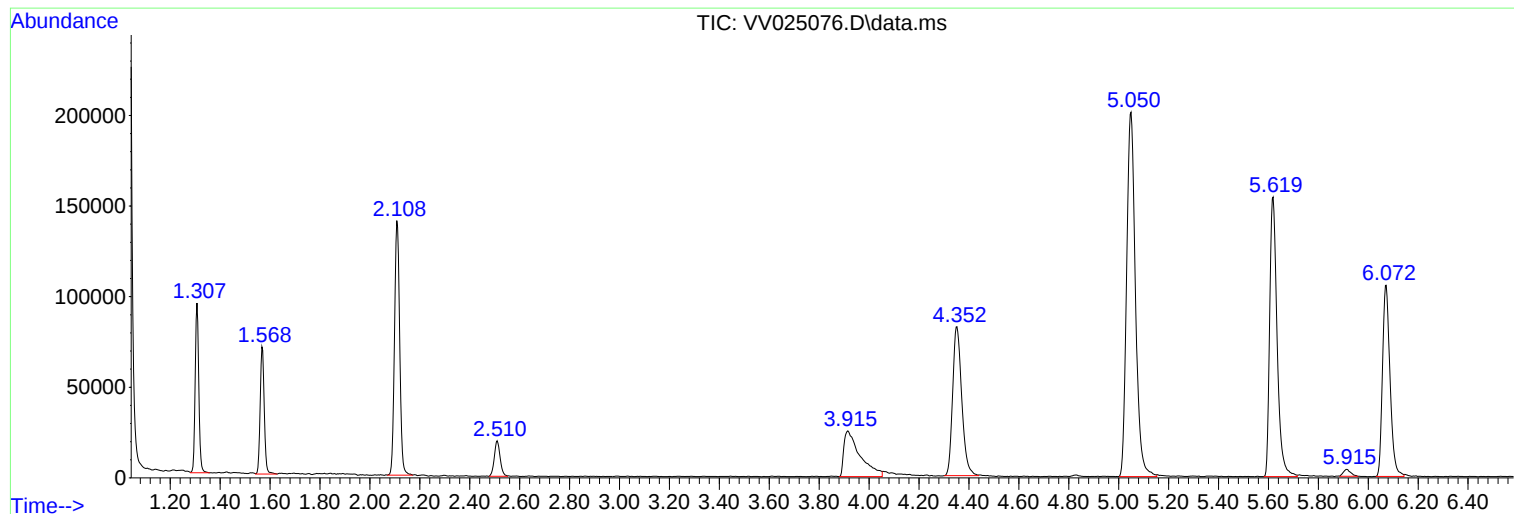

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025076.D
Acq On : 17 Mar 2022 12:41
Operator : SY/MD
Sample : VIBLK262
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025076.D
Acq On : 17 Mar 2022 12:41
Operator : SY/MD
Sample : VIBLK262
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK262

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------