

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
 Data File : VV025081.D
 Acq On : 17 Mar 2022 14:46
 Operator : SY/MD
 Sample : N1941-01DL 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLF1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	96739	95379	19.33%	2.325%
2	1.568	156	164	183	rVB	69902	80466	16.30%	1.961%
3	2.108	320	332	355	rVB	142480	203419	41.22%	4.958%
4	2.510	446	457	469	rVB2	8936	14528	2.94%	0.354%
5	3.912	883	893	934	rBV2	25931	117846	23.88%	2.872%
6	4.352	1013	1030	1062	rBV	83887	210879	42.73%	5.140%
7	5.050	1232	1247	1276	rBV2	201152	493512	100.00%	12.029%
8	5.619	1413	1424	1457	rBV	138997	283118	57.37%	6.901%
9	5.915	1504	1516	1534	rVB7	4822	11006	2.23%	0.268%
10	6.069	1552	1564	1592	rBV2	108344	223558	45.30%	5.449%
11	6.989	1840	1850	1880	rBV	47167	88982	18.03%	2.169%
12	7.317	1941	1952	1973	rBV	246336	431099	87.35%	10.508%
13	7.397	1974	1977	1991	rVB4	3263	5458	1.11%	0.133%
14	7.625	2036	2048	2077	rBV	24909	45792	9.28%	1.116%
15	7.976	2135	2157	2177	rBV	216854	376931	76.38%	9.187%
16	8.092	2184	2193	2226	rBV	157150	328582	66.58%	8.009%
17	8.854	2415	2430	2448	rBV	206065	345322	69.97%	8.417%
18	10.217	2839	2854	2872	rVB	62156	100601	20.38%	2.452%
19	10.381	2897	2905	2915	rVB3	6311	9789	1.98%	0.239%
20	11.249	3164	3175	3194	rBV	201603	310890	63.00%	7.578%
21	11.622	3277	3291	3315	rBV	203049	319764	64.79%	7.794%
22	12.249	3473	3486	3503	rVB2	3655	5818	1.18%	0.142%




Sum of corrected areas: 4102739

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025081.D
Acq On : 17 Mar 2022 14:46
Operator : SY/MD
Sample : N1941-01DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

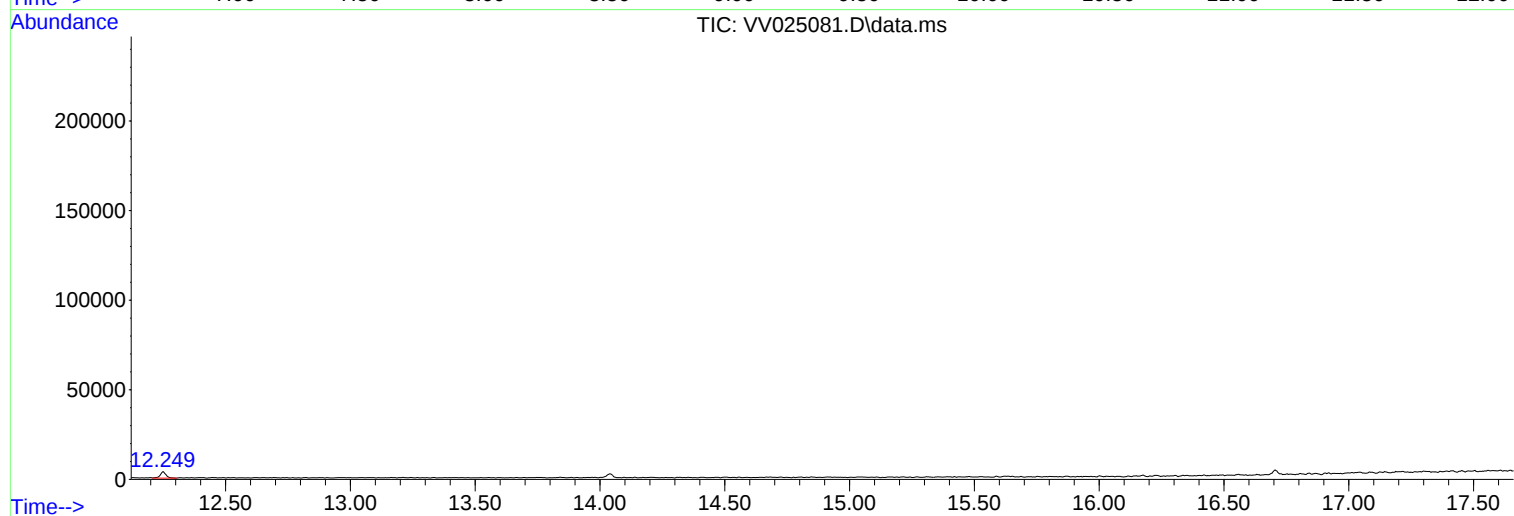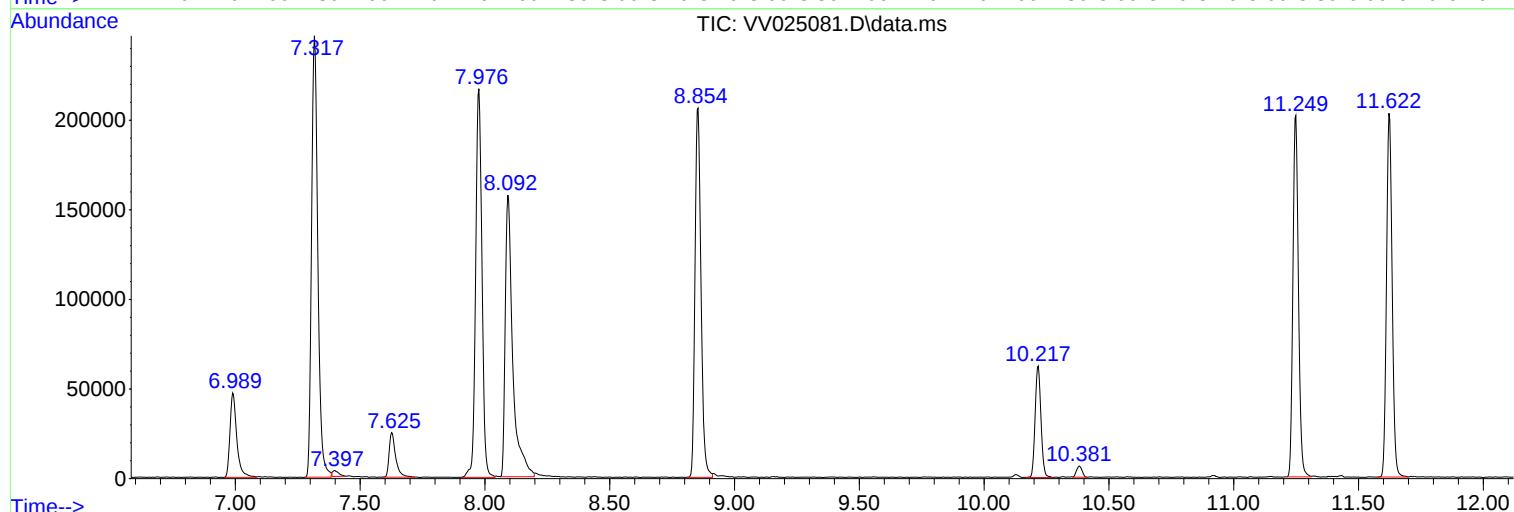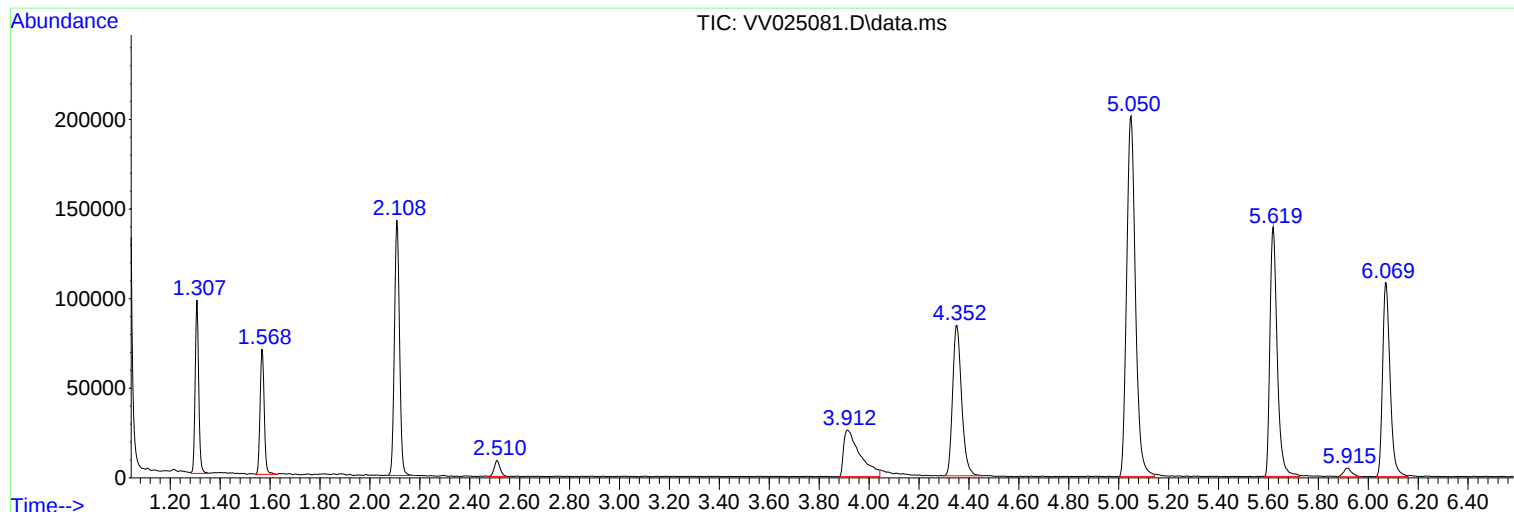

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025081.D
Acq On : 17 Mar 2022 14:46
Operator : SY/MD
Sample : N1941-01DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025081.D
Acq On : 17 Mar 2022 14:46
Operator : SY/MD
Sample : N1941-01DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc