

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
 Data File : VV025083.D
 Acq On : 17 Mar 2022 15:33
 Operator : SY/MD
 Sample : N1933-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDD2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025083.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	97	rVB	91539	96921	4.50%	1.451%
2	1.571	156	165	180	rVB	70400	78137	3.63%	1.170%
3	2.111	322	333	346	rBV	138386	199570	9.27%	2.988%
4	2.188	346	357	386	rVB	15053	45920	2.13%	0.688%
5	3.902	877	890	901	rBV	39958	108469	5.04%	1.624%
6	3.973	902	912	952	rVB2	100181	339723	15.78%	5.087%
7	4.346	1014	1028	1079	rBV2	217633	634329	29.46%	9.498%
8	4.828	1158	1178	1210	rBV	908051	2153277	100.00%	32.242%
9	5.050	1230	1247	1274	rBV2	198575	483976	22.48%	7.247%
10	5.619	1412	1424	1451	rBV	159146	323579	15.03%	4.845%
11	6.072	1553	1565	1587	rBV	104392	215049	9.99%	3.220%
12	6.989	1838	1850	1873	rBV2	47916	88749	4.12%	1.329%
13	7.317	1941	1952	1972	rBV	232910	413081	19.18%	6.185%
14	7.625	2038	2048	2071	rBV2	26068	47198	2.19%	0.707%
15	8.091	2183	2193	2224	rBV	152617	308748	14.34%	4.623%
16	8.850	2419	2429	2451	rBV	235472	386203	17.94%	5.783%
17	10.217	2844	2854	2872	rVB	59936	94891	4.41%	1.421%
18	11.249	3164	3175	3196	rBV	226731	350495	16.28%	5.248%
19	11.622	3280	3291	3310	rVV	197408	310265	14.41%	4.646%




Sum of corrected areas: 6678580

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025083.D
Acq On : 17 Mar 2022 15:33
Operator : SY/MD
Sample : N1933-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

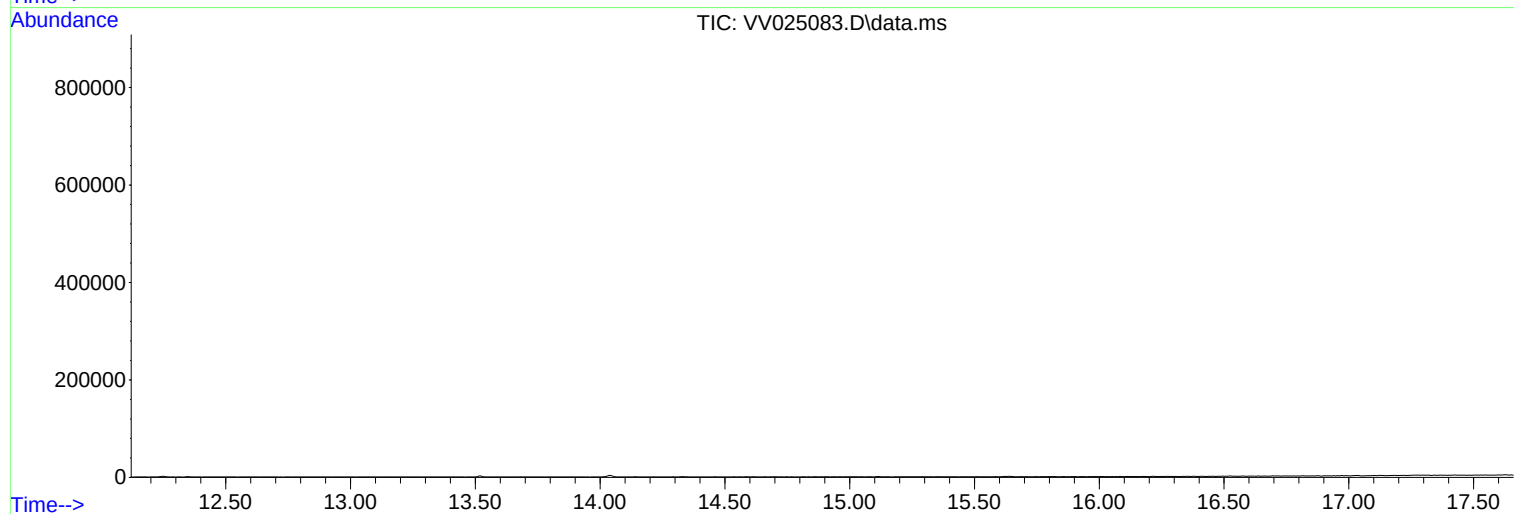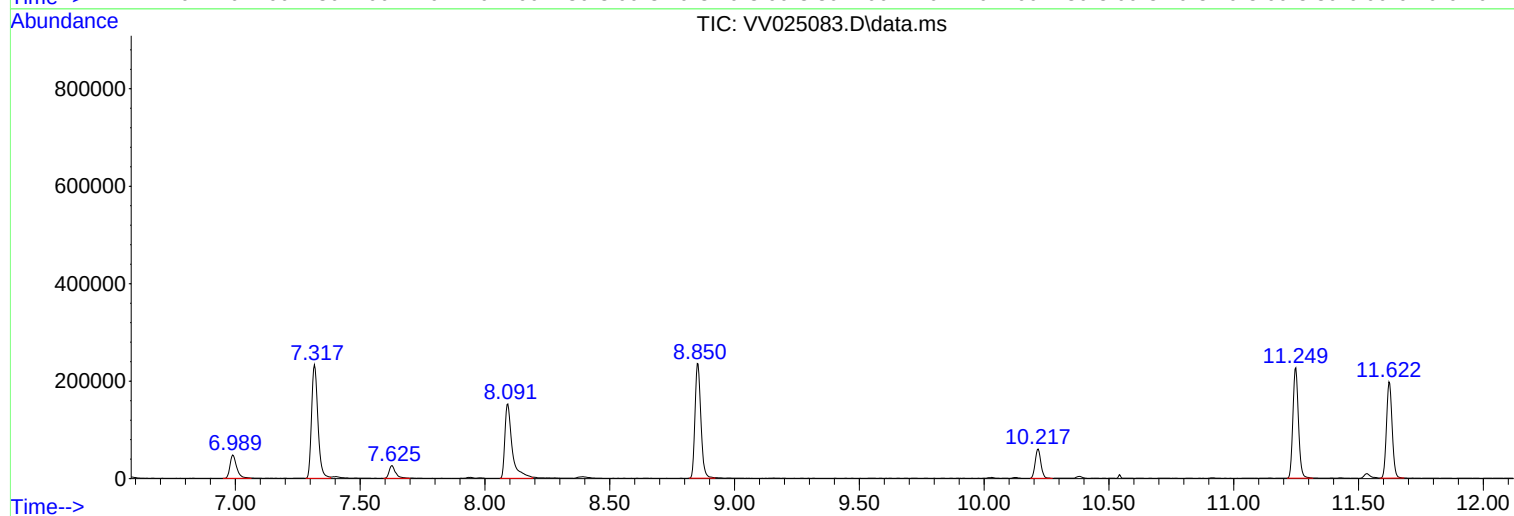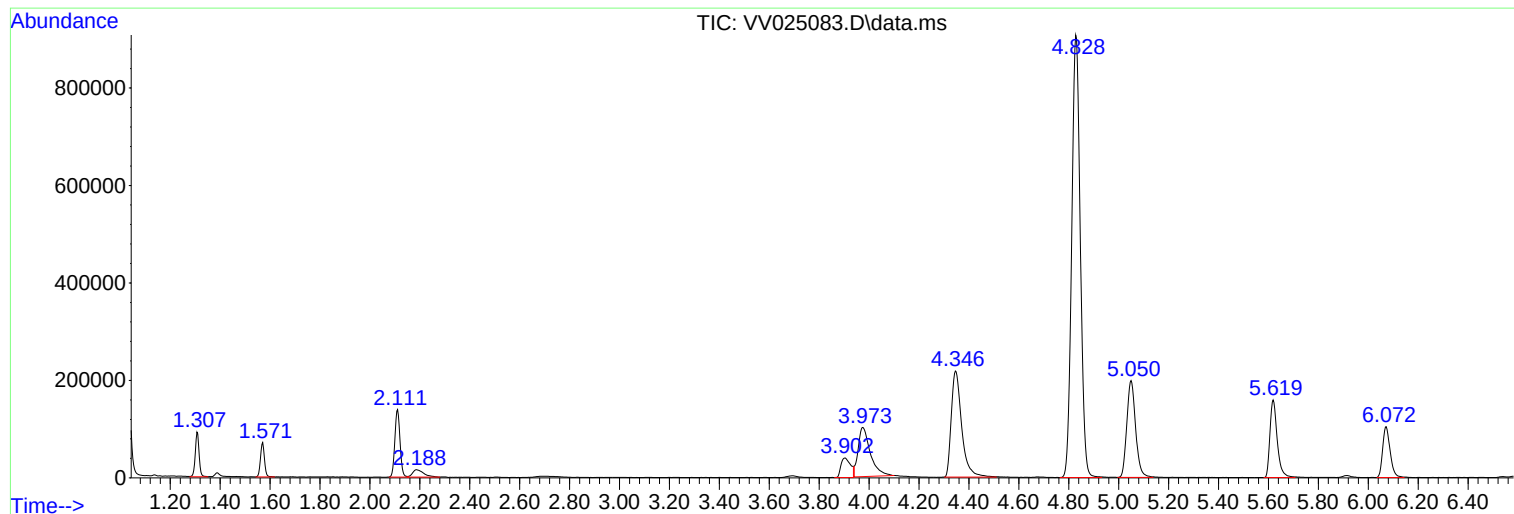

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025083.D
Acq On : 17 Mar 2022 15:33
Operator : SY/MD
Sample : N1933-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025083.D
Acq On : 17 Mar 2022 15:33
Operator : SY/MD
Sample : N1933-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
