

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
 Data File : VV025084.D
 Acq On : 17 Mar 2022 15:57
 Operator : SY/MD
 Sample : N1933-22
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rVB	92961	92547	19.83%	2.518%
2	1.568	157	164	180	rBV	65637	75403	16.16%	2.051%
3	2.111	322	333	350	rBV	134587	194275	41.62%	5.285%
4	2.513	448	458	468	rBV2	4563	7692	1.65%	0.209%
5	3.905	882	891	923	rBV2	27996	107384	23.01%	2.921%
6	4.352	1014	1030	1056	rBV	79830	200768	43.01%	5.462%
7	5.050	1232	1247	1280	rBV2	190209	466745	100.00%	12.698%
8	5.619	1409	1424	1452	rBV	156557	315263	67.55%	8.577%
9	5.918	1507	1517	1530	rVB6	3457	8275	1.77%	0.225%
10	6.072	1552	1565	1589	rBV	101993	211207	45.25%	5.746%
11	6.989	1841	1850	1877	rBV	44719	84138	18.03%	2.289%
12	7.317	1941	1952	1970	rBV	231885	401977	86.12%	10.936%
13	7.625	2036	2048	2069	rBV	24557	44310	9.49%	1.205%
14	7.937	2134	2145	2157	rBV3	5282	9199	1.97%	0.250%
15	8.091	2182	2193	2225	rBV	149208	307641	65.91%	8.369%
16	8.853	2418	2430	2454	rBV	232768	387133	82.94%	10.532%
17	10.214	2843	2853	2866	rBV	61427	94731	20.30%	2.577%
18	10.381	2896	2905	2923	rVB3	7211	11485	2.46%	0.312%
19	11.249	3163	3175	3197	rBV	224076	345941	74.12%	9.411%
20	11.622	3279	3291	3306	rBV	193872	302435	64.80%	8.228%
21	12.246	3474	3485	3499	rVB2	4242	7199	1.54%	0.196%




Sum of corrected areas: 3675748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025084.D
Acq On : 17 Mar 2022 15:57
Operator : SY/MD
Sample : N1933-22
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

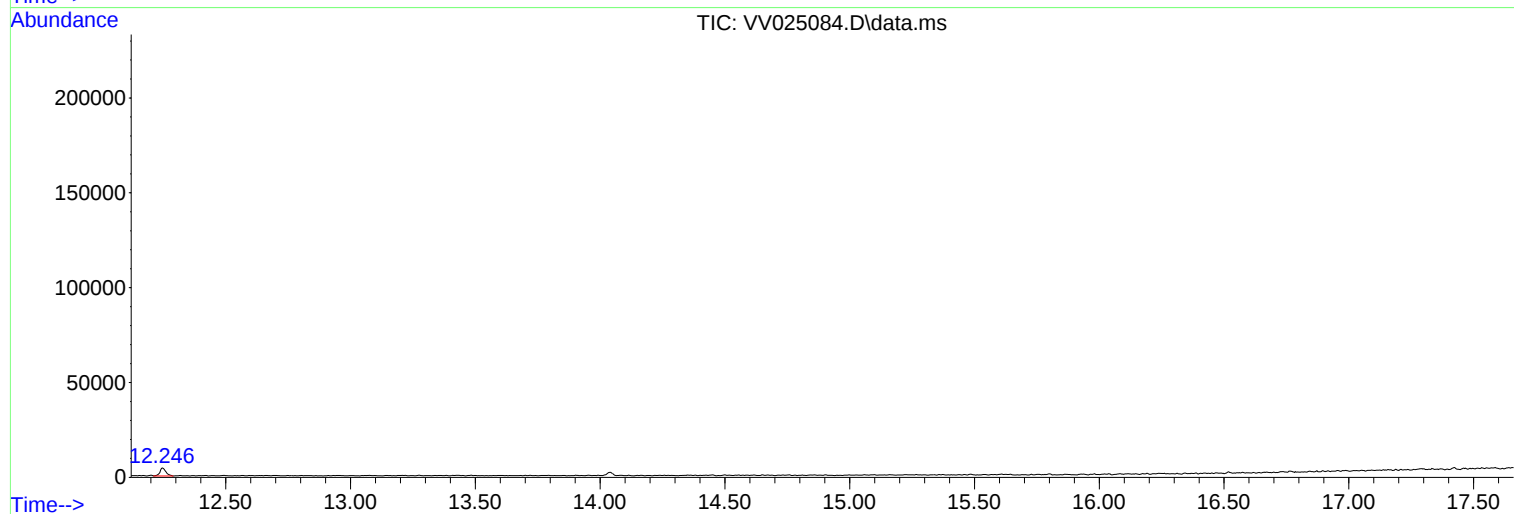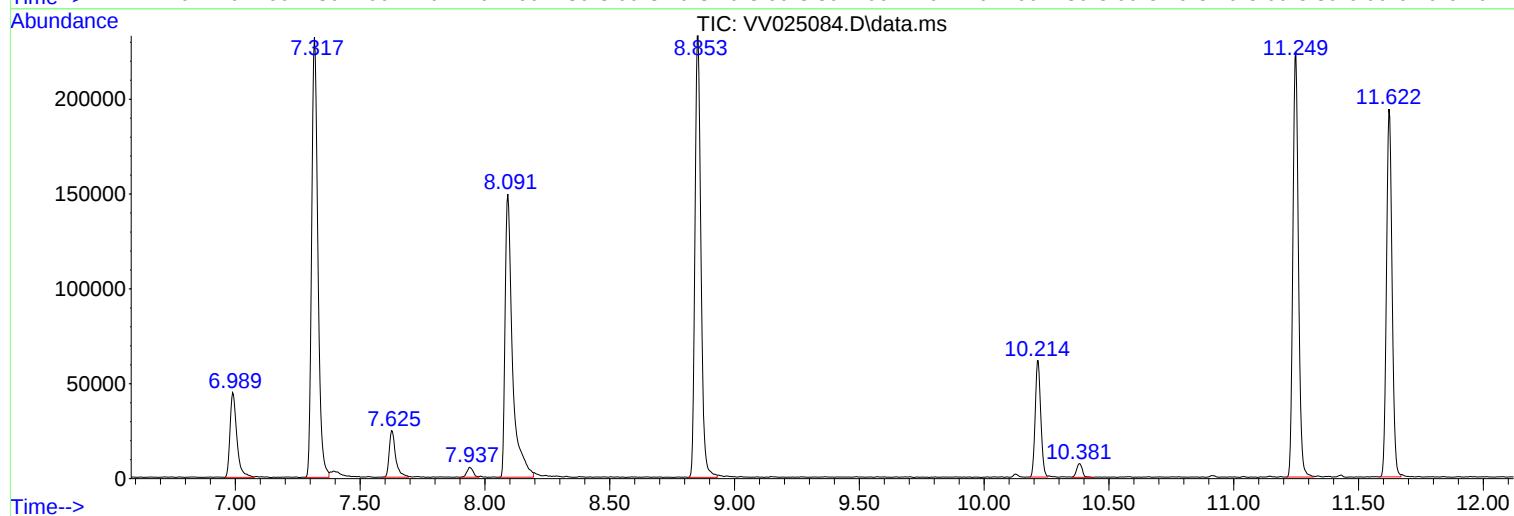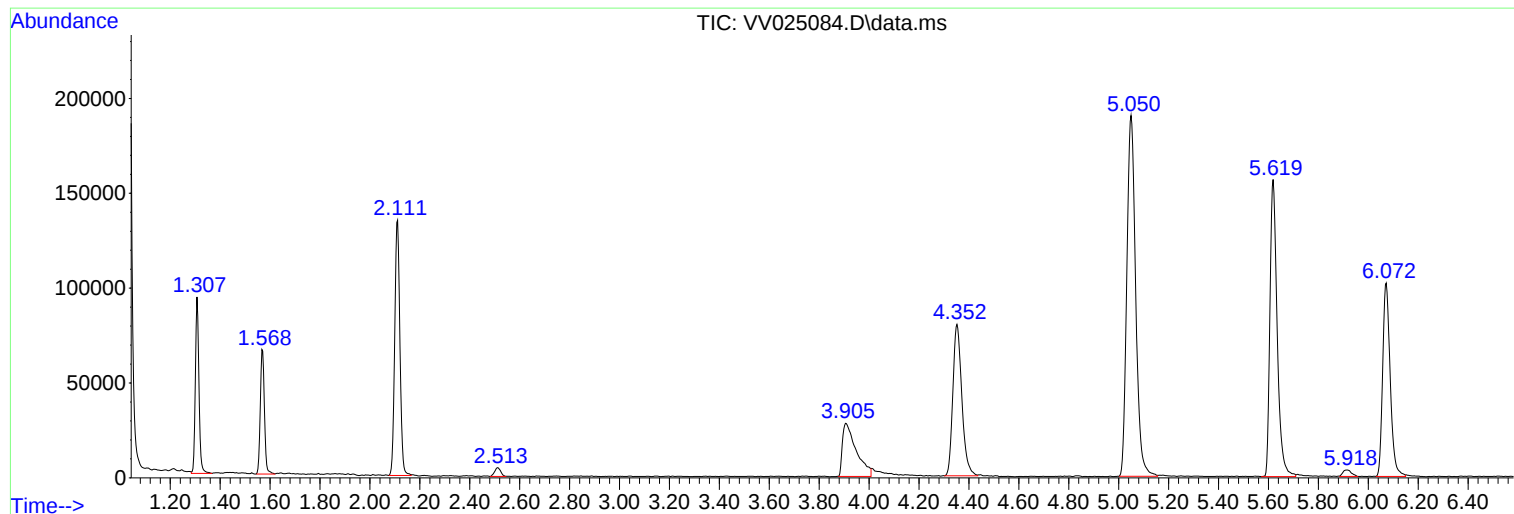

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025084.D
Acq On : 17 Mar 2022 15:57
Operator : SY/MD
Sample : N1933-22
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
Data File : VV025084.D
Acq On : 17 Mar 2022 15:57
Operator : SY/MD
Sample : N1933-22
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc