
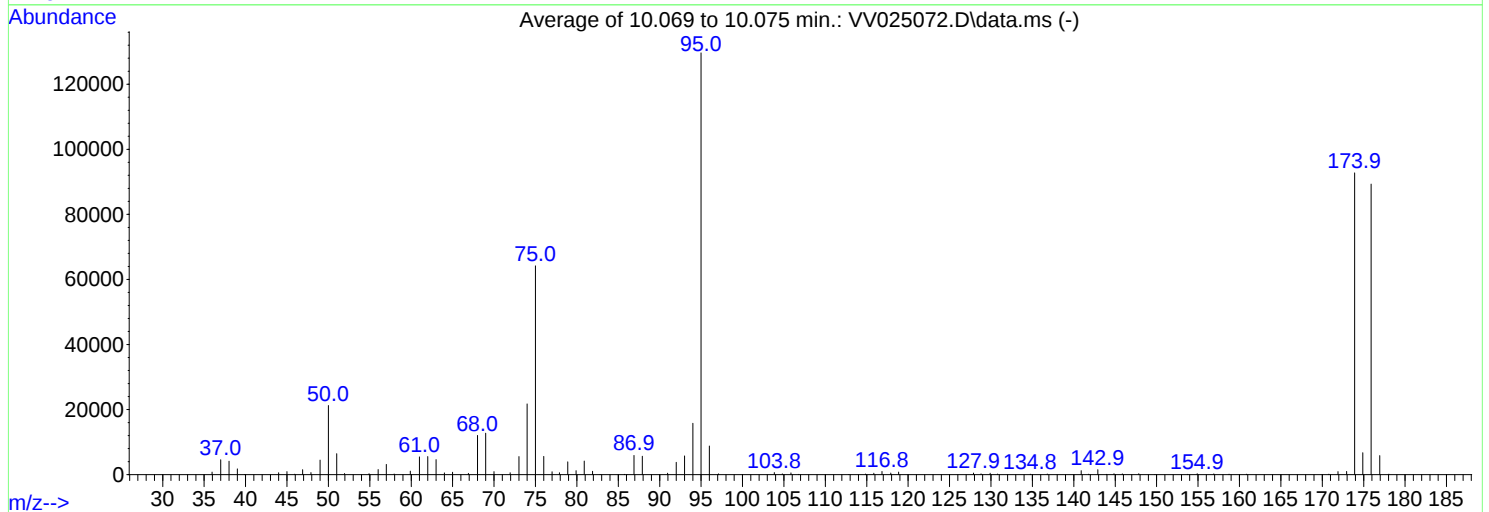


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031722\
 Data File : VV025072.D
 Acq On : 17 Mar 2022 09:49
 Operator : SY/MD
 Sample : BFB281
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB281

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 25 23:19:44 2022

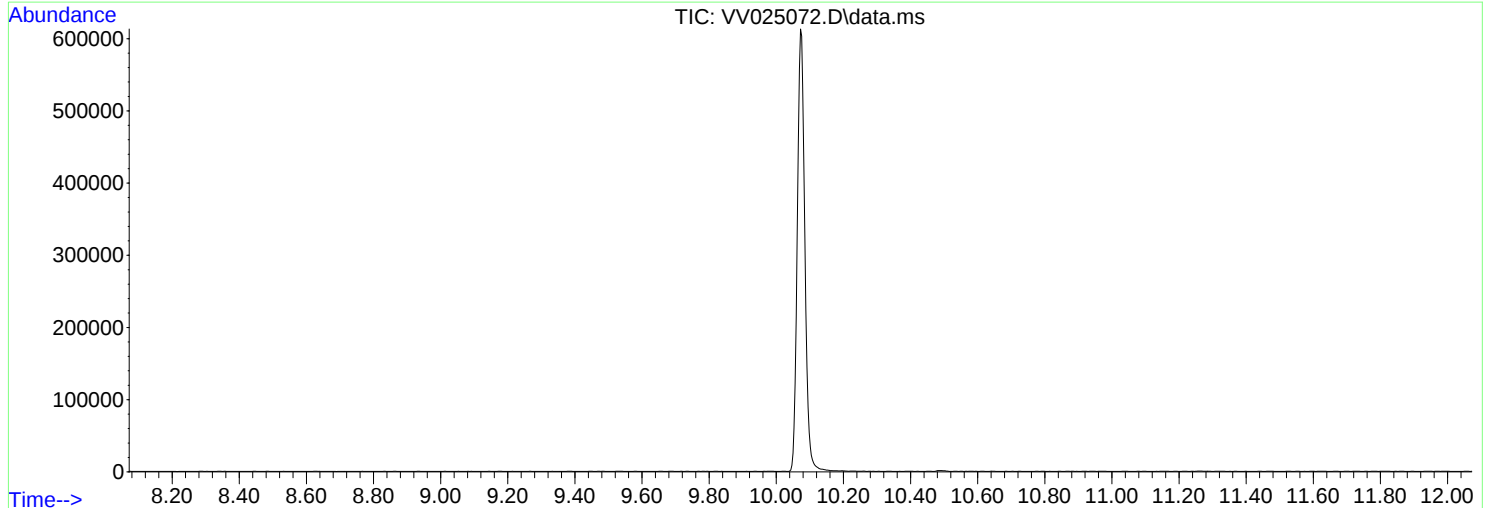

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	21259	PASS
75	95	30	80	49.5	64200	PASS
95	95	100	100	100.0	129651	PASS
96	95	5	9	6.8	8784	PASS
173	174	0.00	2	1.0	968	PASS
174	95	50	120	71.5	92739	PASS
175	174	5	9	7.3	6742	PASS
176	174	95	105	96.3	89331	PASS
177	176	5	10	6.6	5867	PASS

m/z	Abundance
39.90	522.0
44.00	236.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
35.90	779.0
37.00	4529.0
38.00	4061.0
39.00	1687.0
39.90	619.0
44.00	751.0
45.00	941.0
46.00	123.0
46.90	1439.0
47.90	647.0
49.00	4270.0
50.00	20536.0
51.00	6474.0
51.90	332.0
54.90	281.0
56.00	1578.0
57.00	2925.0
58.00	177.0
59.90	1075.0
61.00	5284.0
62.00	5290.0
63.00	4391.0
64.00	530.0
65.00	660.0
66.90	400.0
68.00	11454.0
69.00	12341.0
70.00	852.0
71.90	650.0
73.00	5289.0
74.00	20640.0
75.00	60936.0
76.00	5349.0
77.00	771.0
78.00	585.0
78.90	3707.0
79.90	1186.0
80.90	4016.0
81.90	1022.0
85.80	174.0
86.90	5773.0
87.90	5402.0
91.00	404.0
92.00	3691.0
93.00	5562.0
94.00	15089.0
95.00	123032.0
96.00	8486.0
97.10	233.0
103.80	530.0
104.80	221.0
105.80	498.0
106.80	116.0
112.90	106.0
114.90	160.0
115.80	481.0
116.80	916.0
117.90	436.0
118.80	766.0
127.90	481.0
128.80	185.0
129.90	444.0
130.80	172.0
134.70	161.0
136.80	205.0
140.90	1205.0
141.80	117.0
142.90	1542.0
144.00	101.0
144.90	304.0
145.90	228.0
147.80	277.0
149.80	114.0
154.90	259.0
156.90	234.0
158.70	115.0
160.90	140.0
170.80	148.0
171.90	950.0
173.00	856.0
173.90	85392.0
174.90	6312.0
175.90	81896.0
177.00	5717.0
178.00	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
36.00	808.0
37.00	4747.0
38.00	4247.0
39.00	1835.0
39.90	611.0
44.00	849.0
45.00	1011.0
46.00	146.0
46.90	1633.0
47.90	655.0
49.00	4664.0
50.00	22048.0
51.00	6637.0
51.90	404.0
54.90	309.0
56.00	1649.0
57.00	3309.0
57.90	204.0
59.90	1148.0
61.00	5622.0
62.00	5745.0
63.00	4819.0
64.00	551.0
65.00	765.0
66.90	441.0
68.00	12502.0
69.00	13198.0
70.00	945.0
72.00	611.0
73.00	5795.0
74.00	22688.0
75.00	66576.0
76.00	5824.0
77.00	927.0
77.90	625.0
78.90	4070.0
79.90	1300.0
80.90	4292.0
81.90	1050.0
85.70	121.0
86.00	119.0
86.90	6124.0
87.90	5800.0
91.00	430.0
92.00	3970.0
93.00	5978.0
94.00	16325.0
95.00	134400.0
96.00	9178.0
97.10	258.0
103.90	639.0
104.80	271.0
105.90	593.0
106.80	128.0
112.80	106.0
114.90	196.0
115.80	471.0
116.80	1010.0
117.90	504.0
118.90	839.0
127.90	537.0
128.80	243.0
129.90	473.0
130.80	191.0
134.80	159.0
136.80	214.0
140.90	1280.0
141.80	154.0
142.90	1610.0
144.00	114.0
144.80	319.0
145.80	234.0
147.80	319.0
149.80	111.0
153.80	121.0
154.90	312.0
156.90	239.0
158.70	143.0
160.90	169.0
170.80	130.0
171.90	941.0
172.90	1008.0
173.90	96024.0
174.90	6977.0
175.90	92448.0
177.00	6033.0
178.10	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
36.00	726.0
37.00	4434.0
38.00	4104.0
39.00	1821.0
39.90	561.0
44.00	845.0
45.00	950.0
45.90	133.0
46.90	1576.0
47.90	648.0
49.00	4538.0
50.00	21192.0
51.00	6265.0
52.00	371.0
54.90	309.0
56.00	1568.0
57.00	3270.0
58.00	166.0
59.90	1079.0
61.00	5426.0
62.00	5596.0
63.00	4708.0
64.00	513.0
65.00	795.0
66.90	396.0
68.00	12170.0
69.00	12728.0
70.00	945.0
72.00	574.0
73.00	5551.0
74.00	21904.0
75.00	65088.0
76.00	5598.0
77.00	953.0
77.80	600.0
78.90	4038.0
79.90	1261.0
80.90	4172.0
81.90	1000.0
82.80	116.0
86.10	111.0
86.90	5821.0
87.90	5739.0
90.90	440.0
92.00	3756.0
93.00	5809.0
94.00	15961.0
95.00	131520.0
96.00	8687.0
97.10	227.0
103.90	713.0
104.80	238.0
105.90	588.0
106.80	138.0
114.80	185.0
115.90	423.0
116.90	1020.0
117.90	497.0
118.90	787.0
127.90	508.0
128.80	277.0
129.90	463.0
130.80	180.0
134.80	156.0
136.80	200.0
140.90	1271.0
141.80	220.0
142.90	1489.0
143.90	115.0
144.80	270.0
145.80	210.0
147.90	311.0
153.70	151.0
154.90	320.0
156.90	210.0
158.80	148.0
160.80	169.0
170.80	115.0
171.90	866.0
172.90	1041.0
173.90	96800.0
174.90	6937.0
175.90	93648.0
176.90	5850.0
178.10	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281