

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031822\
 Data File : VW025099.D
 Acq On : 18 Mar 2022 15:45
 Operator : SY/MD
 Sample : N2018-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QA5

Quant Time: Mar 19 00:56:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 19 00:53:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	132841	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	128934	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	68016	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	50449	4.810	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.200%
7) Chloroethane-d5	1.565	69	40680	5.297	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.000%
11) 1,1-Dichloroethene-d2	2.108	63	64505	3.806	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.200%
20) 2-Butanone-d5	3.899	46	72557	57.246	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.500%
24) Chloroform-d	4.349	84	83966	4.827	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.600%
26) 1,2-Dichloroethane-d4	5.034	65	36478	5.016	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	5.050	84	173541	4.640	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.800%
36) 1,2-Dichloropropane-d6	6.069	67	52600	4.891	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.800%
41) Toluene-d8	7.317	98	149768	4.394	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
43) trans-1,3-Dichloroprop...	7.625	79	13971	3.726	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.600%
46) 2-Hexanone-d5	8.092	63	63977	50.025	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.060%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	34273	5.417	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	56074	4.870	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.400%
Target Compounds						
					Qvalue	
3) Chloromethane	1.240	50	762	0.069	ug/L #	80
5) Vinyl chloride	1.311	62	1621	0.139	ug/L #	63
8) Chloroethane	1.507	64	141957	20.045	ug/L #	51
12) 1,1-Dichloroethene	2.114	96	836	0.099	ug/L #	1
14) Carbon disulfide	2.294	76	7333	0.242	ug/L	96
17) Methyl tert-butyl Ether	2.767	73	105011	5.697	ug/L	99
19) 1,1-Dichloroethane	3.191	63	2067	0.119	ug/L	99
22) cis-1,2-Dichloroethene	3.915	96	13580	1.321	ug/L	99
25) Chloroform	4.375	83	1308	0.072	ug/L #	55
27) 1,2-Dichloroethane	5.053	62	783	0.087	ug/L #	71
30) Cyclohexane	4.674	56	955	0.060	ug/L #	90
33) Benzene	5.111	78	3949	0.094	ug/L	100
34) Trichloroethene	5.918	95	10754	0.963	ug/L	98
35) Methylcyclohexane	6.130	83	5791	0.328	ug/L	95
37) 1,2-Dichloropropane	6.069	63	5301	0.550	ug/L #	86
39) cis-1,3-Dichloropropene	6.986	75	1094	0.082	ug/L	87
45) 1,1,2-Trichloroethane	7.786	97	1605	0.249	ug/L #	21
47) Tetrachloroethene	7.979	164	4328	0.551	ug/L	97
49) Dibromochloromethane	7.976	129	4299	0.597	ug/L #	10

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031822\
 Data File : VW025099.D
 Acq On : 18 Mar 2022 15:45
 Operator : SY/MD
 Sample : N2018-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QA5

Quant Time: Mar 19 00:56:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 19 00:53:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


51) Chlorobenzene	8.886	112	5927	0.216	ug/L	96
52) Ethylbenzene	9.014	91	85919	1.851	ug/L	100
53) m,p-xylene	9.143	106	5397	0.302	ug/L	90
54) o-xylene	9.542	106	141308	8.265	ug/L	95
55) Styrene	9.542	104	7063	0.254	ug/L #	1
57) 1,1,2,2-Tetrachloroethane	10.239	83	1779	0.282	ug/L #	40
60) Isopropylbenzene	9.931	105	125430	2.445	ug/L	99
61) 1,2,3-Trichloropropane	10.735	75	3761	0.657	ug/L #	1
62) 1,3,5-Trimethylbenzene	10.538	105	33131	1.423	ug/L	99
63) 1,2,4-Trimethylbenzene	10.915	105	111930	2.715	ug/L	98
64) 1,3-Dichlorobenzene	11.178	146	131413	5.906	ug/L	99
65) 1,4-Dichlorobenzene	11.272	146	266082	11.863	ug/L	100
67) 1,2-Dichlorobenzene	11.641	146	183312	9.298	ug/L	98
68) 1,2-Dibromo-3-chloropr...	12.410	75	5647	5.759	ug/L #	1
71) Naphthalene	13.500	128	357069	17.560	ug/L #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
Data File : VV025099.D
Acq On : 18 Mar 2022 15:45
Operator : SY/MD
Sample : N2018-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QA5

Quant Time: Mar 19 00:56:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 19 00:53:30 2022
Response via : Initial Calibration




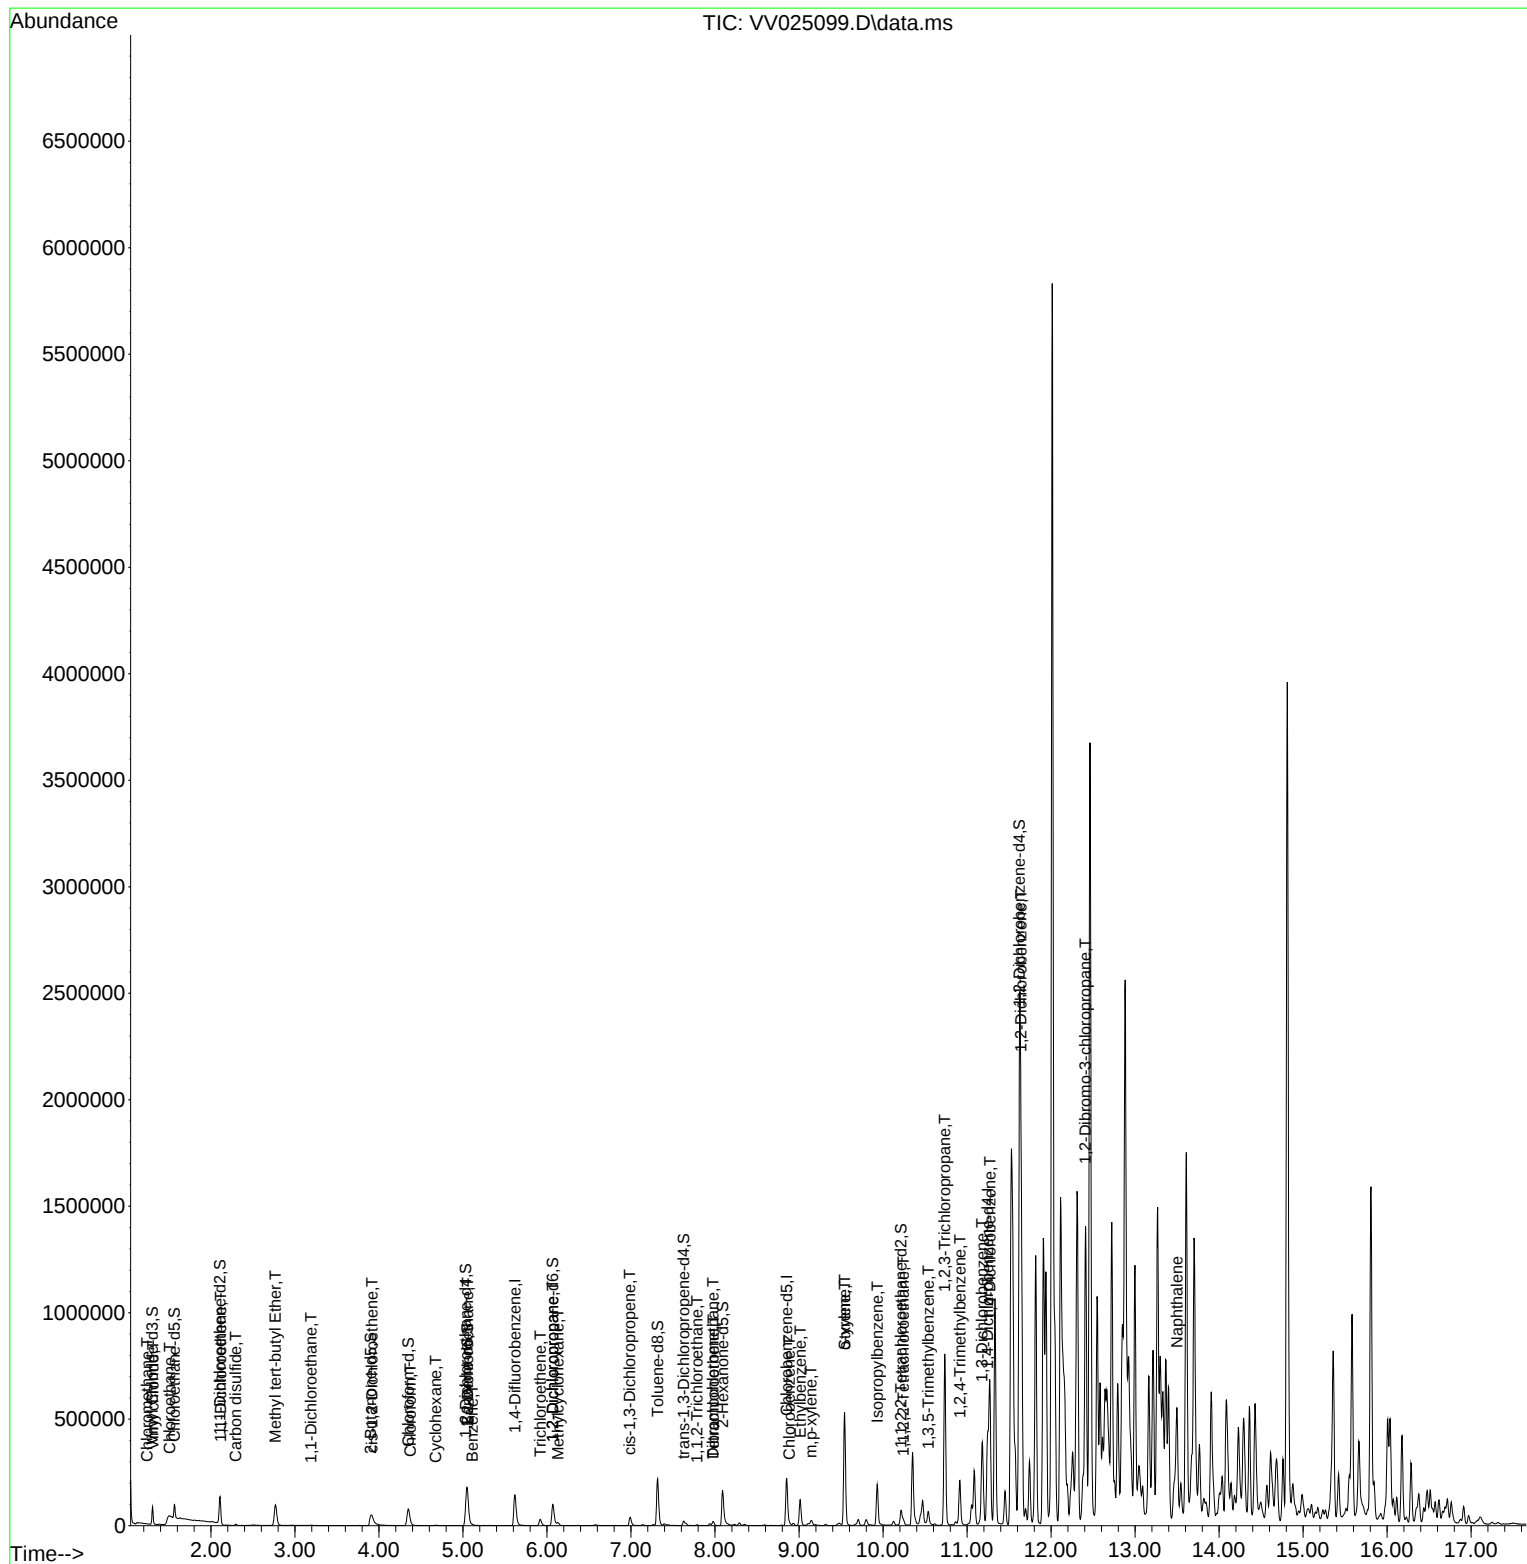


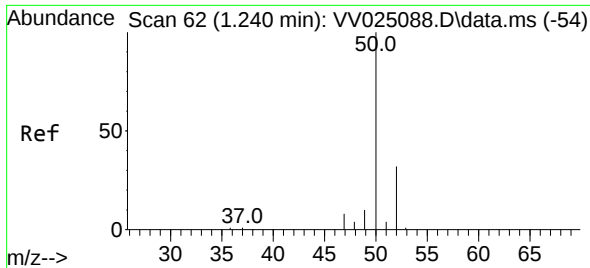

#3
Chloromethane
Concen: 0.069 ug/L
RT: 1.240 min Scan# 61
Delta R.T. 0.000 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45




Instrument :
MSVOA_V
ClientSampleId :
C0QA5


Tgt Ion: 50 Resp: 762
Ion Ratio Lower Upper
50 100
52 44.6 23.2 43.2#

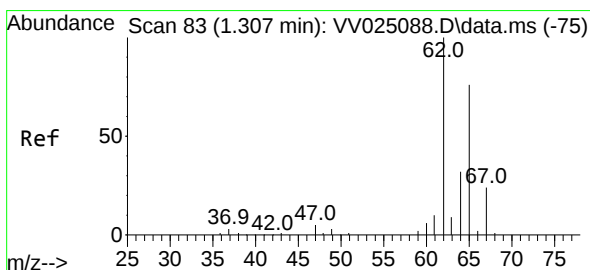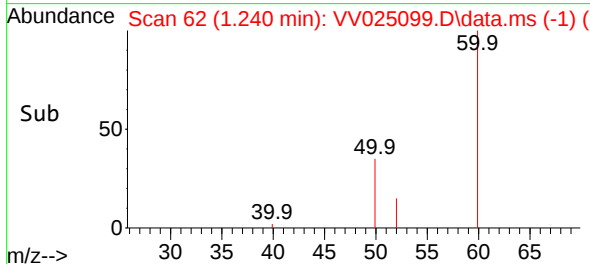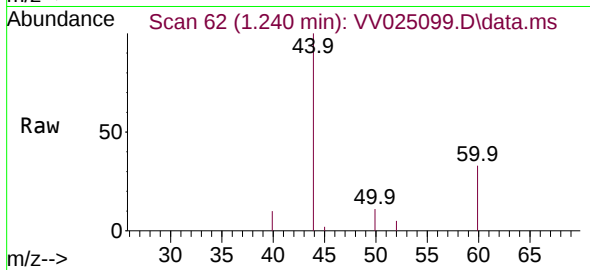

#5
Vinyl chloride
Concen: 0.139 ug/L
RT: 1.311 min Scan# 84
Delta R.T. 0.003 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion: 62 Resp: 1621
Ion Ratio Lower Upper
62 100
64 54.5 23.4 43.4#


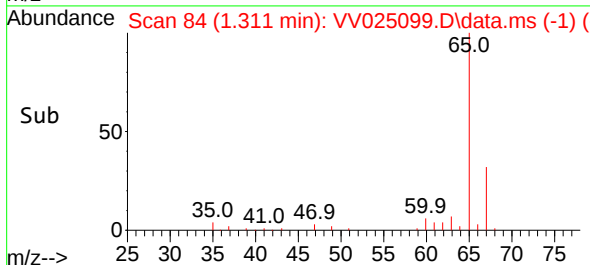

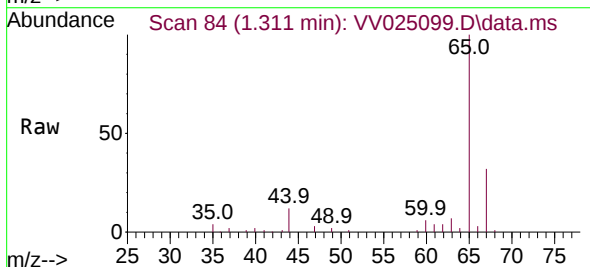


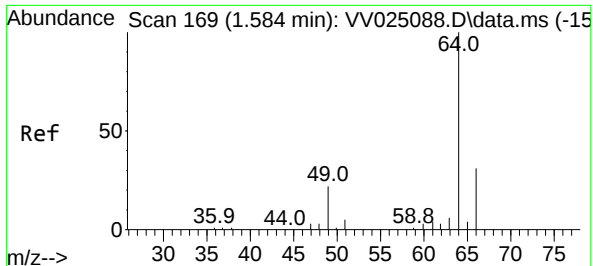

#8
Chloroethane
Concen: 20.045 ug/L
RT: 1.507 min Scan# 14
Delta R.T. -0.077 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45




Instrument :
MSVOA_V
ClientSampleId :
C0QA5


Tgt Ion: 64 Resp: 141957
Ion Ratio Lower Upper
64 100
66 4.7 22.5 41.7#

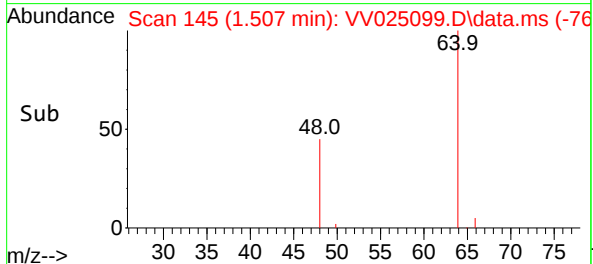

#12
1,1-Dichloroethene
Concen: 0.099 ug/L
RT: 2.114 min Scan# 334
Delta R.T. 0.000 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion: 96 Resp: 836
Ion Ratio Lower Upper
96 100
61 647.6 113.0 209.9#
63 4945.3 82.1 152.5#


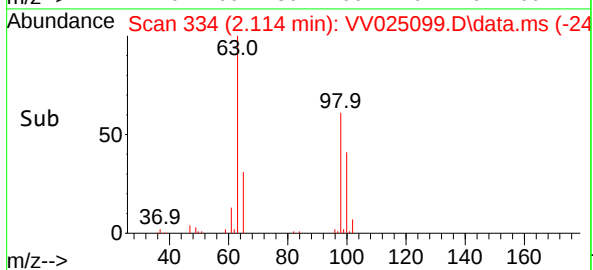

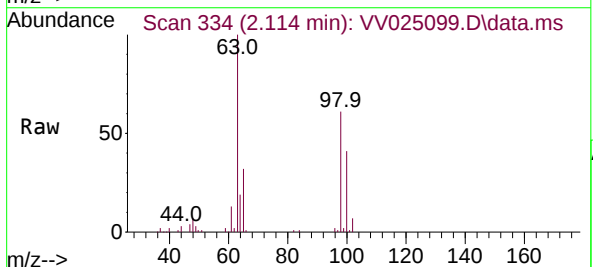




#14
Carbon disulfide
Concen: 0.242 ug/L
RT: 2.294 min Scan# 389
Delta R.T. 0.003 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45




Instrument :
MSVOA_V
ClientSampleId :
C0QA5


Tgt Ion: 76 Resp: 7333
Ion Ratio Lower Upper
76 100
78 10.8 7.4 11.0

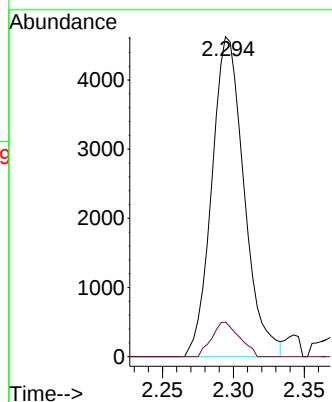

#17
Methyl tert-butyl Ether
Concen: 5.697 ug/L
RT: 2.767 min Scan# 537
Delta R.T. 0.000 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion: 73 Resp: 105011
Ion Ratio Lower Upper
73 100
43 16.5 13.2 19.8
57 21.6 16.7 25.1

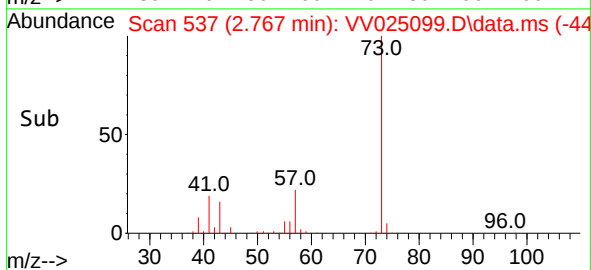



#19

1,1-Dichloroethane

Concen: 0.119 ug/L

RT: 3.191 min Scan# 6

Delta R.T. 0.007 min

Lab File: VV025099.D

Acq: 18 Mar 2022 15:45

Instrument :

MSVOA_V

ClientSampleId :

C0QA5





Tgt Ion: 63 Resp: 2067

Ion Ratio Lower Upper

63 100

65 32.2 22.2 41.2

83 13.6 9.4 17.4

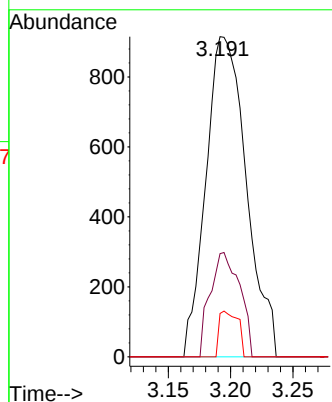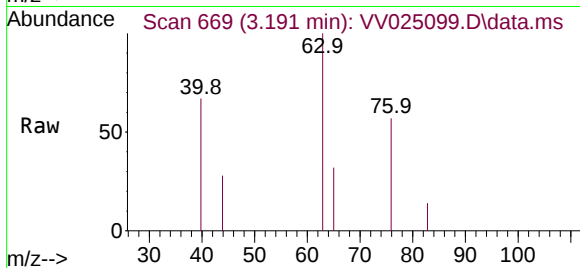

#22

cis-1,2-Dichloroethene

Concen: 1.321 ug/L

RT: 3.915 min Scan# 894

Delta R.T. 0.006 min

Lab File: VV025099.D

Acq: 18 Mar 2022 15:45




Tgt Ion: 96 Resp: 13580


Ion Ratio Lower Upper

96 100

61 112.6 79.7 147.9

68 0.0 0.0 0.0

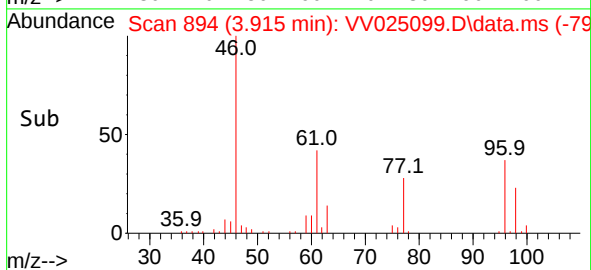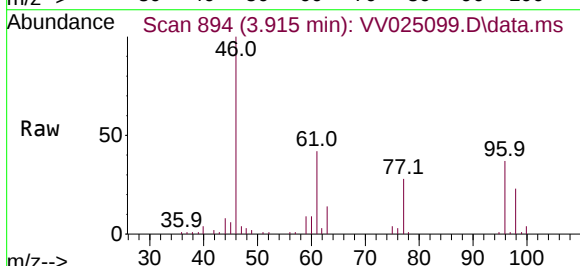

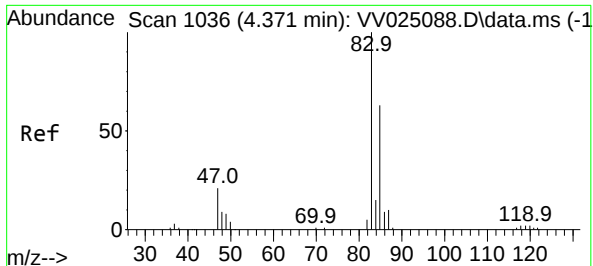

#25

Chloroform

Concen: 0.072 ug/L

RT: 4.375 min Scan# 1

Delta R.T. 0.003 min

Lab File: VV025099.D

Acq: 18 Mar 2022 15:45

Instrument :

MSVOA_V

ClientSampleId :





C0QA5

Tgt Ion: 83 Resp: 1308

Ion Ratio Lower Upper

83 100

85 98.8 44.5 82.7#

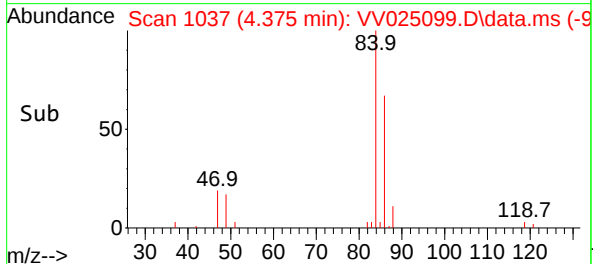

#27

1,2-Dichloroethane

Concen: 0.087 ug/L

RT: 5.053 min Scan# 1248

Delta R.T. -0.074 min

Lab File: VV025099.D




Acq: 18 Mar 2022 15:45


Tgt Ion: 62 Resp: 783

Ion Ratio Lower Upper

62 100

98 0.0 9.0 13.4#


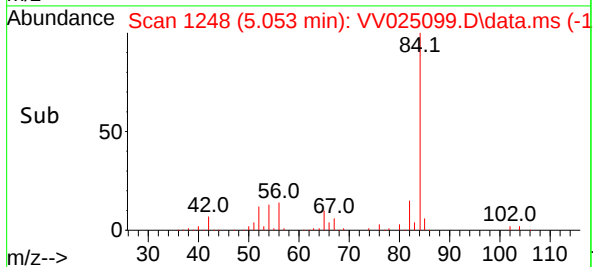

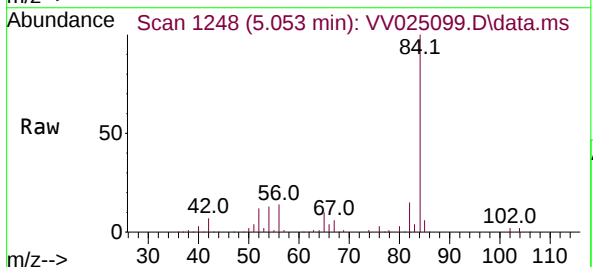




#30
Cyclohexane
Concen: 0.060 ug/L
RT: 4.674 min Scan# 1129
Delta R.T. 0.003 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45




Instrument :
MSVOA_V
ClientSampleId :
C0QA5


Tgt Ion: 56 Resp: 955
Ion Ratio Lower Upper
56 100
69 9.4 24.9 37.3#
84 94.1 75.9 113.9

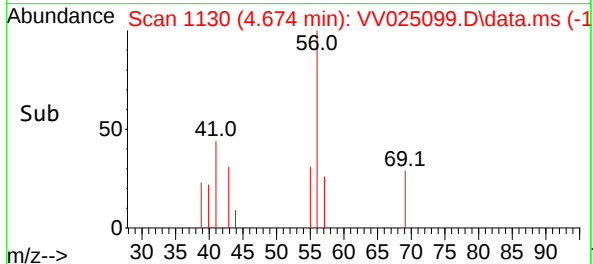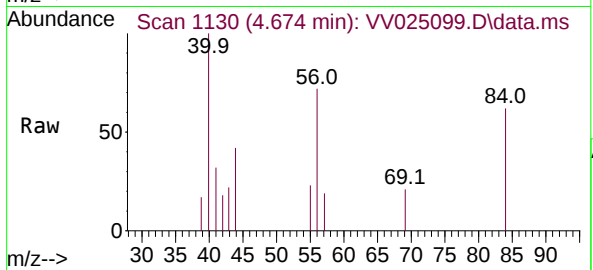

#33
Benzene
Concen: 0.094 ug/L
RT: 5.111 min Scan# 1266
Delta R.T. 0.016 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion: 78 Resp: 3949

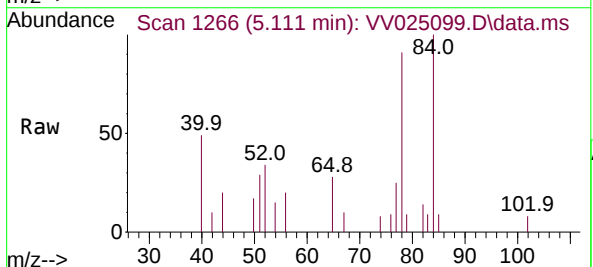




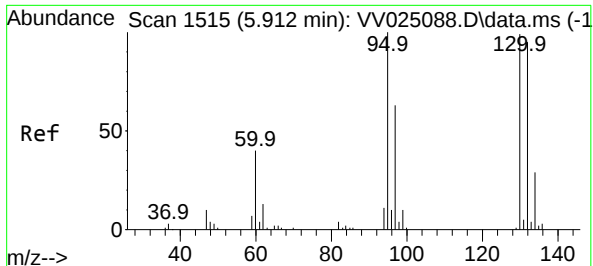


#34
Trichloroethene
Concen: 0.963 ug/L
RT: 5.918 min Scan# 1515
Delta R.T. 0.006 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Instrument :
MSVOA_V
ClientSampleId :
C0QA5

Tgt Ion: 95 Resp: 10754




Ion	Ratio	Lower	Upper
95	100		
97	61.7	44.5	82.7
132	95.3	66.5	123.5
130	99.7	68.0	126.2

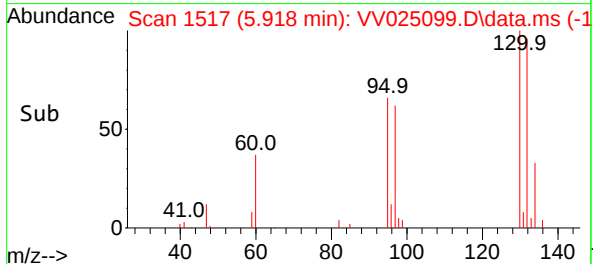


#35
Methylcyclohexane
Concen: 0.328 ug/L
RT: 6.130 min Scan# 1583
Delta R.T. 0.006 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion: 83 Resp: 5791

Ion	Ratio	Lower	Upper
83	100		
55	76.4	55.4	83.0
98	48.3	38.4	57.6

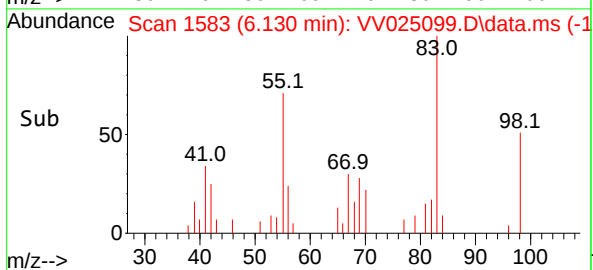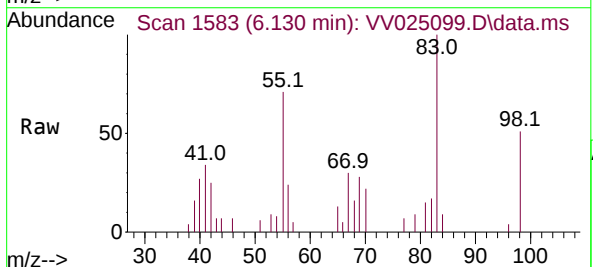

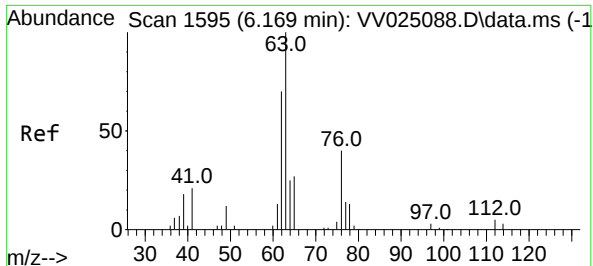

#37

1,2-Dichloropropane

Concen: 0.550 ug/L

RT: 6.069 min Scan# 11

Delta R.T. -0.100 min

Lab File: VV025099.D

Acq: 18 Mar 2022 15:45

Instrument :

MSVOA_V

ClientSampleId :





C0QA5

Tgt Ion: 63 Resp: 5301

Ion Ratio Lower Upper

63 100

112 0.0 3.8 5.6#

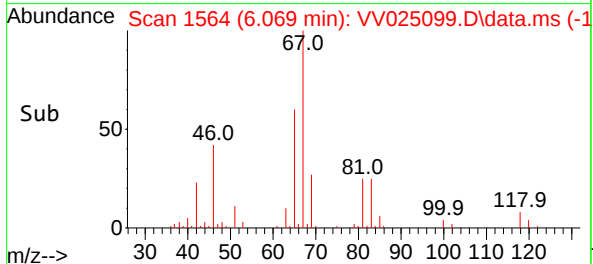

#39

cis-1,3-Dichloropropene

Concen: 0.082 ug/L

RT: 6.986 min Scan# 1849

Delta R.T. -0.039 min

Lab File: VV025099.D




Acq: 18 Mar 2022 15:45


Tgt Ion: 75 Resp: 1094

Ion Ratio Lower Upper

75 100

77 40.3 23.0 42.8


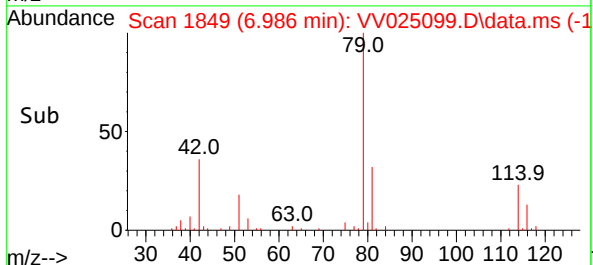

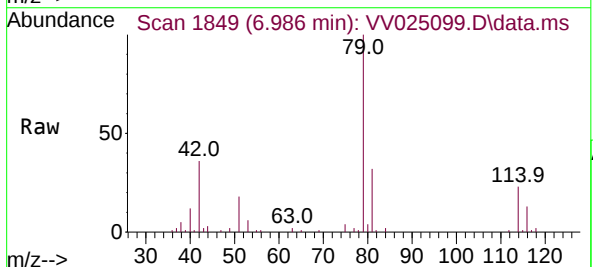




#45
1,1,2-Trichloroethane
Concen: 0.249 ug/L
RT: 7.786 min Scan# 2098
Delta R.T. -0.051 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45




Instrument :
MSVOA_V
ClientSampleId :
C0QA5


Tgt Ion:	97	Resp:	1605
Ion	Ratio	Lower	Upper
97	100		
99	0.0	43.7	81.1#
83	11.9	58.9	109.3#
85	0.0	38.8	72.0#



#47
Tetrachloroethene
Concen: 0.551 ug/L
RT: 7.979 min Scan# 2158
Delta R.T. 0.006 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion:	164	Resp:	4328
Ion	Ratio	Lower	Upper
164	100		
129	100.3	70.3	130.7
131	105.9	69.4	129.0
166	126.1	90.3	167.7

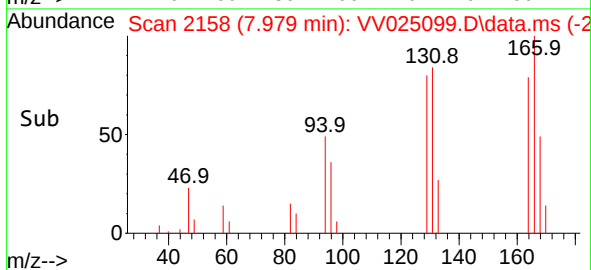



#49

Dibromochloromethane

Concen: 0.597 ug/L

RT: 7.976 min Scan# 2157

Delta R.T. -0.267 min

Lab File: VV025099.D

Acq: 18 Mar 2022 15:45

Instrument :

MSVOA_V

ClientSampleId :





C0QA5

Tgt Ion:129 Resp: 4299

Ion Ratio Lower Upper

129 100

127 0.0 54.9 102.1#



#51

Chlorobenzene

Concen: 0.216 ug/L

RT: 8.886 min Scan# 2440

Delta R.T. 0.006 min

Lab File: VV025099.D

Acq: 18 Mar 2022 15:45




Tgt Ion:112 Resp: 5927


Ion Ratio Lower Upper

112 100

114 32.5 22.5 41.7

77 60.5 45.3 67.9


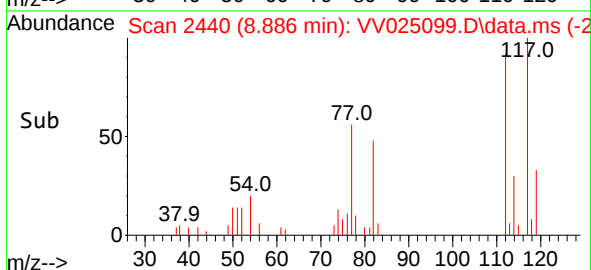






#52
Ethylbenzene
Concen: 1.851 ug/L
RT: 9.014 min Scan# 2479
Delta R.T. 0.003 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45




Instrument :
MSVOA_V
ClientSampleId :
C0QA5


Tgt Ion: 91 Resp: 85919
Ion Ratio Lower Upper
91 100
106 31.3 21.9 40.7

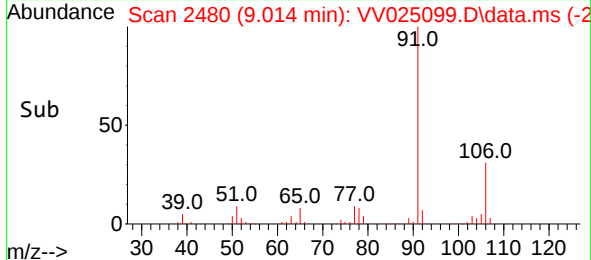

#53
m,p-xylene
Concen: 0.302 ug/L
RT: 9.143 min Scan# 2520
Delta R.T. 0.007 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion: 106 Resp: 5397
Ion Ratio Lower Upper
106 100
91 189.7 143.4 266.4


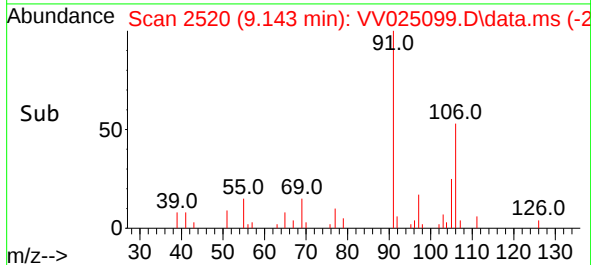

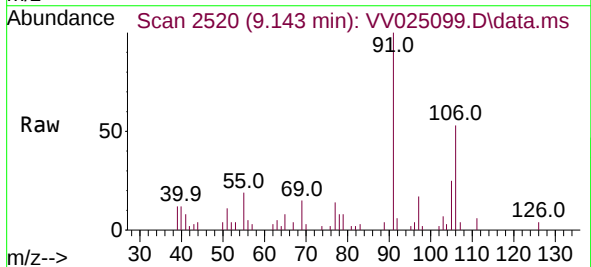




#54
o-xylene
Concen: 8.265 ug/L
RT: 9.542 min Scan# 2644
Delta R.T. 0.000 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45




Instrument :
MSVOA_V
ClientSampleId :
C0QA5


Tgt Ion:106 Resp: 141308
Ion Ratio Lower Upper
106 100
91 217.5 146.7 272.5



#55
Styrene
Concen: 0.254 ug/L
RT: 9.542 min Scan# 2644
Delta R.T. -0.016 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion:104 Resp: 7063
Ion Ratio Lower Upper
104 100
78 286.7 30.2 56.2#



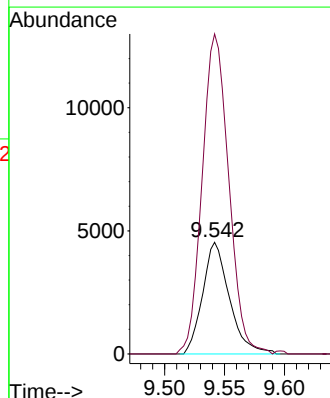
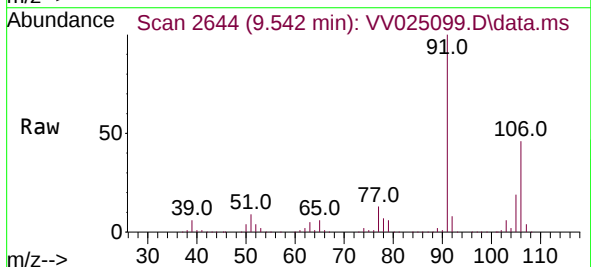




#57
1,1,2,2-Tetrachloroethane
Concen: 0.282 ug/L
RT: 10.239 min Scan# 2861
Delta R.T. 0.000 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45




Instrument :
MSVOA_V
ClientSampleId :
C0QA5


Tgt Ion: 83 Resp: 1779
Ion Ratio Lower Upper
83 100
85 12.3 43.9 81.5#
131 0.0 7.5 11.3#

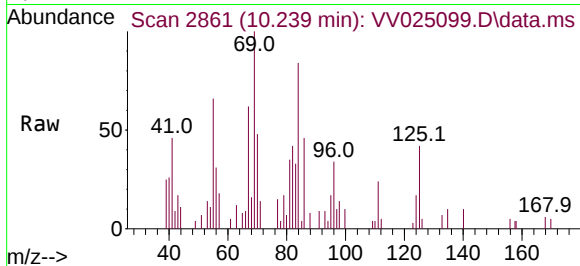

#60
Isopropylbenzene
Concen: 2.445 ug/L
RT: 9.931 min Scan# 2765
Delta R.T. 0.003 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion: 105 Resp: 125430
Ion Ratio Lower Upper
105 100
120 25.4 20.7 31.1
77 15.3 12.2 18.2


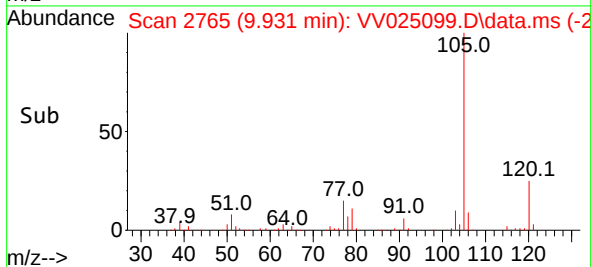

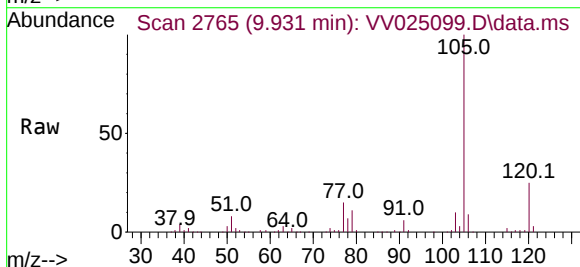




#61
 1,2,3-Trichloropropane
 Concen: 0.657 ug/L
 RT: 10.735 min Scan# 3015
 Delta R.T. 0.463 min
 Lab File: VV025099.D
 Acq: 18 Mar 2022 15:45




Instrument :
 MSVOA_V
 ClientSampleId :
 C0QA5


Tgt Ion: 75 Resp: 3761
 Ion Ratio Lower Upper
 75 100
 77 1487.7 25.7 38.5#
 110 0.0 31.2 46.8#

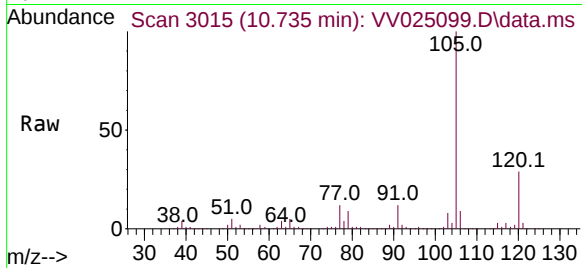

#62
 1,3,5-Trimethylbenzene
 Concen: 1.423 ug/L
 RT: 10.538 min Scan# 2954
 Delta R.T. 0.003 min
 Lab File: VV025099.D
 Acq: 18 Mar 2022 15:45

Tgt Ion: 105 Resp: 33131
 Ion Ratio Lower Upper
 105 100
 120 48.9 38.5 57.7




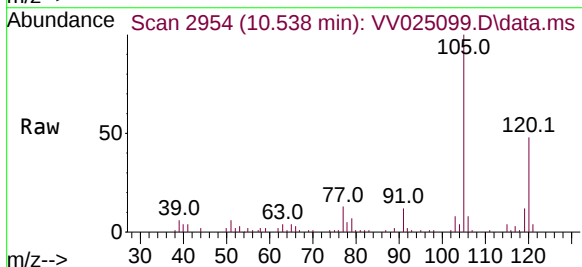




#63
1,2,4-Trimethylbenzene
Concen: 2.715 ug/L
RT: 10.915 min Scan# 3070
Delta R.T. 0.003 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45




Instrument :
MSVOA_V
ClientSampleId :
C0QA5


Tgt Ion:105 Resp: 111930
Ion Ratio Lower Upper
105 100
120 46.0 35.8 53.8



#64
1,3-Dichlorobenzene
Concen: 5.906 ug/L
RT: 11.178 min Scan# 3153
Delta R.T. 0.000 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion:146 Resp: 131413
Ion Ratio Lower Upper
146 100
111 42.2 29.2 54.2
148 63.0 43.8 81.4


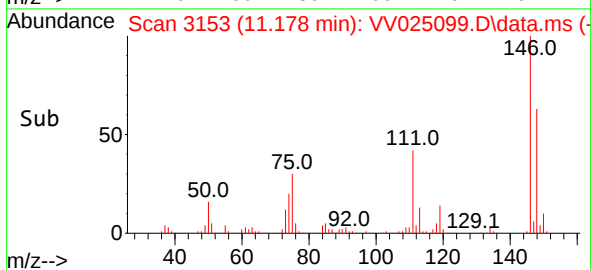

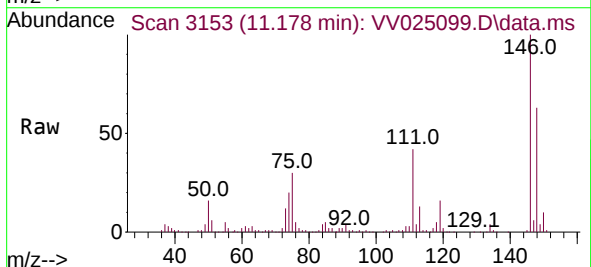




#65
1,4-Dichlorobenzene
Concen: 11.863 ug/L
RT: 11.272 min Scan# 3182
Delta R.T. 0.000 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45




Instrument :
MSVOA_V
ClientSampleId :
C0QA5


Tgt Ion:146 Resp: 266082
Ion Ratio Lower Upper
146 100
111 39.8 28.2 52.4
148 62.8 43.8 81.4



#67
1,2-Dichlorobenzene
Concen: 9.298 ug/L
RT: 11.641 min Scan# 3297
Delta R.T. 0.000 min
Lab File: VV025099.D
Acq: 18 Mar 2022 15:45

Tgt Ion:146 Resp: 183312
Ion Ratio Lower Upper
146 100
111 44.2 35.5 53.3
148 64.2 49.7 74.5


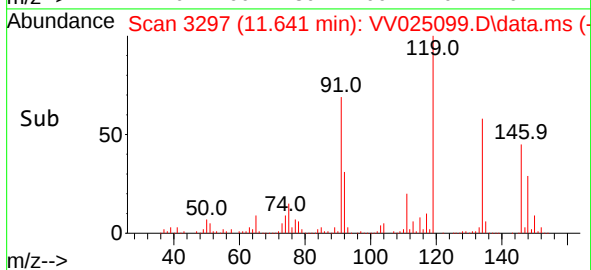

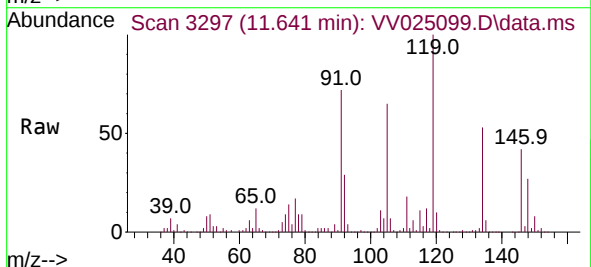




#68
 1,2-Dibromo-3-chloropropane
 Concen: 5.759 ug/L
 RT: 12.410 min Scan# 3536
 Delta R.T. -0.016 min
 Lab File: VV025099.D
 Acq: 18 Mar 2022 15:45

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QA5

Tgt Ion: 75 Resp: 5647
 Ion Ratio Lower Upper
 75 100
 155 0.0 65.9 98.9#
 157 0.0 89.7 134.5#

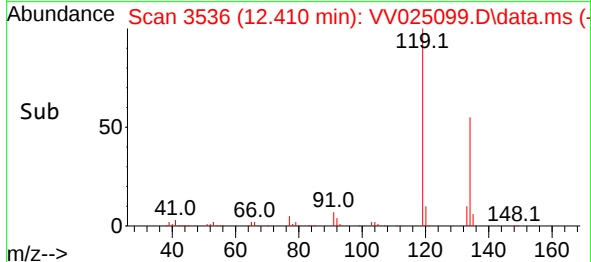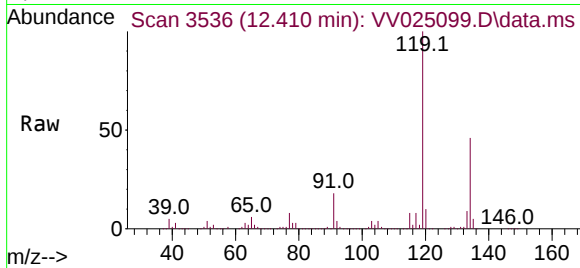

#71
 Naphthalene
 Concen: 17.560 ug/L
 RT: 13.500 min Scan# 3875
 Delta R.T. 0.000 min
 Lab File: VV025099.D
 Acq: 18 Mar 2022 15:45

Tgt Ion: 128 Resp: 357069
 Ion Ratio Lower Upper
 128 100
 129 16.1 8.5 12.7#
 127 13.4 9.8 14.8

