




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
 Data File : VV025093.D
 Acq On : 18 Mar 2022 12:42
 Operator : SY/MD
 Sample : N1941-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLF3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

Quant Time: Mar 19 00:55:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 19 00:53:30 2022
 Response via : Initial Calibration

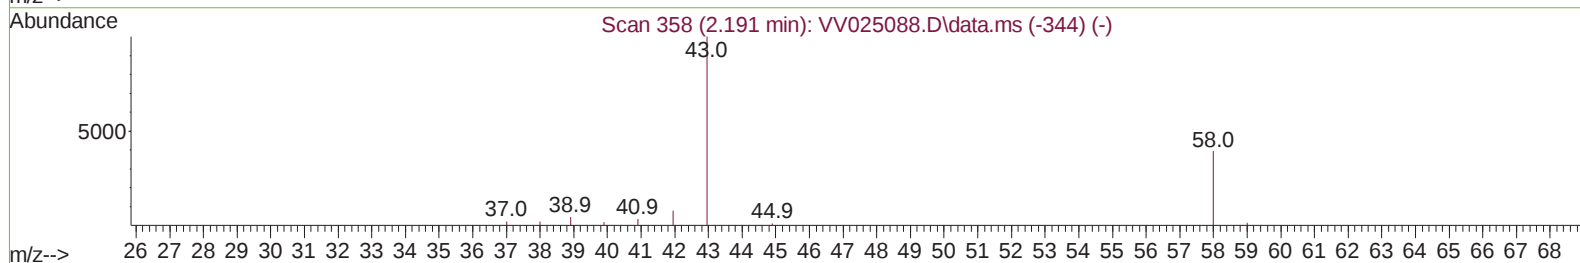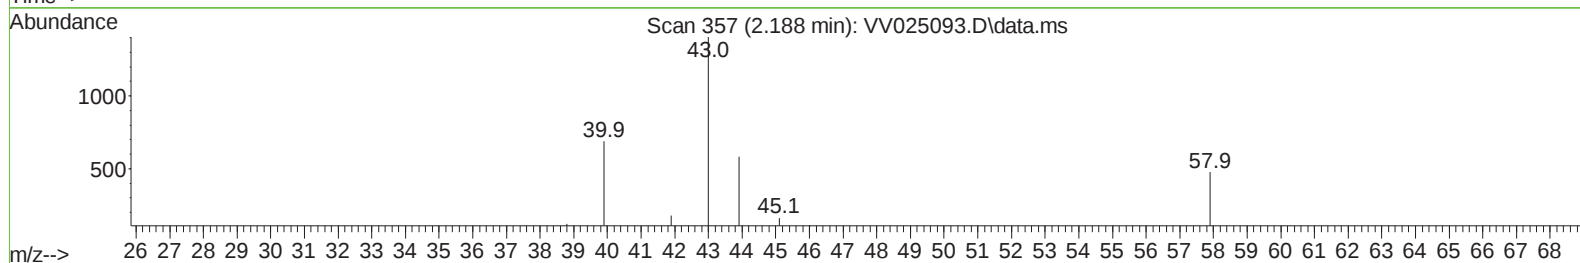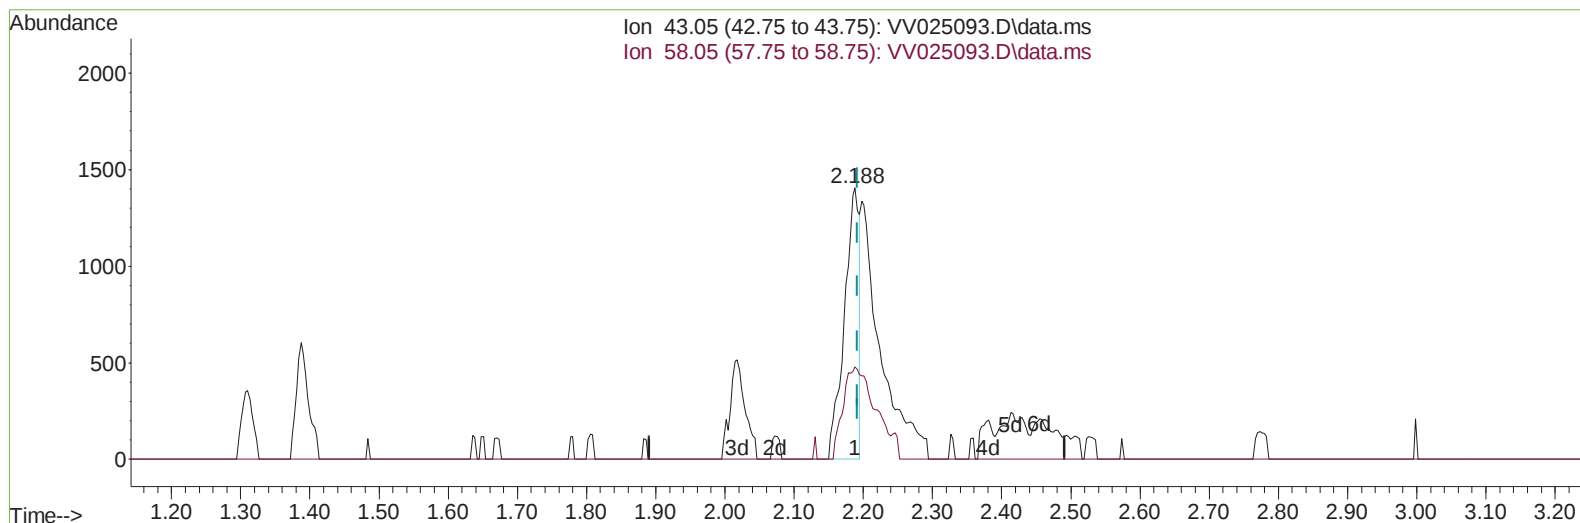

TIC: VV025093.D\data.ms

(13) Acetone (T)

2.188min (-0.003) 2.25 ug/L

response 2114

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.10	71.62#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
 Data File : VV025093.D
 Acq On : 18 Mar 2022 12:42
 Operator : SY/MD
 Sample : N1941-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLF3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

Quant Time: Mar 19 00:55:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 19 00:53:30 2022
 Response via : Initial Calibration

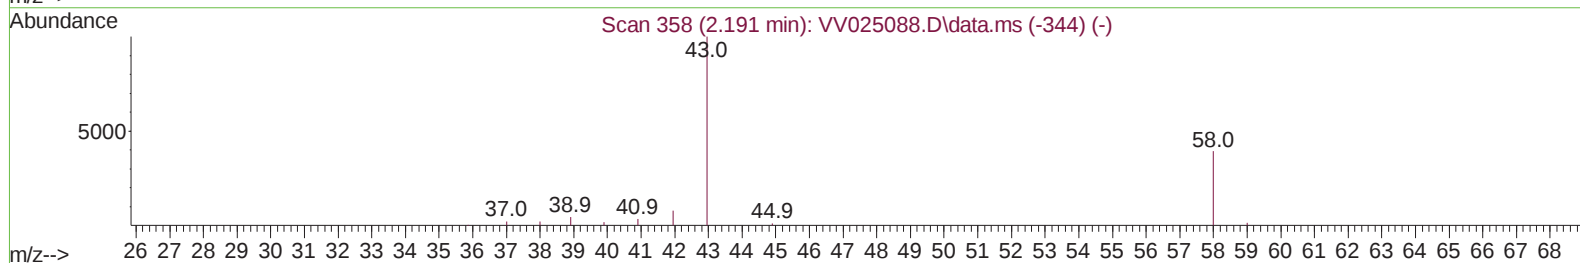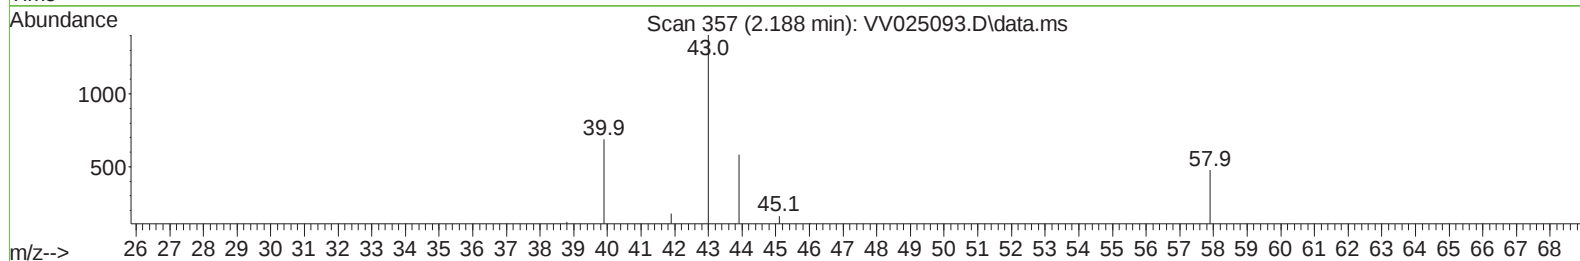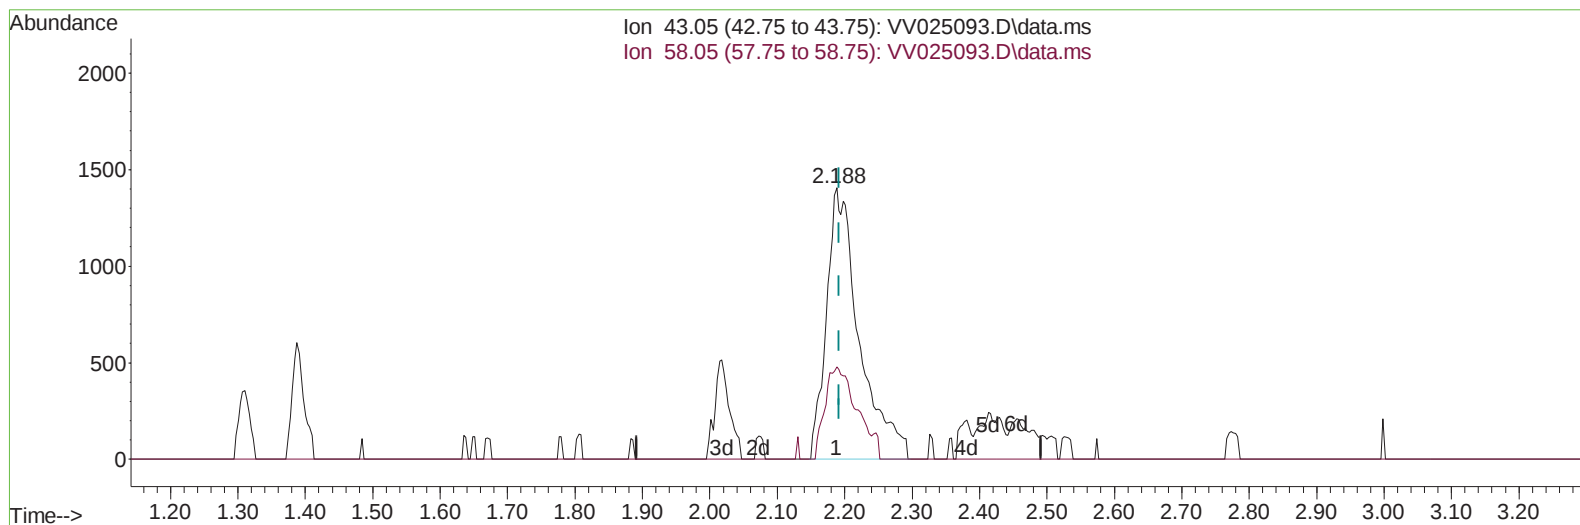

TIC: VV025093.D\data.ms

(13) Acetone (T)

2.188min (-0.003) 5.05 ug/L m

response 4736

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.10	31.97
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
 Data File : VV025093.D
 Acq On : 18 Mar 2022 12:42
 Operator : SY/MD
 Sample : N1941-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JNLF3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/28/2022
 Supervised By :Mahesh Dadoda 03/28/2022

Quant Time: Mar 19 00:55:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 19 00:53:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	146935	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	139931	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60777	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	54164	4.669	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	93.400%	
7) Chloroethane-d5	1.571	69	43044	5.067	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	101.400%	
11) 1,1-Dichloroethene-d2	2.111	63	68444	3.651	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	73.000%	
20) 2-Butanone-d5	3.899	46	76909	54.859	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	109.720%	
24) Chloroform-d	4.352	84	90080	4.682	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	93.600%	
26) 1,2-Dichloroethane-d4	5.037	65	38661	4.806	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	96.200%	
32) Benzene-d6	5.050	84	185221	4.563	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	91.200%	
36) 1,2-Dichloropropane-d6	6.072	67	55425	4.748	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	95.000%	
41) Toluene-d8	7.316	98	159646	4.315	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	86.400%	
43) trans-1,3-Dichloroprop...	7.625	79	17444	4.287	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	85.800%	
46) 2-Hexanone-d5	8.091	63	60039	43.256	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	86.520%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31020	4.517	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	90.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	50516	4.910	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	98.200%	
Target Compounds						
3) Chloromethane	1.243	50	2190	0.179	ug/L	90
13) Acetone	2.188	43	4736m	5.051	ug/L	
25) Chloroform	4.384	83	1598	0.080	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
Data File : VV025093.D
Acq On : 18 Mar 2022 12:42
Operator : SY/MD
Sample : N1941-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JNLF3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/28/2022
Supervised By :Mahesh Dadoda 03/28/2022

Quant Time: Mar 19 00:55:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 19 00:53:30 2022
Response via : Initial Calibration

