

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
 Data File : VV025089.D
 Acq On : 18 Mar 2022 10:52
 Operator : SY/MD
 Sample : VV0318WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK319

Quant Time: Mar 19 00:54:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 19 00:53:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	145005	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	137352	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	59023	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	53284	4.654	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.000%
7) Chloroethane-d5	1.568	69	41187	4.913	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.200%
11) 1,1-Dichloroethene-d2	2.105	63	67235	3.634	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.600%
20) 2-Butanone-d5	3.915	46	66559	48.108	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.220%
24) Chloroform-d	4.346	84	87933	4.631	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
26) 1,2-Dichloroethane-d4	5.031	65	38621	4.865	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.400%
32) Benzene-d6	5.047	84	184420	4.629	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
36) 1,2-Dichloropropane-d6	6.069	67	53618	4.680	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.600%
41) Toluene-d8	7.313	98	157344	4.333	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
43) trans-1,3-Dichloroprop...	7.625	79	16526	4.138	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.800%
46) 2-Hexanone-d5	8.092	63	60020	44.055	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.100%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	31021	4.602	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	48501	4.854	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.000%
Target Compounds					Qvalue	
25) Chloroform	4.375	83	2689	0.137	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
Data File : VV025089.D
Acq On : 18 Mar 2022 10:52
Operator : SY/MD
Sample : VV0318WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK319

Quant Time: Mar 19 00:54:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 19 00:53:30 2022
Response via : Initial Calibration

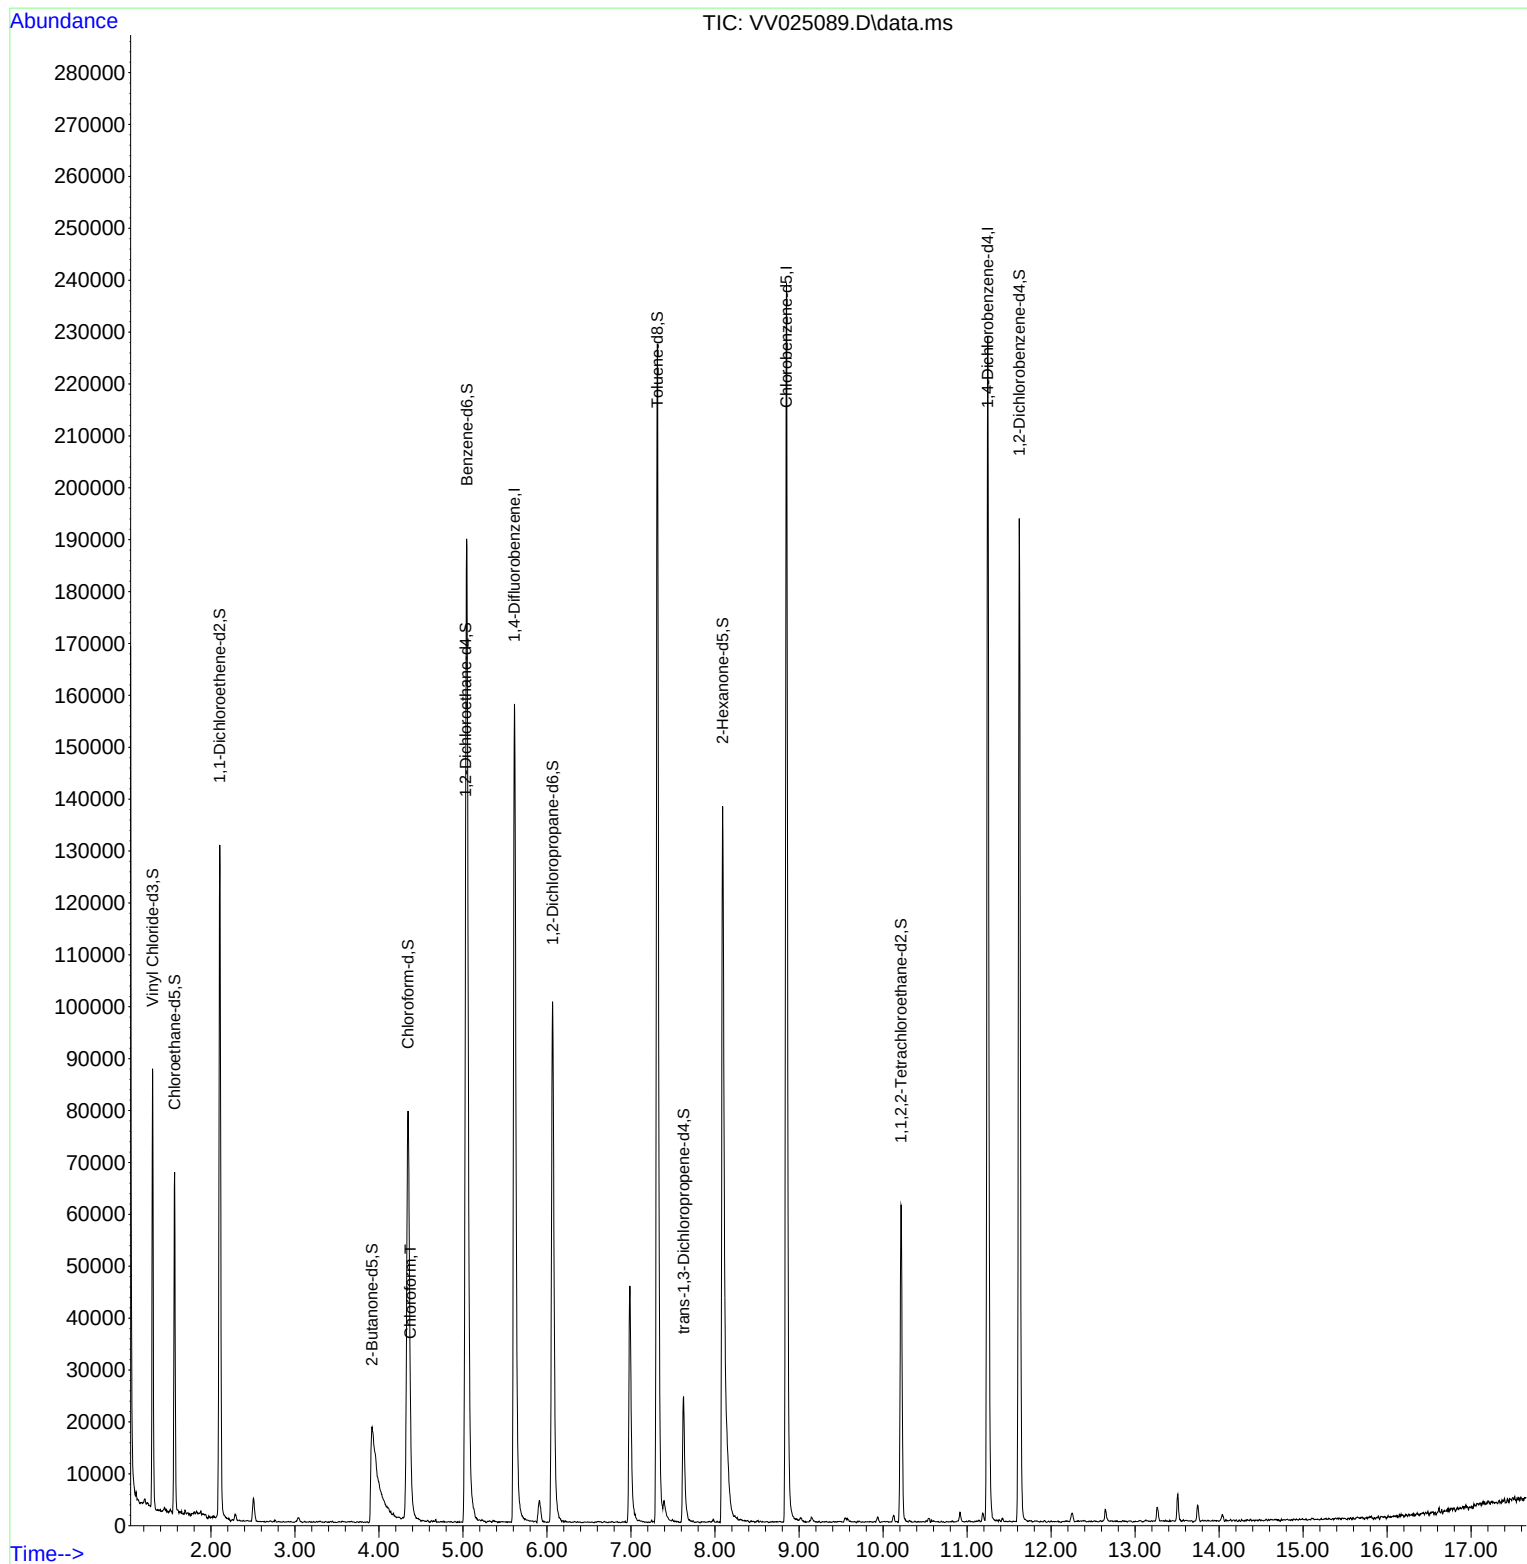

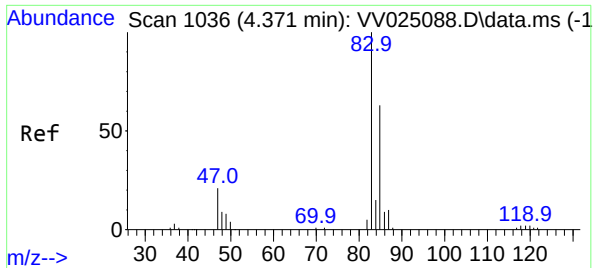

#25
 Chloroform
 Concen: 0.137 ug/L
 RT: 4.375 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VV025089.D
 Acq: 18 Mar 2022 10:52

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK319

Tgt Ion: 83 Resp: 2689
 Ion Ratio Lower Upper
 83 100
 85 70.5 44.5 82.7

