

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
 Data File : VV025089.D
 Acq On : 18 Mar 2022 10:52
 Operator : SY/MD
 Sample : VV0318WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK319

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	85091	87261	18.75%	2.372%
2	1.568	156	164	174	rBV	65778	71932	15.46%	1.956%
3	2.105	317	331	347	rBV	129590	184578	39.66%	5.018%
4	2.507	448	456	466	rBV	4502	7067	1.52%	0.192%
5	3.918	882	895	943	rBV2	18498	104397	22.43%	2.838%
6	4.346	1013	1028	1058	rVB	78491	199299	42.83%	5.419%
7	5.043	1229	1245	1279	rBV2	189527	465356	100.00%	12.652%
8	5.613	1411	1422	1459	rBV	157684	327332	70.34%	8.900%
9	5.908	1505	1514	1526	rBV7	4231	8986	1.93%	0.244%
10	6.066	1548	1563	1594	rBV	100305	210105	45.15%	5.712%
11	6.985	1837	1849	1867	rBV	45630	85638	18.40%	2.328%
12	7.313	1940	1951	1971	rBV	227059	397363	85.39%	10.804%
13	7.394	1971	1976	2004	rVB3	3974	9047	1.94%	0.246%
14	7.625	2037	2048	2068	rBV2	24259	45300	9.73%	1.232%
15	8.092	2183	2193	2233	rBV	137997	312891	67.24%	8.507%
16	8.850	2418	2429	2458	rBV	238691	392565	84.36%	10.673%
17	10.214	2842	2853	2869	rBV	61205	97016	20.85%	2.638%
18	11.246	3163	3174	3202	rVB	228277	354030	76.08%	9.626%
19	11.622	3280	3291	3311	rBV	193243	305866	65.73%	8.316%
20	13.509	3868	3878	3886	rBV	5238	7236	1.55%	0.197%
21	13.744	3943	3951	3961	rVB5	3206	4767	1.02%	0.130%




Sum of corrected areas: 3678032

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
Data File : VV025089.D
Acq On : 18 Mar 2022 10:52
Operator : SY/MD
Sample : VV0318WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

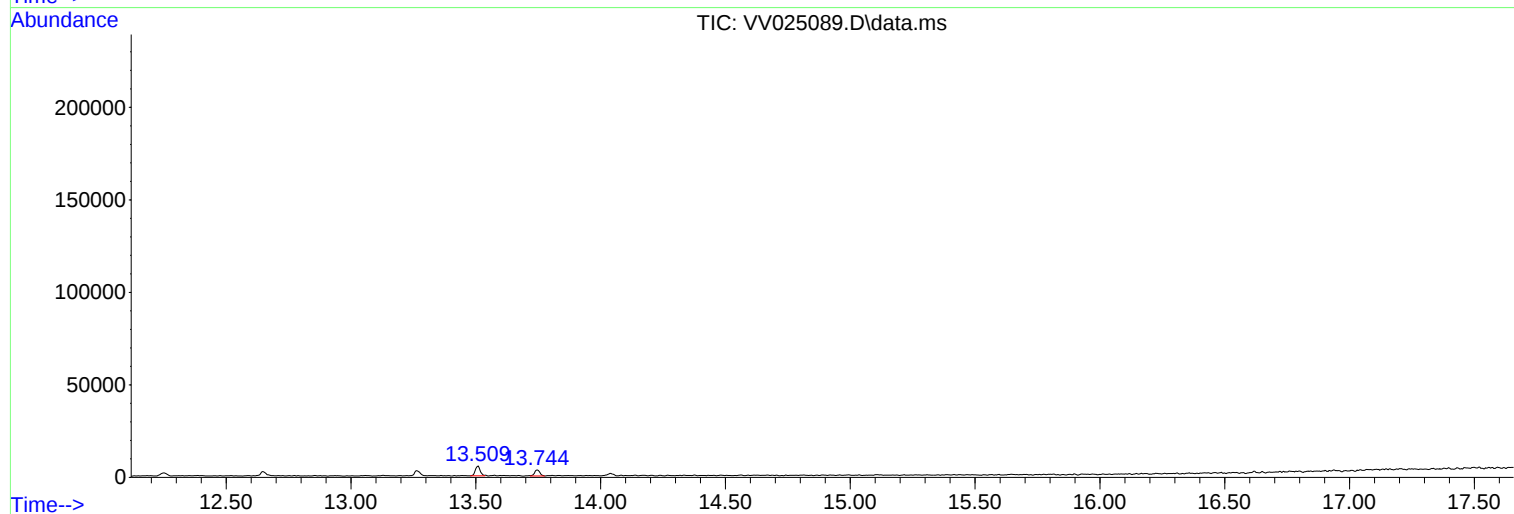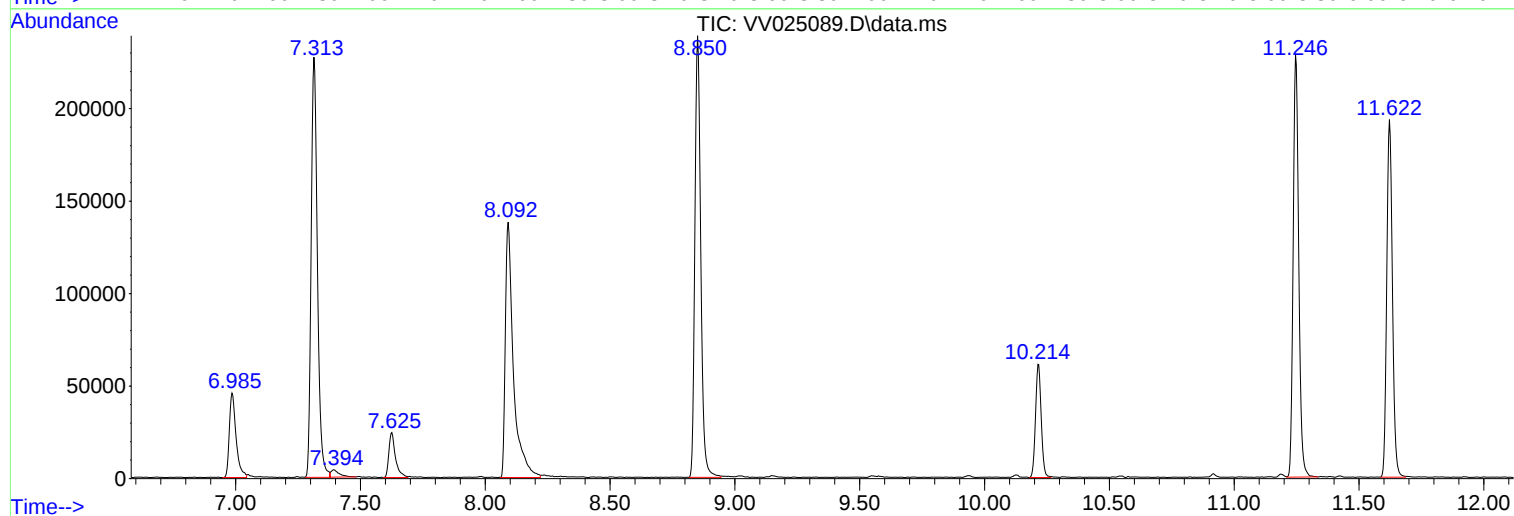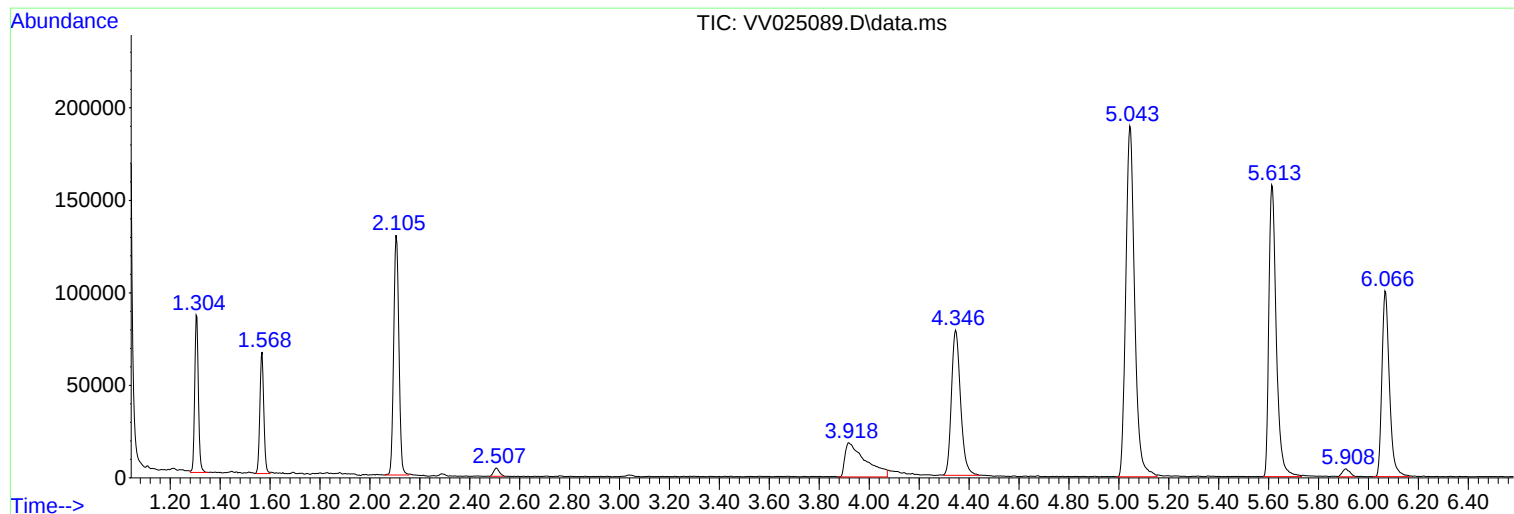

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
Data File : VV025089.D
Acq On : 18 Mar 2022 10:52
Operator : SY/MD
Sample : VV0318WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
Data File : VV025089.D
Acq On : 18 Mar 2022 10:52
Operator : SY/MD
Sample : VV0318WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK319

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc