

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
 Data File : VV025094.D
 Acq On : 18 Mar 2022 13:48
 Operator : SY/MD
 Sample : N1858-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	88144	88461	18.69%	2.391%
2	1.568	156	164	177	rBV	67527	76260	16.11%	2.061%
3	2.108	320	332	348	rBV	131799	189500	40.03%	5.121%
4	2.507	445	456	471	rVB	10278	16667	3.52%	0.450%
5	3.905	878	891	915	rBV2	26237	100290	21.19%	2.710%
6	4.346	1012	1028	1053	rBV	81663	206477	43.62%	5.580%
7	5.044	1230	1245	1274	rBV2	192418	473354	100.00%	12.792%
8	5.613	1408	1422	1455	rBV	153122	319745	67.55%	8.641%
9	5.912	1502	1515	1526	rBV5	4301	8471	1.79%	0.229%
10	6.066	1551	1563	1589	rBV	104210	215490	45.52%	5.824%
11	6.986	1838	1849	1873	rBV	45922	87024	18.38%	2.352%
12	7.314	1940	1951	1970	rBV	224688	401121	84.74%	10.840%
13	7.622	2038	2047	2070	rBV	24498	45586	9.63%	1.232%
14	7.931	2135	2143	2155	rVB4	3517	6630	1.40%	0.179%
15	8.088	2182	2192	2235	rBV	151775	316235	66.81%	8.546%
16	8.850	2415	2429	2453	rBV	235233	387096	81.78%	10.461%
17	10.214	2840	2853	2869	rBV	61669	96454	20.38%	2.607%
18	10.378	2894	2904	2915	rBV3	5401	8605	1.82%	0.233%
19	11.246	3164	3174	3196	rBV	225477	344332	72.74%	9.306%
20	11.622	3280	3291	3308	rBV	197028	306373	64.72%	8.280%
21	12.249	3475	3486	3497	rVB	3937	6133	1.30%	0.166%




Sum of corrected areas: 3700304

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
Data File : VV025094.D
Acq On : 18 Mar 2022 13:48
Operator : SY/MD
Sample : N1858-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

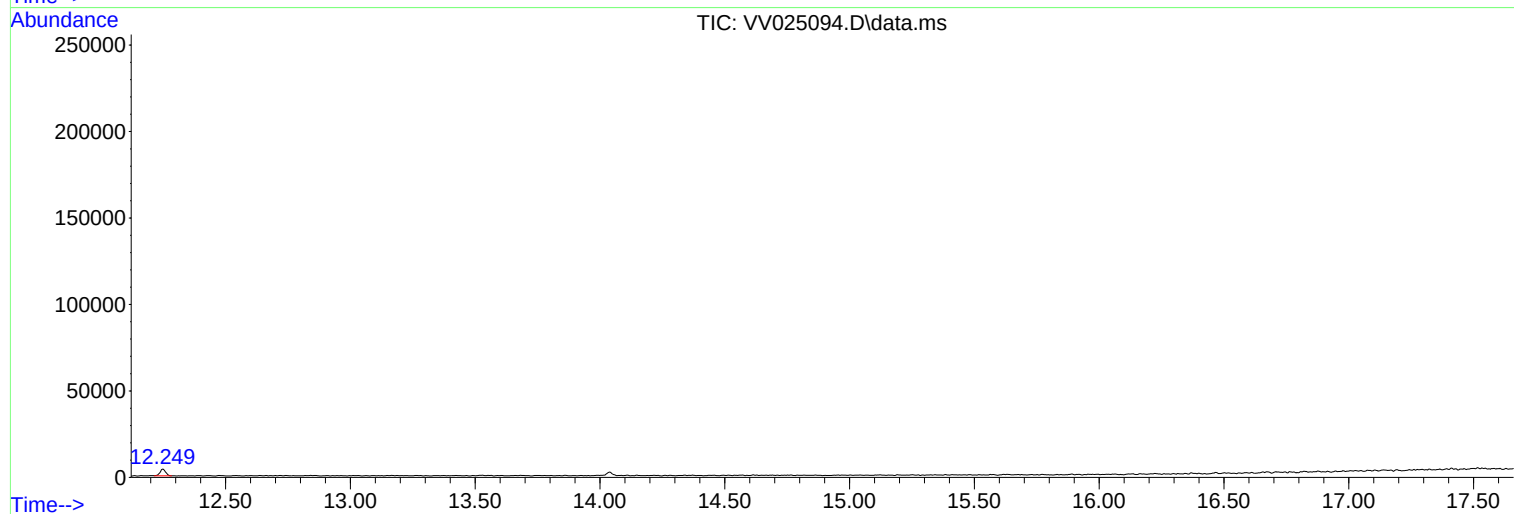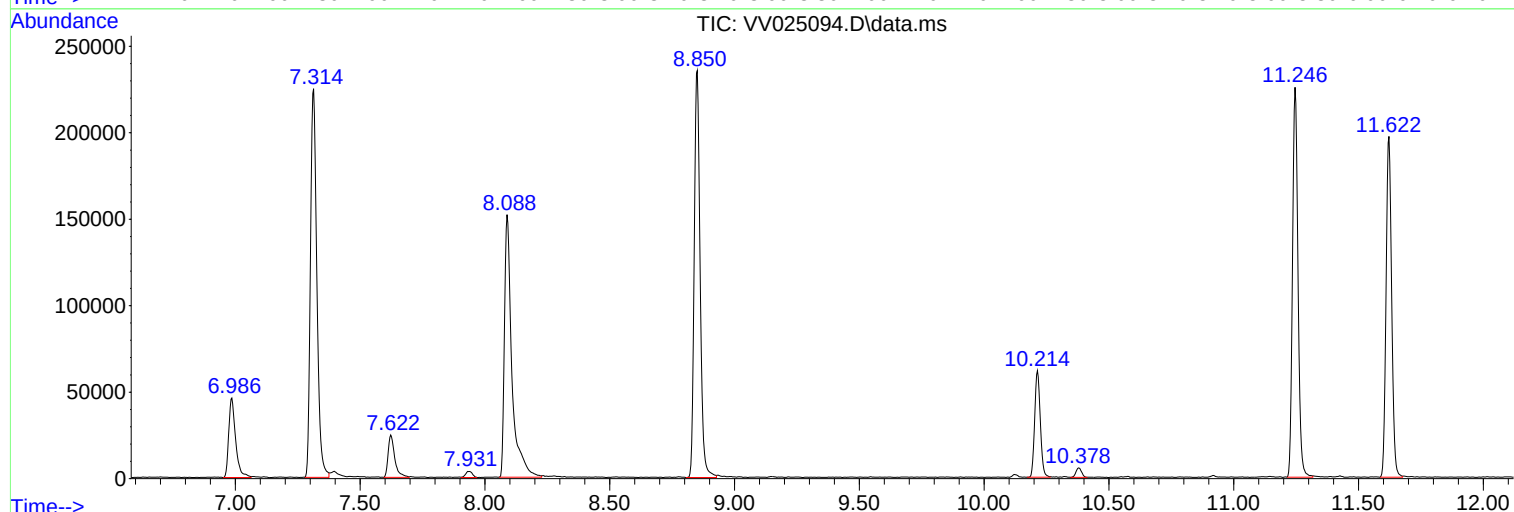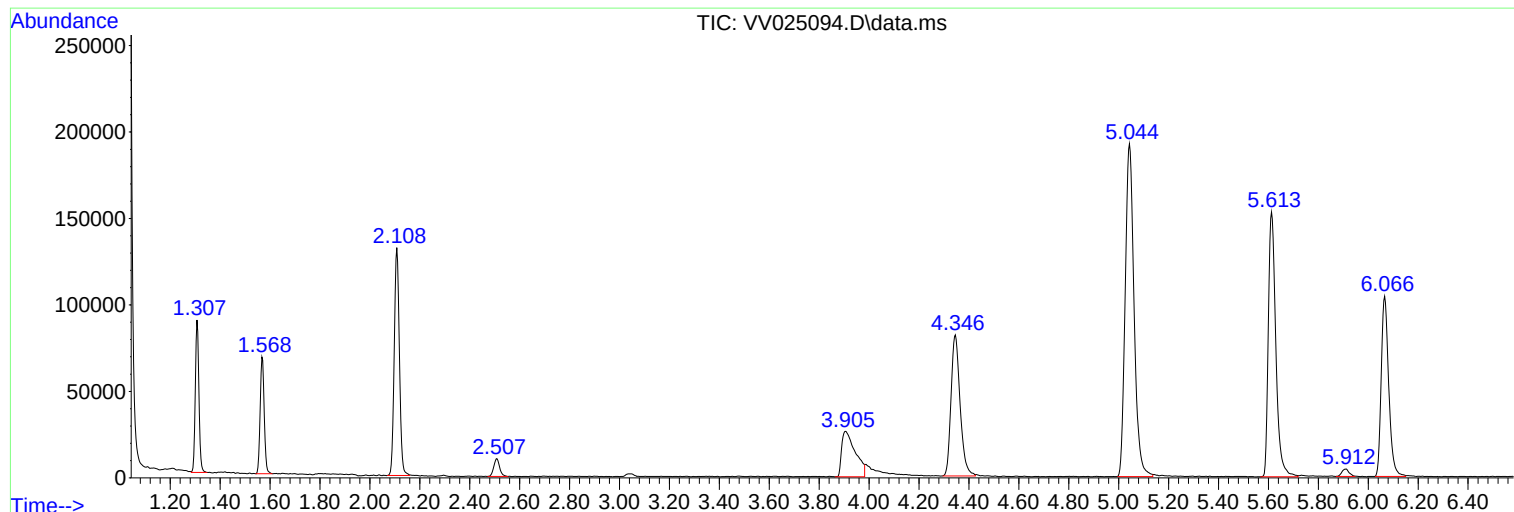

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
Data File : VV025094.D
Acq On : 18 Mar 2022 13:48
Operator : SY/MD
Sample : N1858-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031822\
Data File : VV025094.D
Acq On : 18 Mar 2022 13:48
Operator : SY/MD
Sample : N1858-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc