

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031824\
 Data File : VV034692.D
 Acq On : 18 Mar 2024 12:05
 Operator : SY/MD
 Sample : P1715-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 19 02:20:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 06 04:17:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	11576	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.800	117	10478	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	5205	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	6404	0.516	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	104.000%
4) 1,2-Dichloroethane-d4	4.969	65	4086	0.531	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	106.000%
7) 1,2-Dichloropropane-d6	5.995	67	4399	0.540	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.000%
8) Toluene-d8	7.253	98	12271	0.509	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2821	0.483	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	96.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.185	75	31	0.033	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031824\
Data File : VV034692.D
Acq On : 18 Mar 2024 12:05
Operator : SY/MD
Sample : P1715-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 19 02:20:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 06 04:17:25 2024
Response via : Initial Calibration

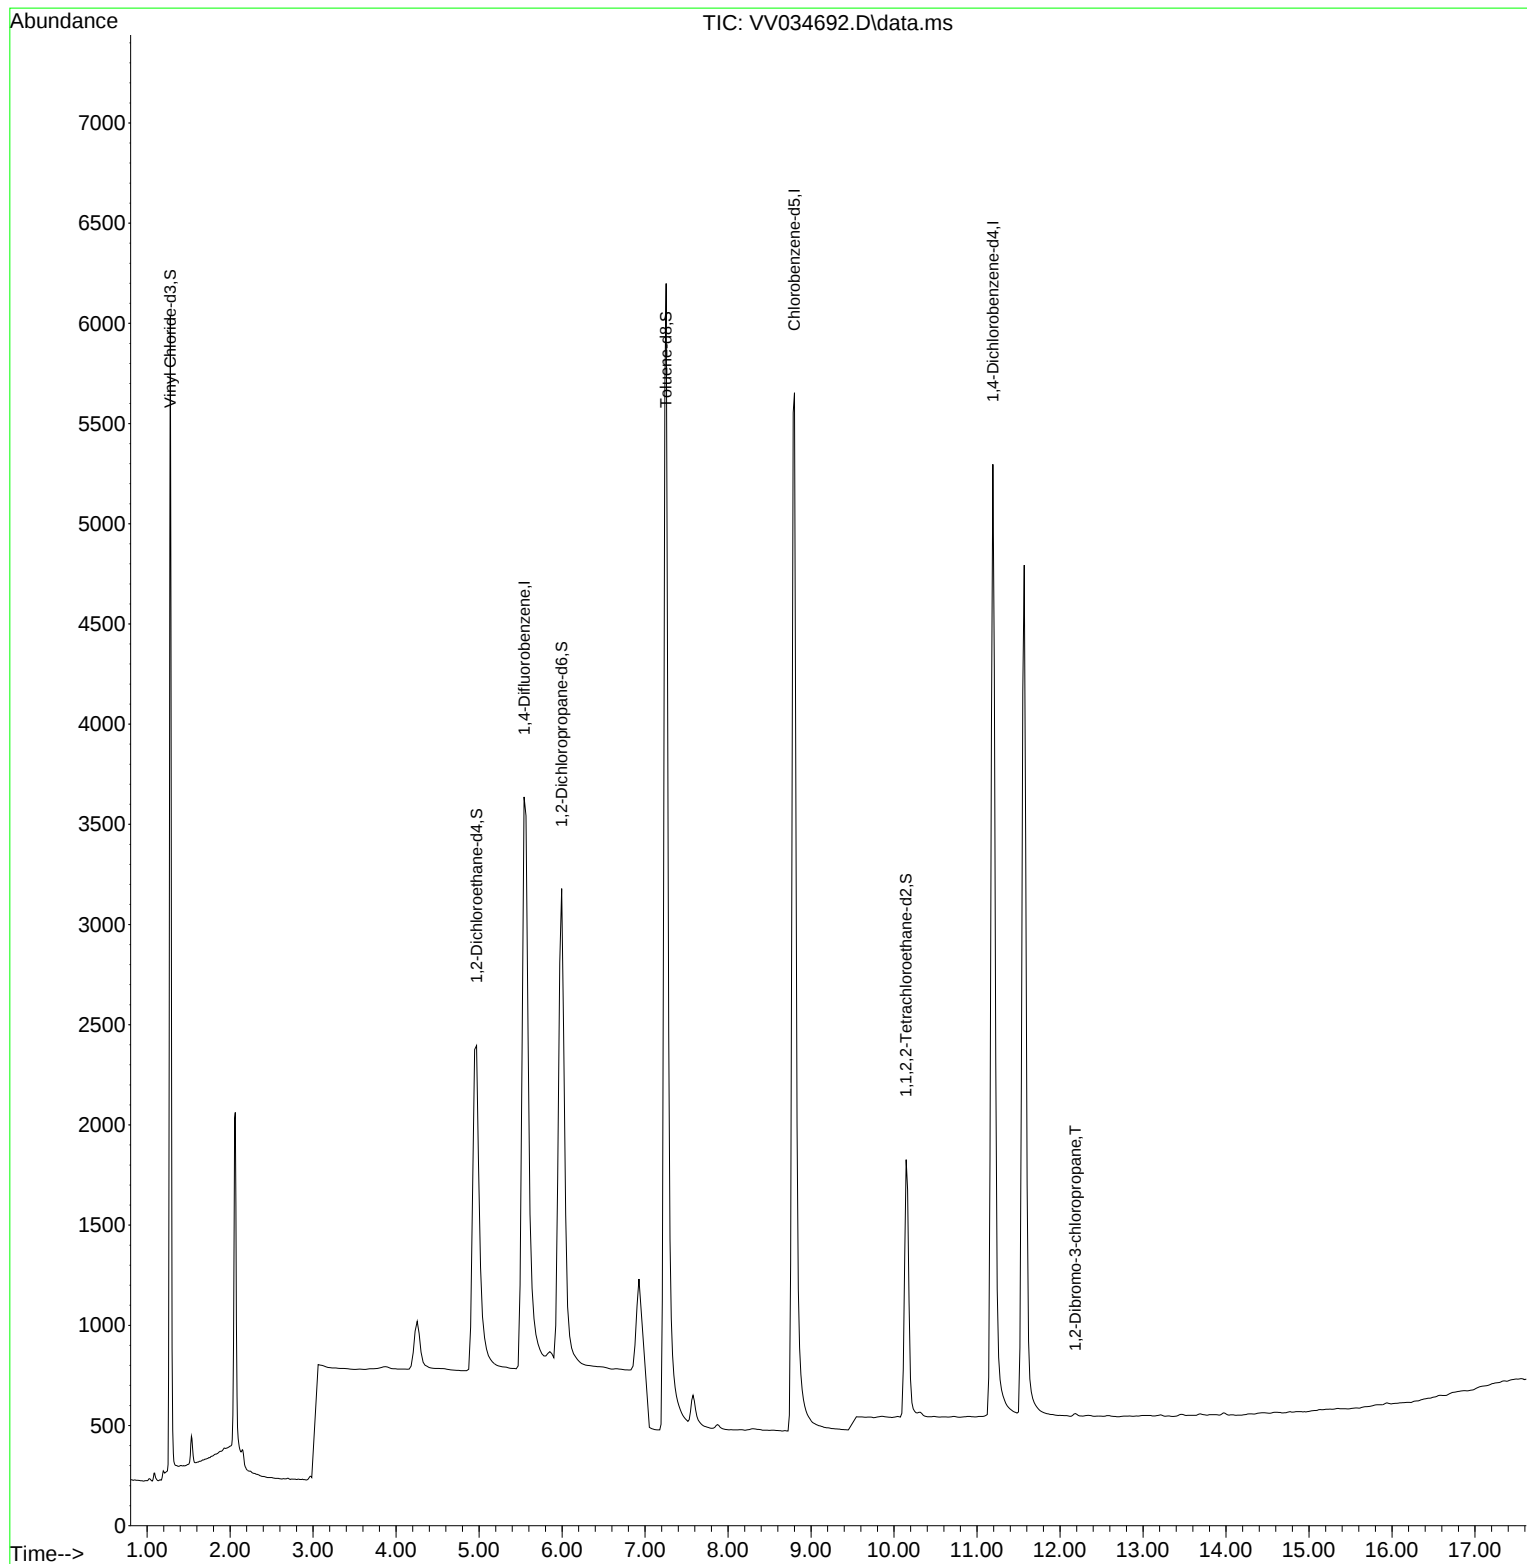

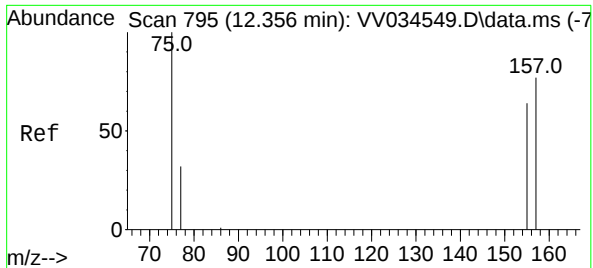

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.033 ug/L
 RT: 12.185 min Scan# 7
 Delta R.T. -0.171 min
 Lab File: VV034692.D
 Acq: 18 Mar 2024 12:05

Instrument :
 MSVOA_V
 ClientSampleId :

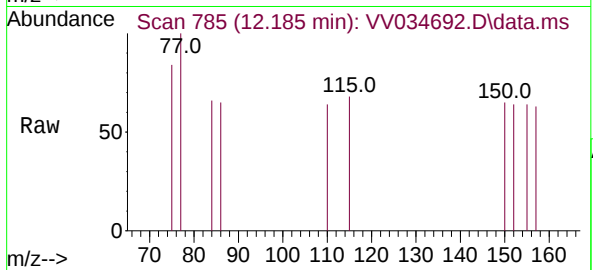

Tgt Ion: 75	Resp:	31
Ion	Ratio	Lower Upper
75	100	
157	74.6	62.9 94.3
155	76.1	56.2 84.4

