

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031824\
 Data File : VV034690.D
 Acq On : 18 Mar 2024 10:54
 Operator : SY/MD
 Sample : P1715-14DL 2X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGQM2DL

Quant Time: Mar 19 02:20:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 06 04:17:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	11701	0.500	ug/L	-0.02
5) Chlorobenzene-d5	8.800	117	10583	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	5287	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	6525	0.520	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 104.000%			
4) 1,2-Dichloroethane-d4	4.969	65	4033	0.519	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 104.000%			
7) 1,2-Dichloropropane-d6	5.995	67	4251	0.517	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 104.000%			
8) Toluene-d8	7.253	98	12089	0.496	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 100.000%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	2836	0.481	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 96.000%			
Target Compounds						
						Qvalue
3) Vinyl chloride	1.280	62	1193	0.091	ug/L	83
6) Trichloroethene	5.828	95	9274	1.119	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031824\
Data File : VV034690.D
Acq On : 18 Mar 2024 10:54
Operator : SY/MD
Sample : P1715-14DL 2X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGQM2DL

Quant Time: Mar 19 02:20:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 06 04:17:25 2024
Response via : Initial Calibration

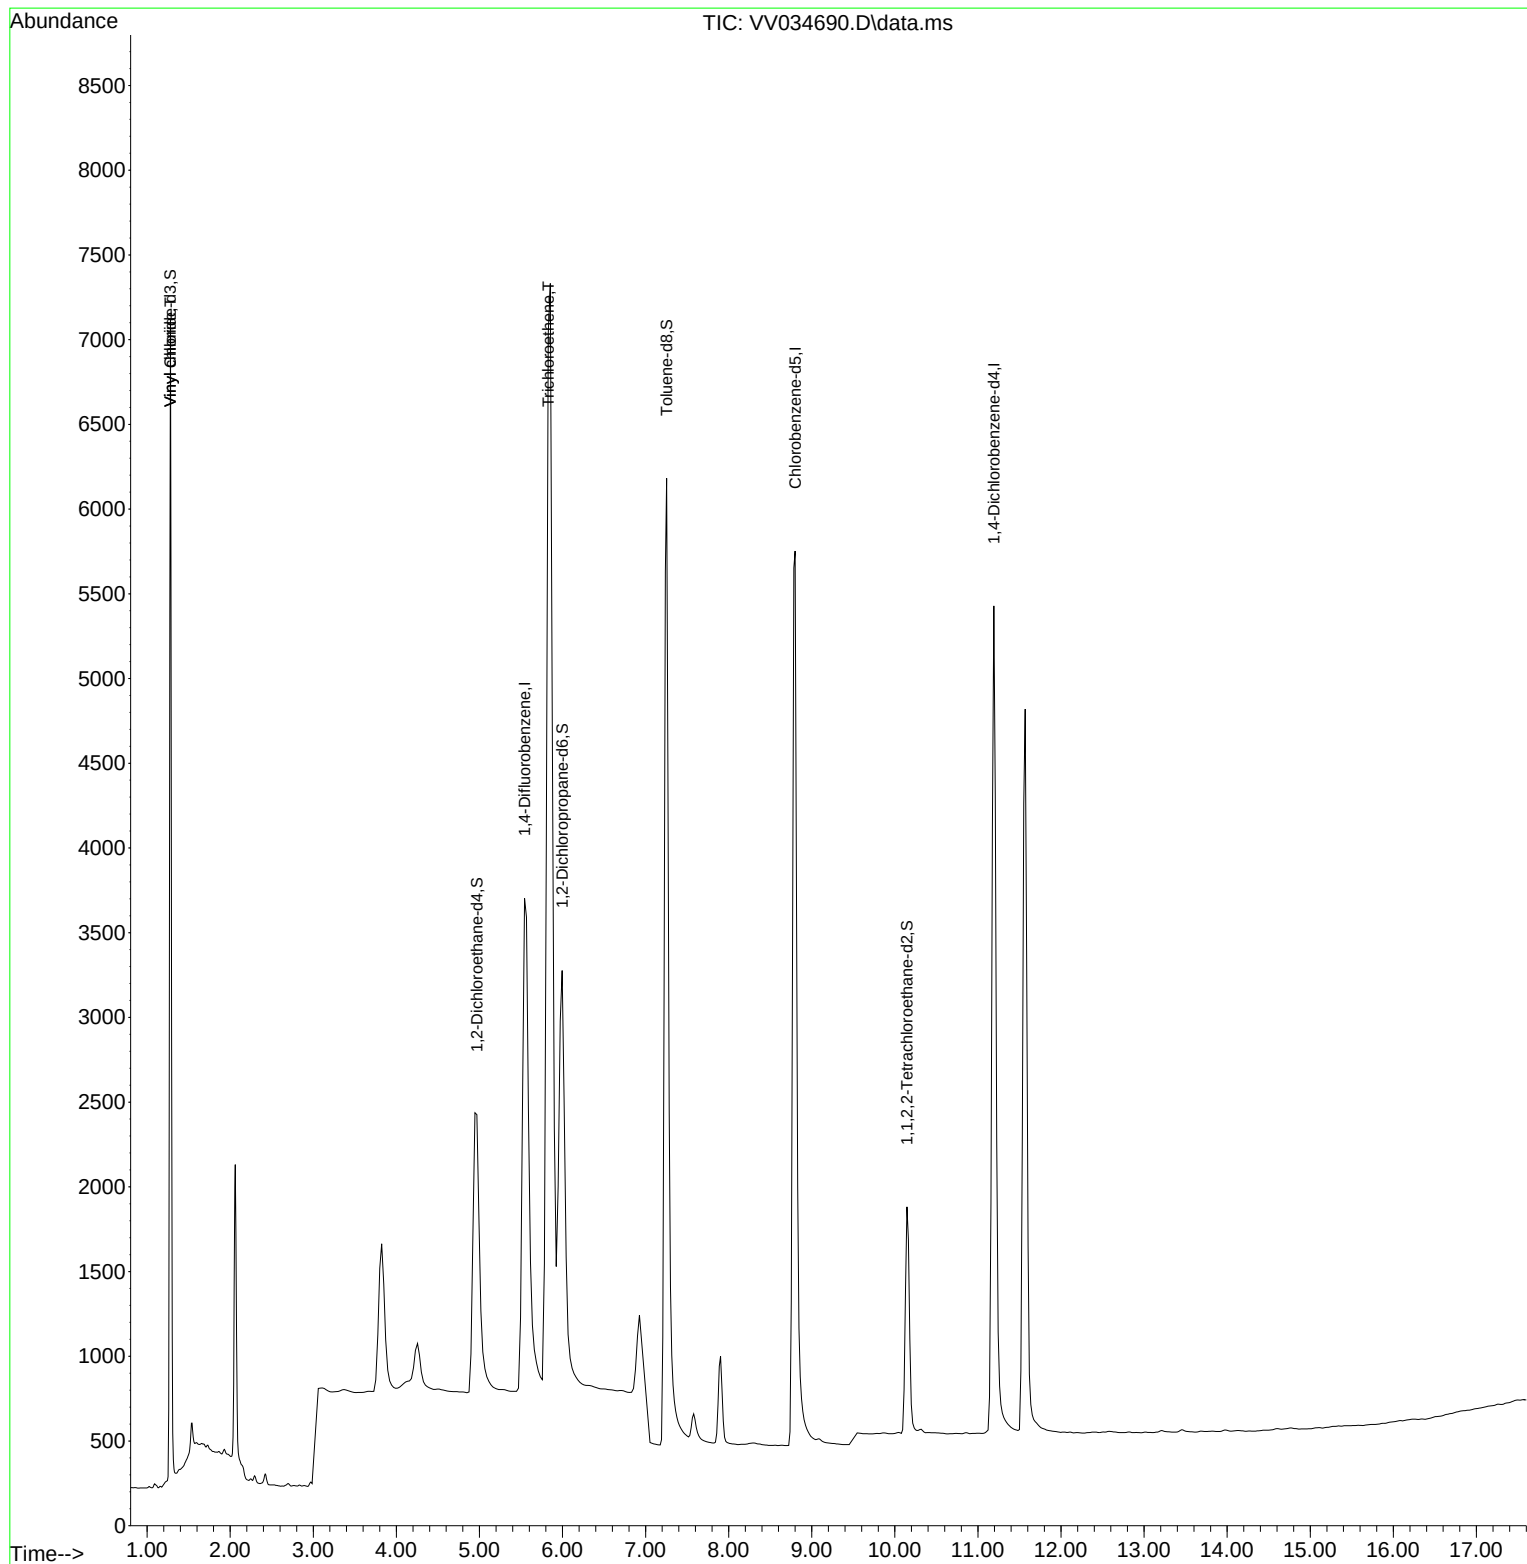

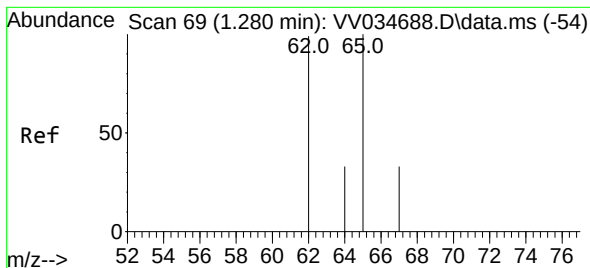

#3

Vinyl chloride

Concen: 0.091 ug/L

RT: 1.280 min Scan# 69

Delta R.T. 0.000 min

Lab File: VV034690.D

Acq: 18 Mar 2024 10:54

Instrument :

MSVOA_V

ClientSampleId :





BGQM2DL

Tgt Ion: 62 Resp: 1193

Ion Ratio Lower Upper

62 100

64 43.6 23.7 44.1

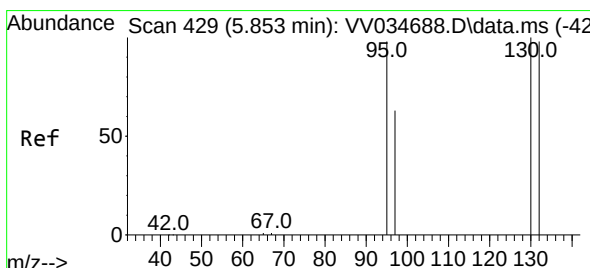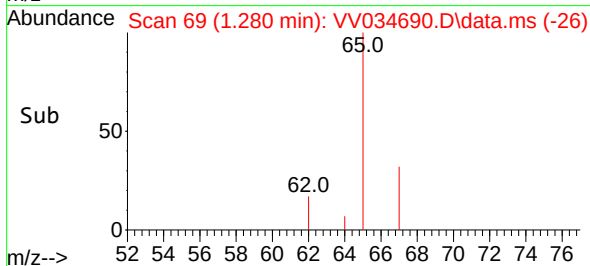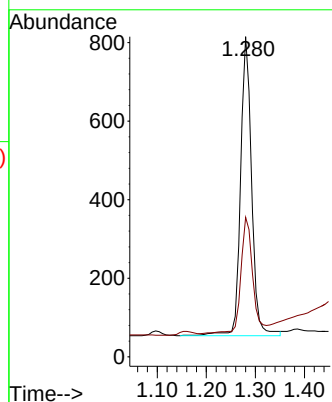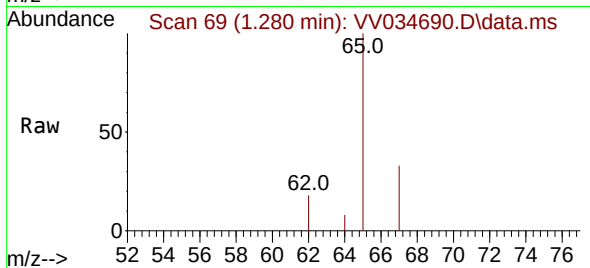

#6

Trichloroethene

Concen: 1.119 ug/L

RT: 5.828 min Scan# 428

Delta R.T. -0.024 min

Lab File: VV034690.D

Acq: 18 Mar 2024 10:54

Tgt Ion: 95 Resp: 9274

Ion Ratio Lower Upper

95 100

97 63.4 47.0 87.2

132 83.5 70.0 130.0

130 91.8 72.4 134.4

