

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031824\
 Data File : VV034691.D
 Acq On : 18 Mar 2024 11:17
 Operator : SY/MD
 Sample : P1715-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGQM2

Quant Time: Mar 19 02:20:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 06 04:17:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	11090	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.801	117	10293	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.192	152	5360	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.281	65	6369	0.536	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	108.000%
4) 1,2-Dichloroethane-d4	4.970	65	4127	0.560	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	112.000%
7) 1,2-Dichloropropane-d6	5.996	67	4321	0.540	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.000%
8) Toluene-d8	7.254	98	11949	0.504	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	3202	0.558	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	112.000%
Target Compounds						
						Qvalue
3) Vinyl chloride	1.281	62	2213	0.179	ug/L	94
6) Trichloroethene	5.829	95	17420	2.161	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031824\
Data File : VV034691.D
Acq On : 18 Mar 2024 11:17
Operator : SY/MD
Sample : P1715-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGQM2

Quant Time: Mar 19 02:20:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 06 04:17:25 2024
Response via : Initial Calibration

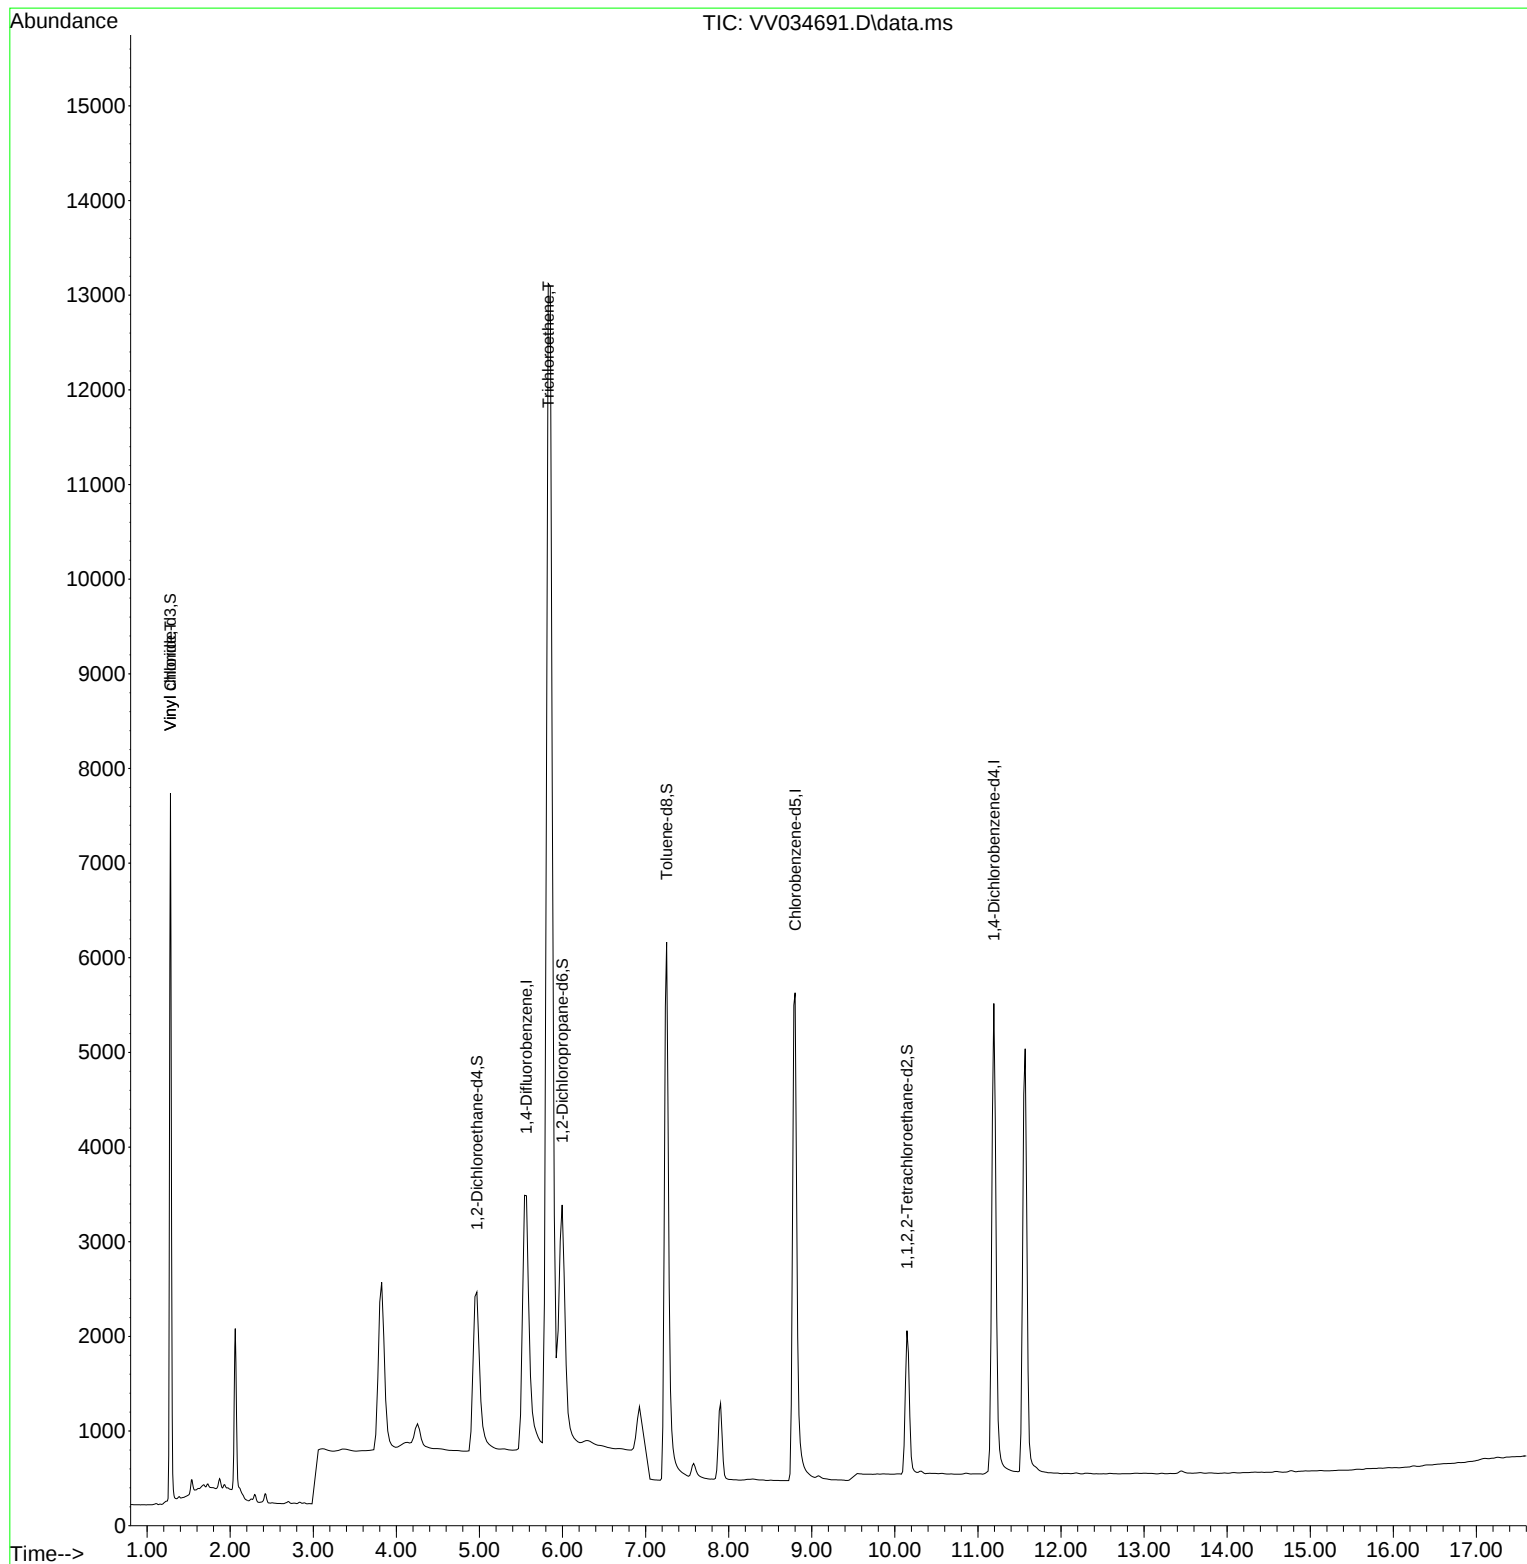

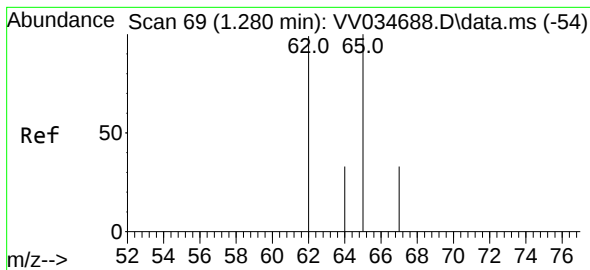

#3

Vinyl chloride

Concen: 0.179 ug/L

RT: 1.281 min Scan# 69

Delta R.T. 0.001 min

Lab File: VV034691.D

Acq: 18 Mar 2024 11:17

Instrument :

MSVOA_V

ClientSampleId :





BGQM2

Tgt Ion: 62 Resp: 2213

Ion Ratio Lower Upper

62 100

64 37.6 23.7 44.1

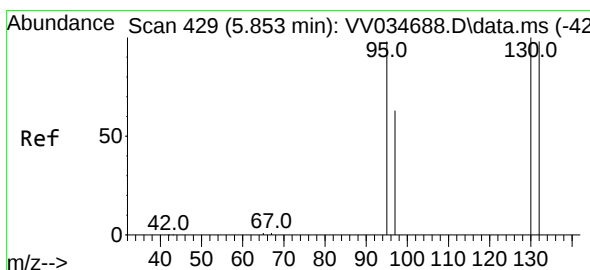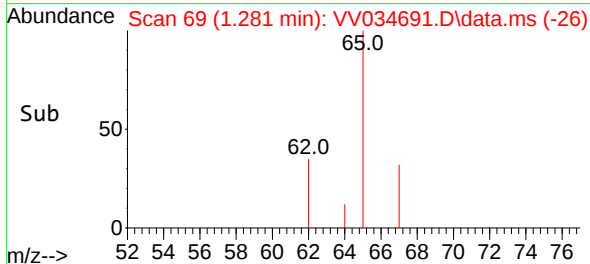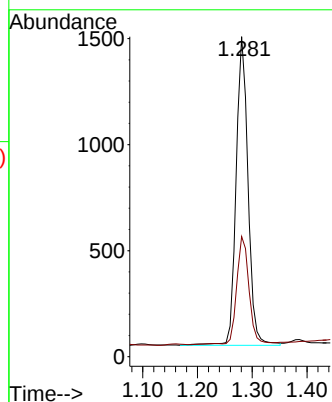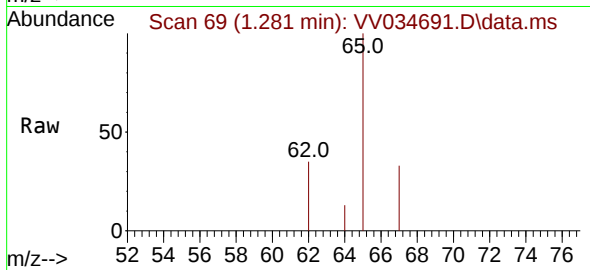

#6

Trichloroethene

Concen: 2.161 ug/L

RT: 5.829 min Scan# 428

Delta R.T. -0.023 min

Lab File: VV034691.D

Acq: 18 Mar 2024 11:17

Tgt Ion: 95 Resp: 17420

Ion Ratio Lower Upper

95 100

97 63.9 47.0 87.2

132 84.6 70.0 130.0

130 92.6 72.4 134.4

