


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031824\
Data File : VV034687.D
Acq On : 18 Mar 2024 08:35
Operator : SY/MD
Sample : BFB204
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB204

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM030524.M
Title : TRACE VOA SOM01.0
Last Update : Wed Mar 06 04:17:25 2024

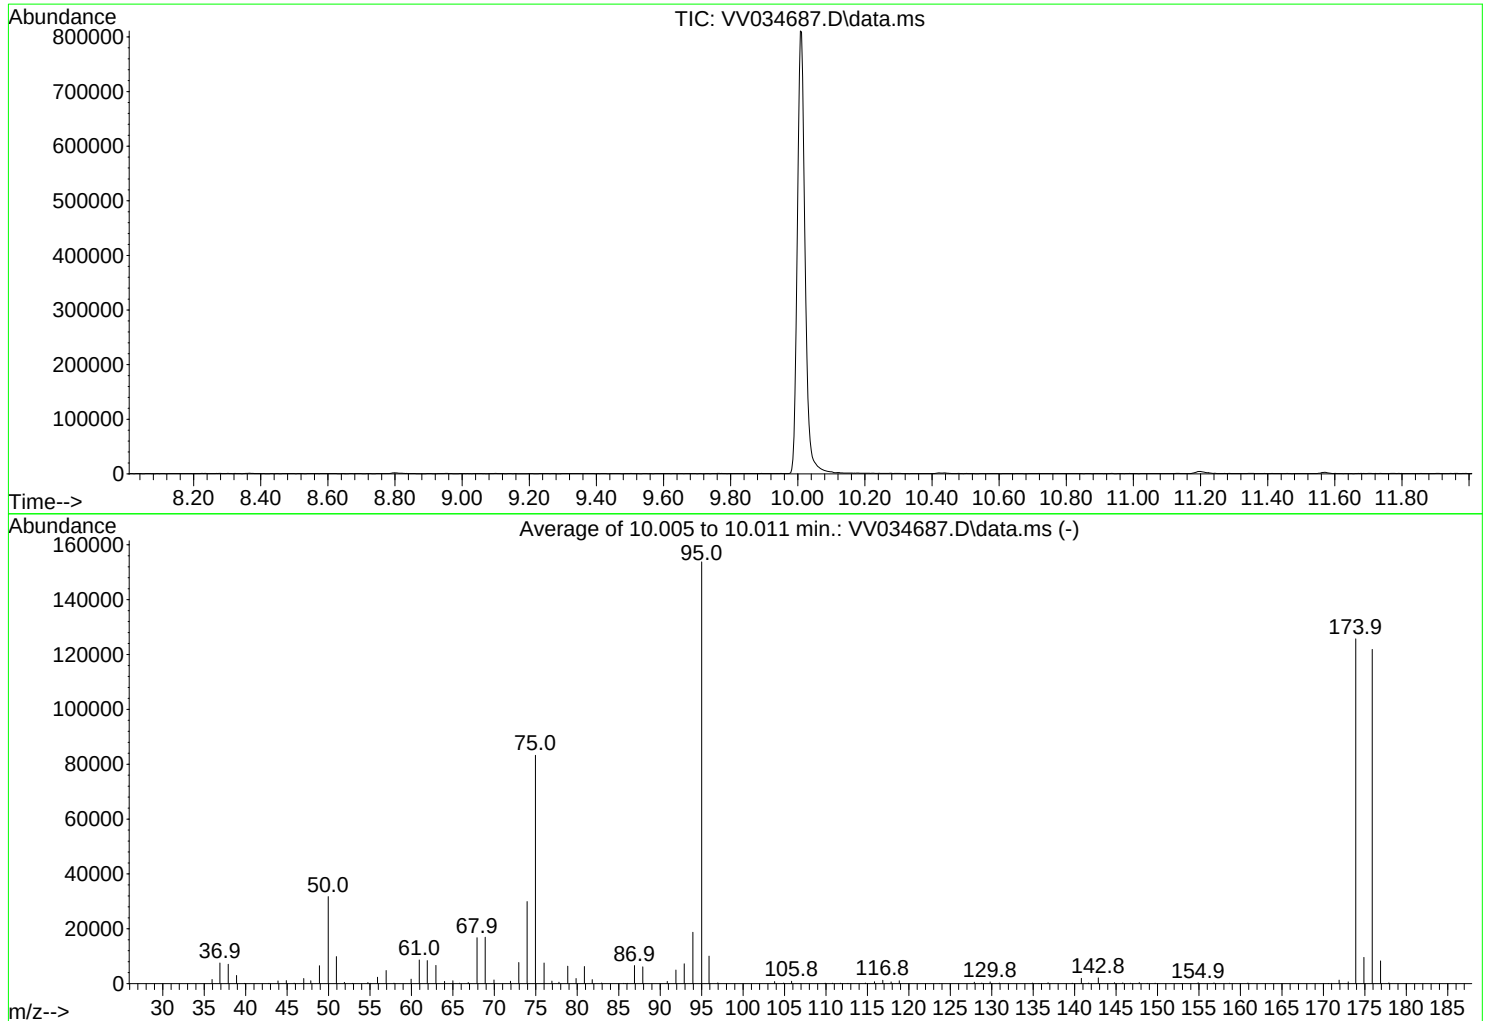

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	31765	PASS
75	95	30	80	54.1	83264	PASS
95	95	100	100	100.0	153792	PASS
96	95	5	9	6.5	10048	PASS
173	174	0.00	2	0.5	637	PASS
174	95	50	120	81.8	125747	PASS
175	174	5	9	7.6	9584	PASS
176	174	95	101	96.9	121896	PASS
177	176	5	9	6.8	8286	PASS

Scan 2776 (9.966 min): VV034687.D\data.ms
BFB204

m/z	Abundance
39.90	261.0
43.90	277.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
35.90	1505.0
36.90	7087.0
37.90	6891.0
38.90	2924.0
39.80	404.0
42.70	124.0
43.90	1232.0
44.90	1089.0
45.80	157.0
47.00	1676.0
47.80	987.0
48.90	6230.0
49.90	30296.0
50.90	9354.0
51.90	501.0
52.90	117.0
54.70	329.0
55.10	319.0
55.90	2291.0
57.00	4524.0
57.90	163.0
60.00	1464.0
61.00	8249.0
61.90	7909.0
63.00	6472.0
64.00	860.0
65.00	1143.0
65.80	157.0
67.00	400.0
67.90	16013.0
68.90	16039.0
69.90	1261.0
71.90	914.0
73.00	7647.0
73.90	28040.0
75.00	78592.0
76.00	7051.0
77.00	880.0
77.80	537.0
78.90	6022.0
79.80	1786.0
80.90	6018.0
81.80	1326.0
83.00	257.0
85.60	159.0
86.10	208.0
86.90	6248.0
87.90	5527.0
90.80	741.0
91.90	4360.0
92.90	6887.0
93.90	17880.0
95.00	143808.0
95.90	9709.0
96.90	336.0
103.80	771.0
104.90	209.0
105.90	793.0
106.90	132.0
110.00	175.0
110.80	189.0
111.70	168.0
112.70	132.0
114.70	234.0
115.80	596.0
116.80	1149.0
117.80	611.0
118.80	1041.0
127.90	530.0
128.80	264.0
129.80	589.0
130.90	231.0
134.90	216.0
136.80	344.0
139.70	107.0
140.80	1707.0
141.70	230.0
142.90	1796.0
144.80	358.0
145.80	252.0
146.80	156.0
147.80	428.0
148.80	108.0
149.70	180.0
154.90	310.0
156.80	270.0
158.70	186.0
161.00	230.0
170.60	168.0
171.90	1205.0
173.90	115720.0
174.90	8779.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

175.90111456.0

176.907949.0

177.90291.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
35.90	1606.0
36.90	7774.0
37.90	7259.0
38.90	3116.0
39.90	385.0
42.80	146.0
44.00	1257.0
44.90	1136.0
45.90	184.0
47.00	1907.0
47.90	1140.0
48.90	6705.0
49.90	32968.0
51.00	10164.0
51.90	497.0
52.90	151.0
54.80	426.0
55.90	2441.0
56.90	5056.0
57.90	156.0
60.00	1686.0
60.90	8891.0
61.90	8674.0
63.00	6767.0
64.00	853.0
65.00	1112.0
65.80	175.0
66.80	439.0
67.90	17328.0
68.90	17400.0
69.90	1370.0
71.90	913.0
73.00	7979.0
73.90	31008.0
75.00	86128.0
76.00	7900.0
77.00	977.0
77.80	510.0
78.80	6564.0
79.90	1925.0
80.90	6419.0
81.80	1475.0
82.90	233.0
85.60	190.0
86.00	203.0
86.90	6771.0
87.90	6470.0
90.80	860.0
91.90	5147.0
92.90	7464.0
94.00	19312.0
95.00	158976.0
95.90	10410.0
96.90	277.0
103.80	812.0
104.90	251.0
105.90	908.0
106.90	128.0
109.90	157.0
110.80	197.0
111.80	194.0
112.60	107.0
113.00	110.0
114.80	257.0
115.80	723.0
116.80	1301.0
117.80	686.0
118.80	1106.0
123.70	105.0
127.90	578.0
128.80	261.0
129.80	643.0
130.90	275.0
134.90	253.0
135.70	110.0
136.80	353.0
139.70	163.0
140.80	2010.0
141.70	258.0
142.80	2201.0
144.80	349.0
145.80	284.0
146.70	196.0
147.80	426.0
148.80	125.0
149.70	194.0
152.90	113.0
154.90	378.0
156.80	293.0
158.70	179.0
160.90	263.0
171.00	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

171.90	1314.0
173.90	129808.0
174.90	9944.0
175.90	126352.0
176.90	8664.0
177.90	282.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
36.00	1506.0
36.90	7709.0
37.90	6962.0
38.90	2887.0
39.80	373.0
42.90	135.0
44.00	1249.0
44.90	1134.0
45.90	187.0
47.00	1981.0
47.90	1052.0
48.90	6658.0
50.00	32032.0
51.00	10126.0
51.90	477.0
52.90	166.0
54.80	489.0
55.90	2357.0
56.90	4785.0
57.90	166.0
59.90	1722.0
60.90	8709.0
61.90	8572.0
62.90	6793.0
64.00	773.0
65.00	1001.0
65.80	160.0
66.80	441.0
67.90	16840.0
68.90	17312.0
70.00	1374.0
72.00	828.0
72.90	7563.0
74.00	30720.0
74.90	85072.0
76.00	7560.0
76.90	989.0
77.80	508.0
78.80	6548.0
79.90	1817.0
80.80	6276.0
81.80	1541.0
82.90	206.0
85.80	197.0
86.90	6710.0
87.90	6431.0
90.90	866.0
91.90	5328.0
92.90	7387.0
94.00	19008.0
95.00	158592.0
95.90	10025.0
97.00	246.0
103.80	781.0
104.90	255.0
105.80	899.0
109.80	144.0
110.80	211.0
111.80	194.0
112.70	103.0
113.00	128.0
114.80	262.0
115.90	744.0
116.90	1259.0
117.90	641.0
118.90	1105.0
123.70	133.0
127.90	558.0
128.80	251.0
129.80	635.0
130.90	304.0
134.90	283.0
135.70	108.0
136.80	351.0
139.70	187.0
140.80	2043.0
141.70	251.0
142.80	2255.0
144.80	342.0
145.80	287.0
146.70	201.0
147.80	401.0
148.70	119.0
149.70	195.0
152.80	103.0
154.90	402.0
156.80	313.0
158.70	169.0
160.80	269.0
171.00	216.0
171.90	1294.0
173.00	1911.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

173.90	131712.0
174.90	10029.0
175.90	127880.0
176.90	8245.0
177.90	248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204