

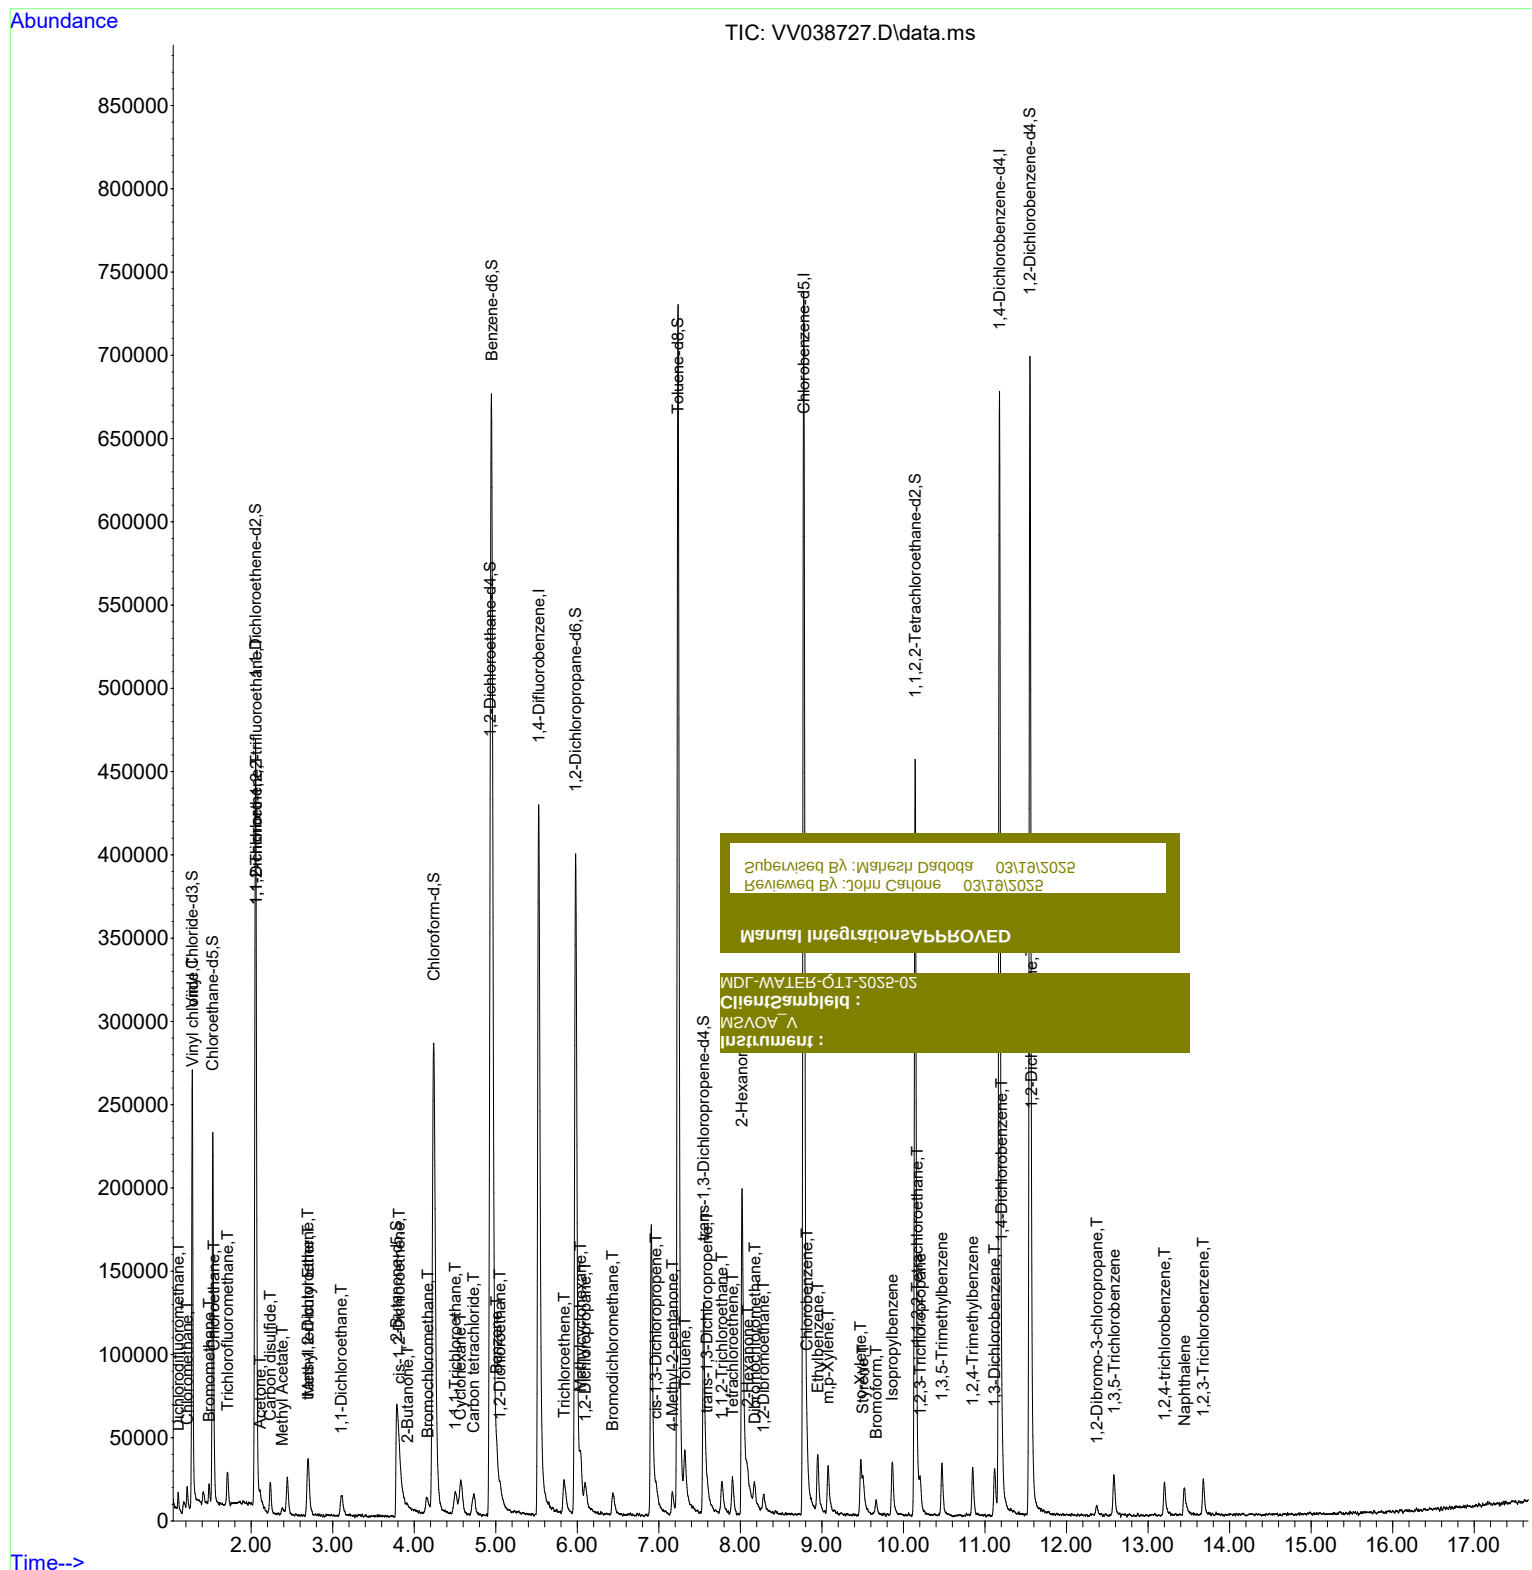
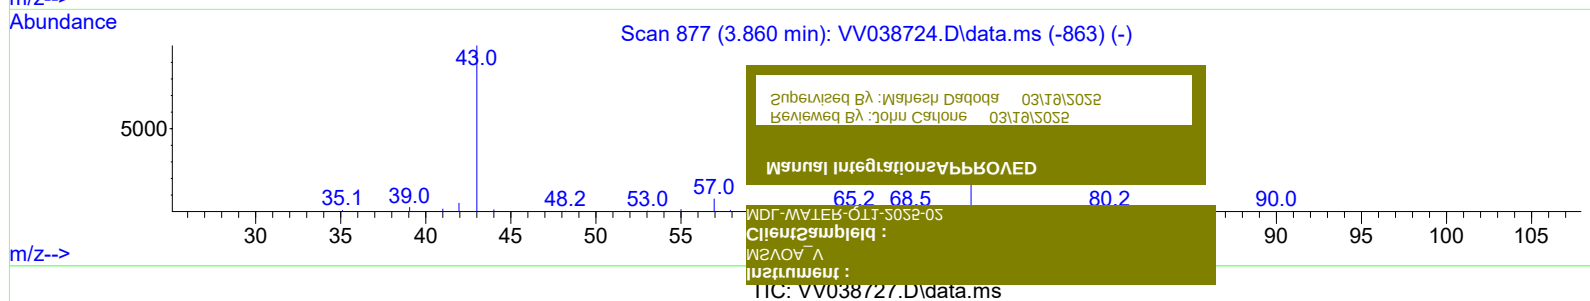


Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

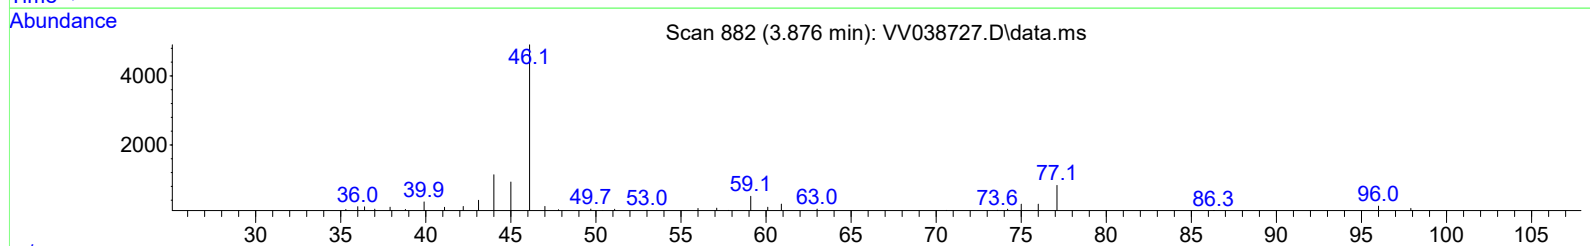

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

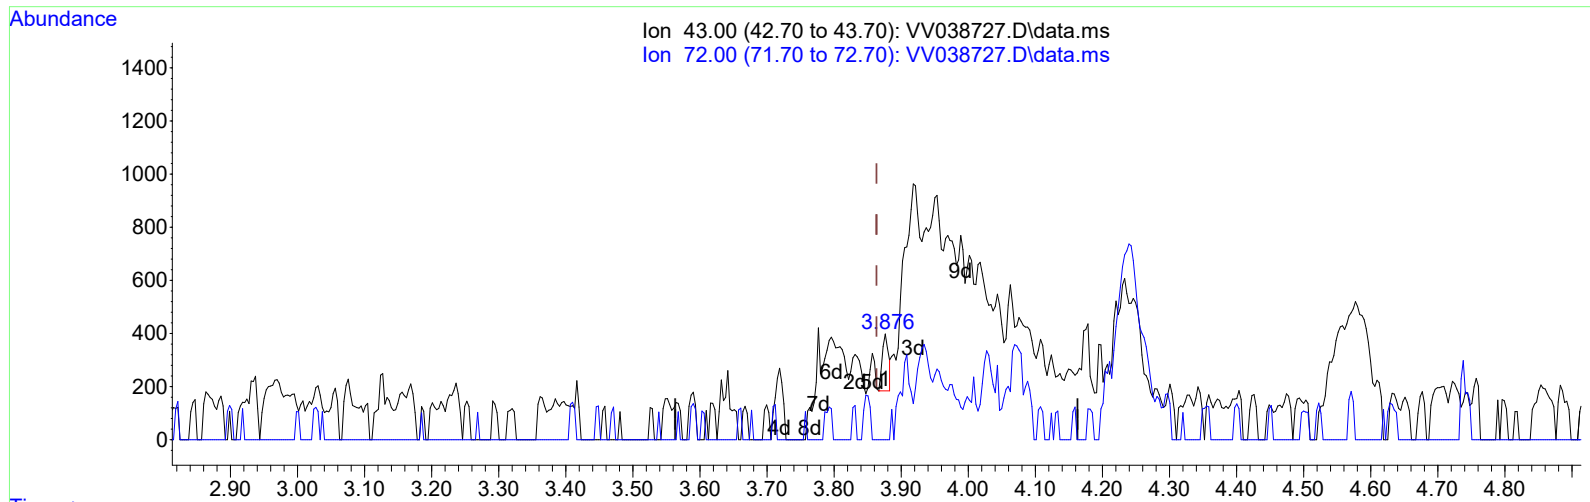

(22) 2-Butanone (T)




3.876min (+ 0.013) 0.09 ug/L

response 141

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	15.60
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

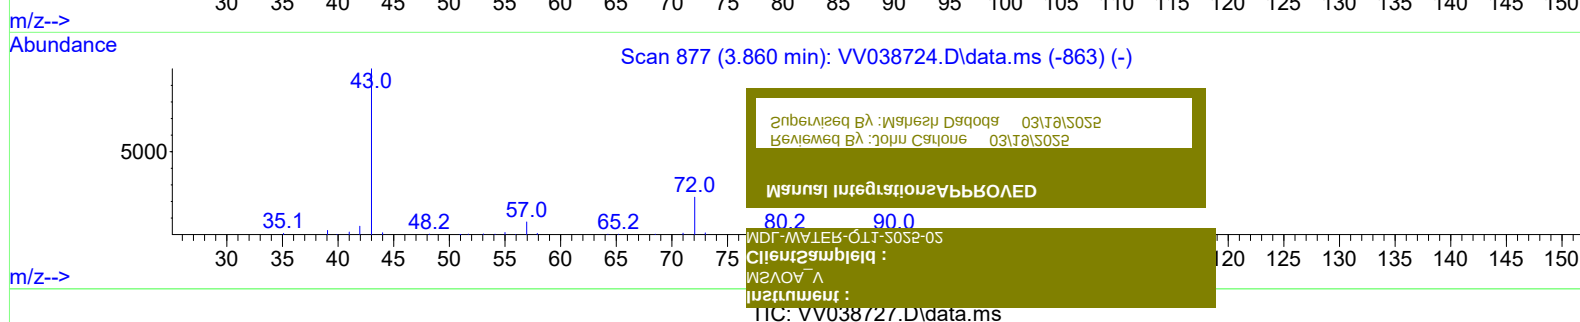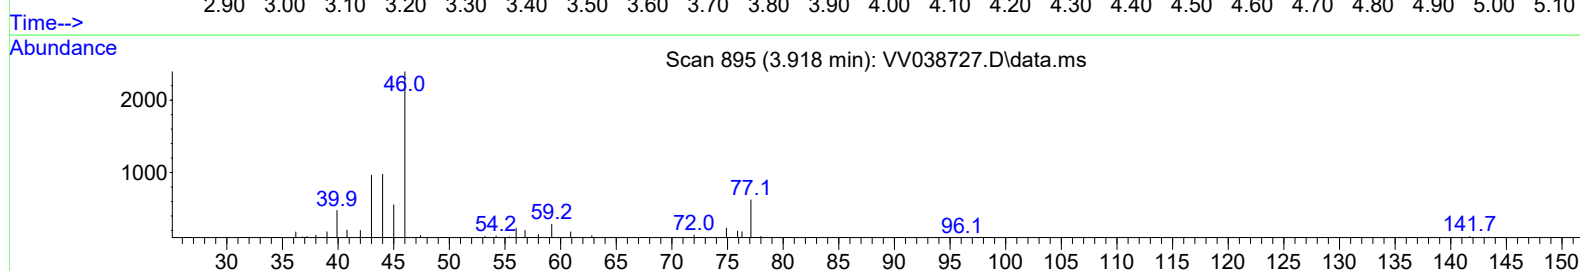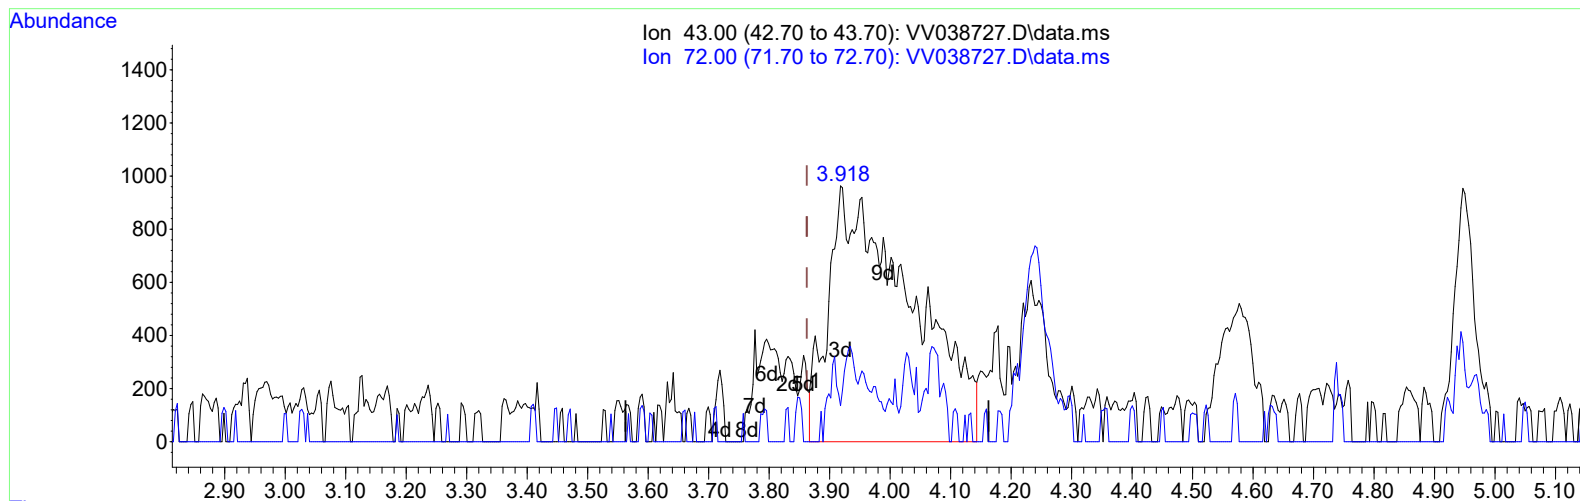

(22) 2-Butanone (T)




3.918min (+ 0.055) 5.89 ug/L m

response 9051

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	0.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

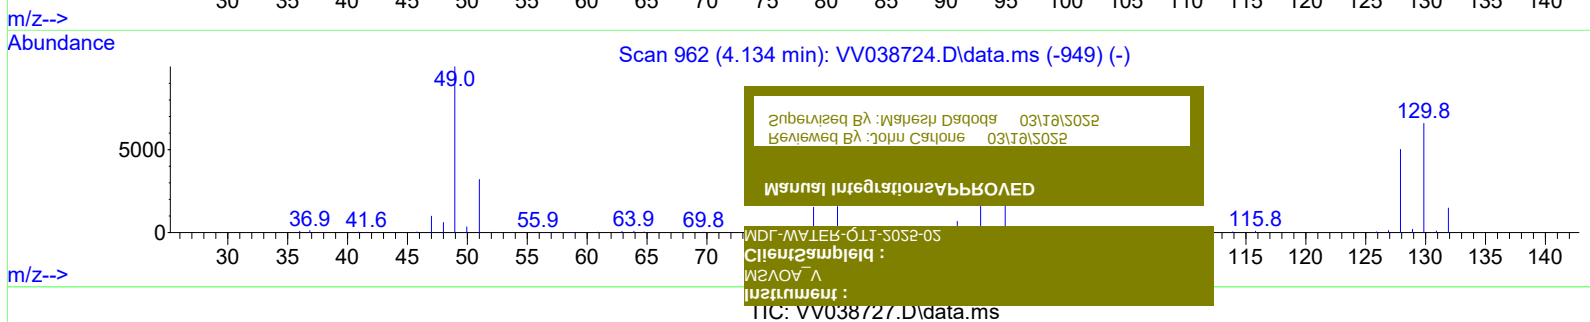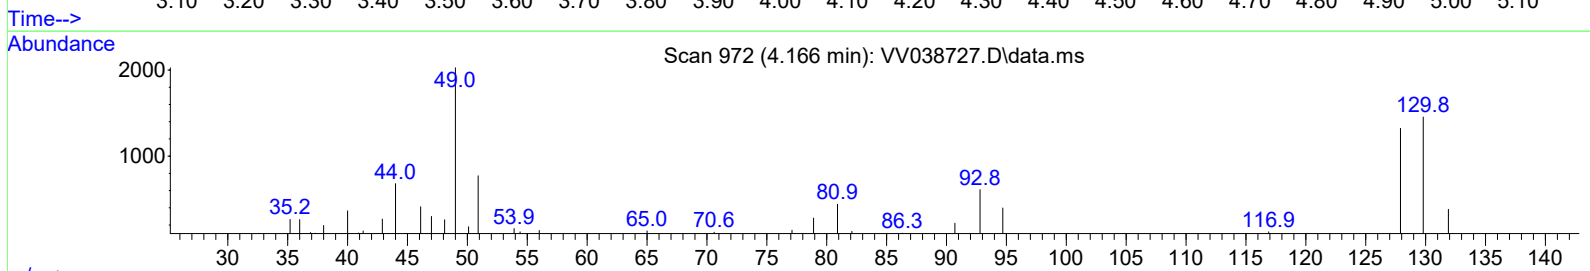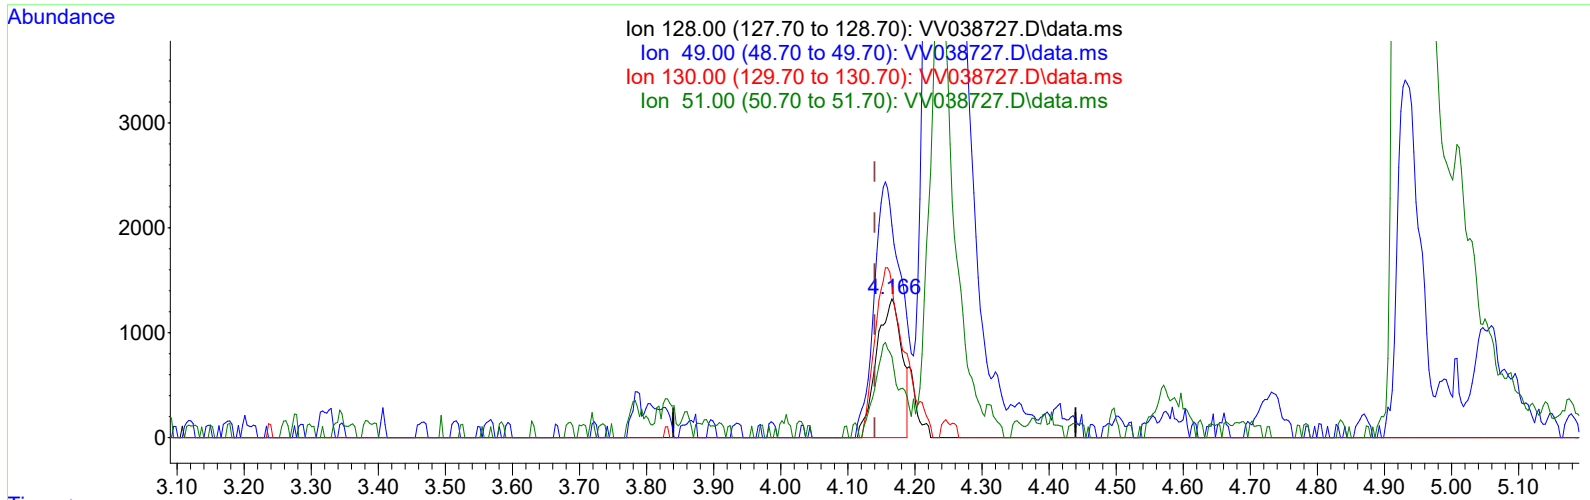

(23) Bromochloromethane (T)




4.166min (+ 0.026) 2.03 ug/L

response 3447

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	152.50	153.14
130.00	133.20	109.90
51.00	50.30	58.35

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

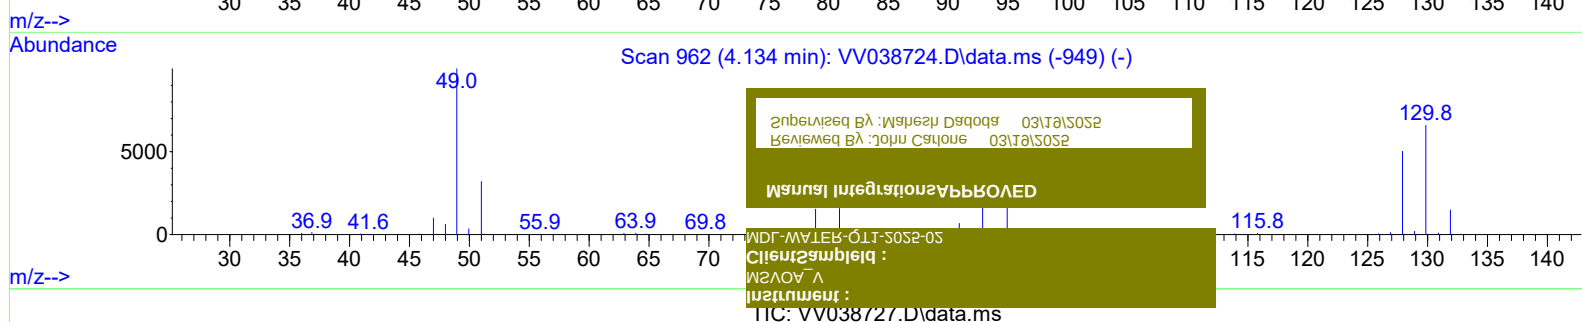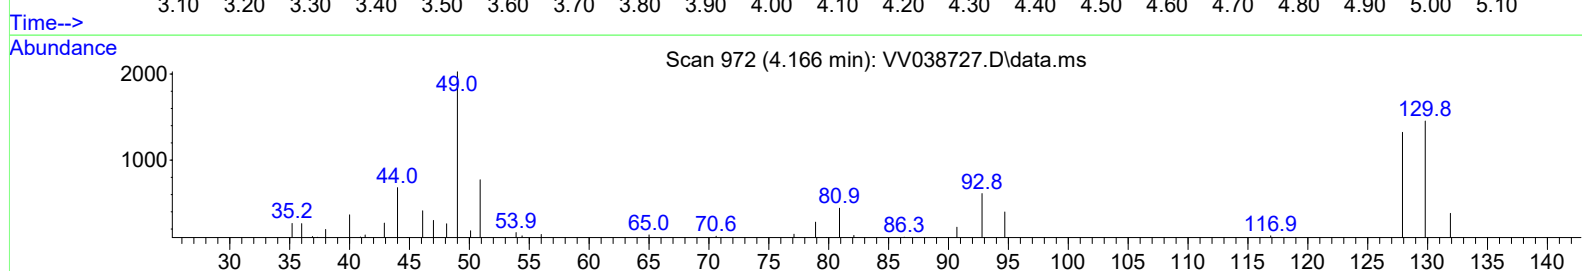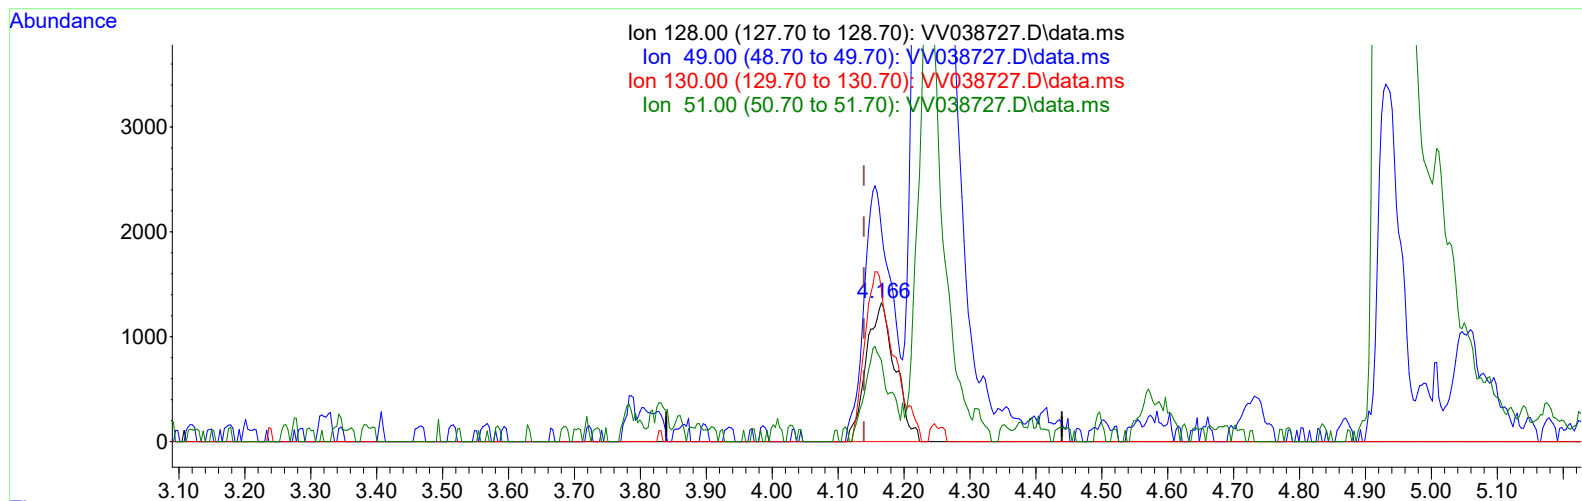

(23) Bromochloromethane (T)




4.166min (+ 0.026) 2.37 ug/L m

response 4026

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	152.50	153.14
130.00	133.20	109.90
51.00	50.30	58.35

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

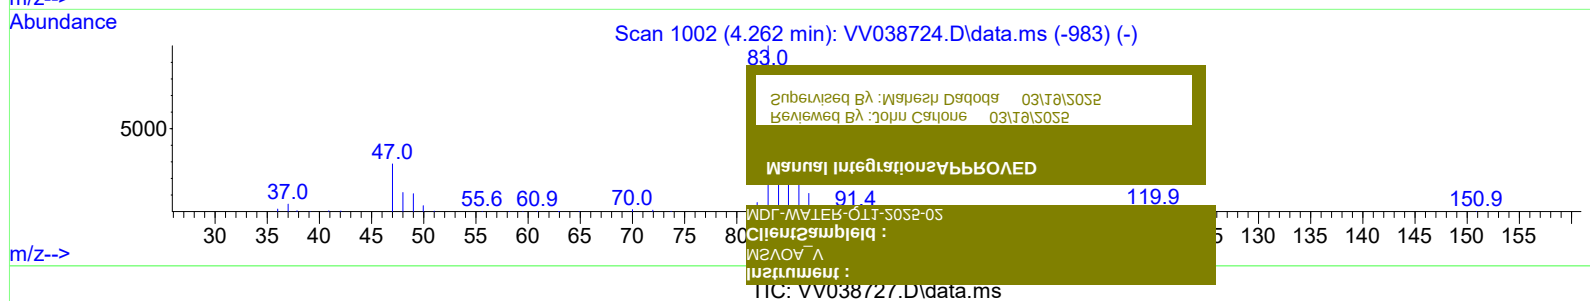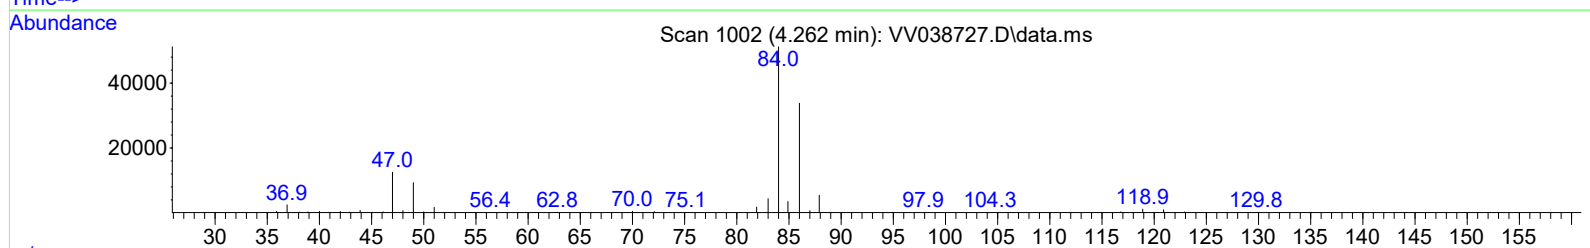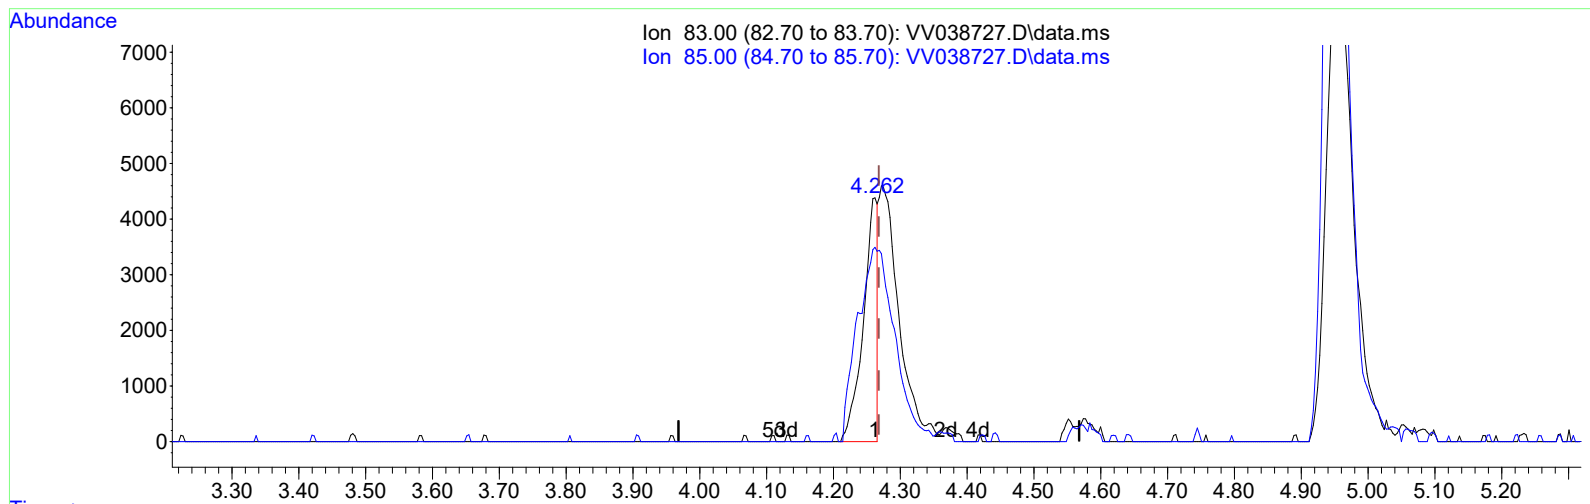

(25) Chloroform (T)




4.262min (-0.006) 1.05 ug/L

response 6414

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	64.60	79.71
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

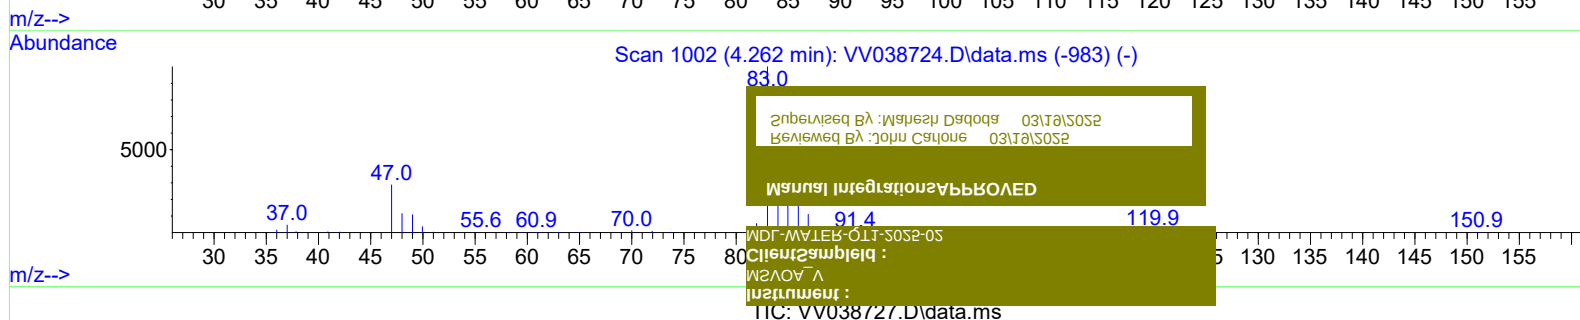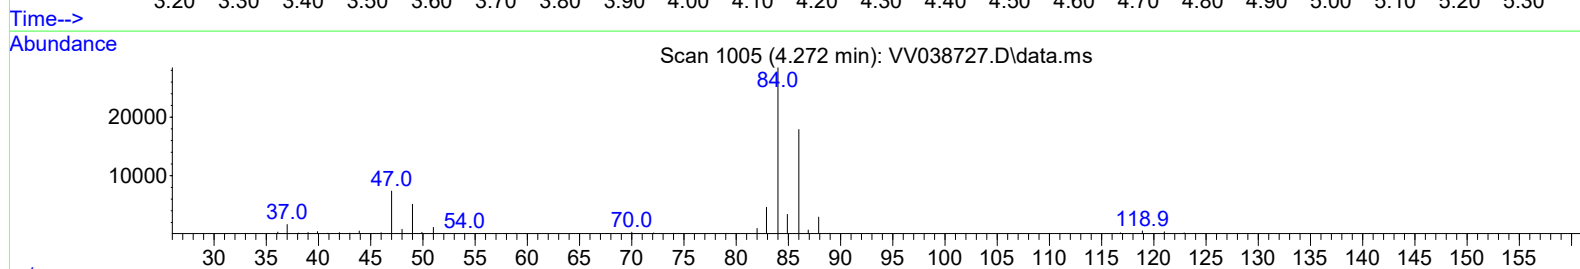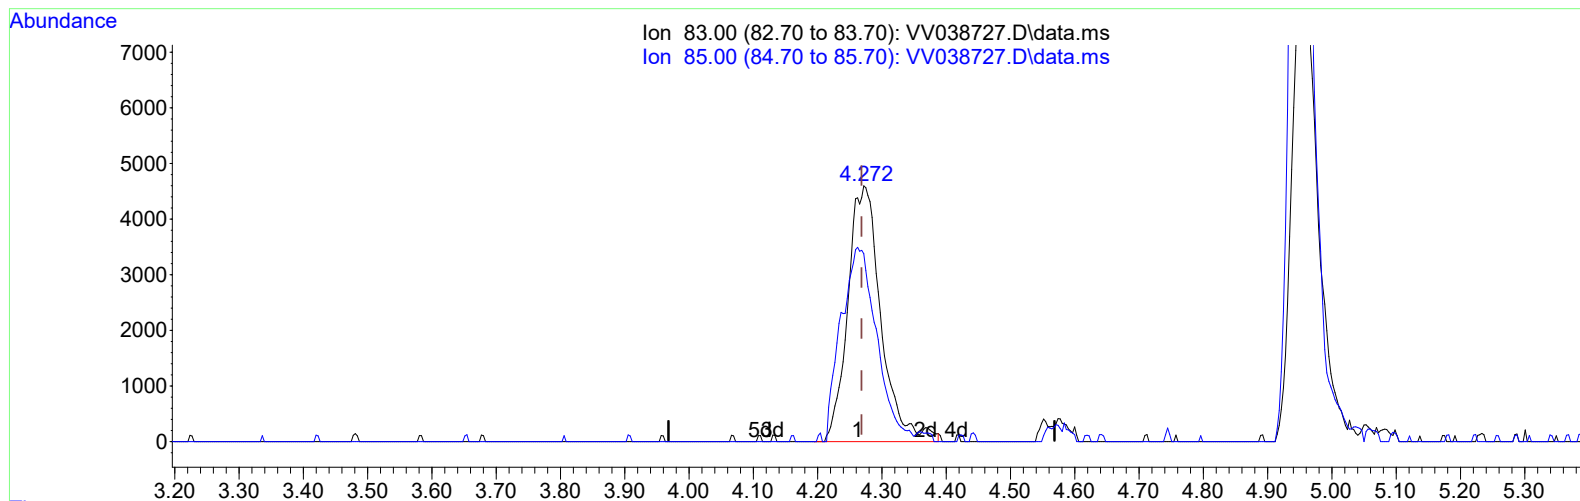

(25) Chloroform (T)




4.272min (+ 0.003) 2.69 ug/L m

response 16453

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	64.60	73.47
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

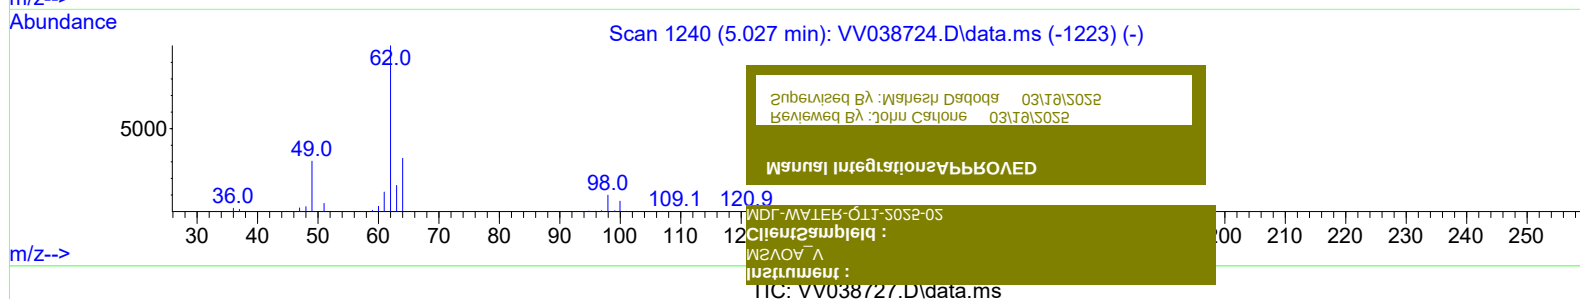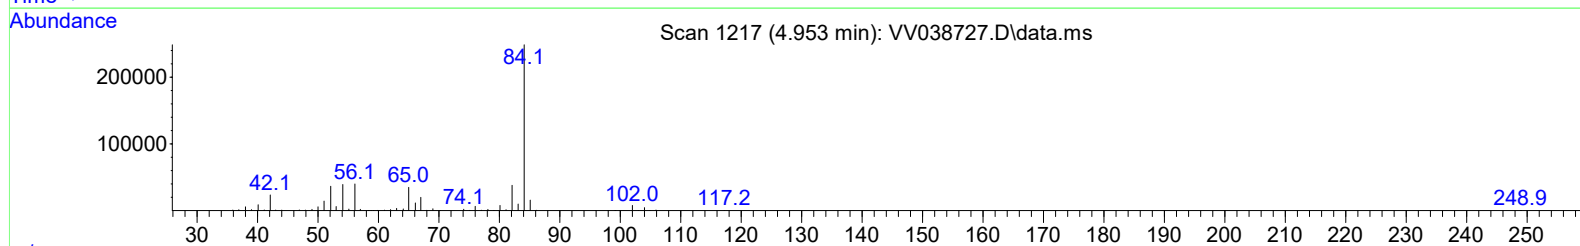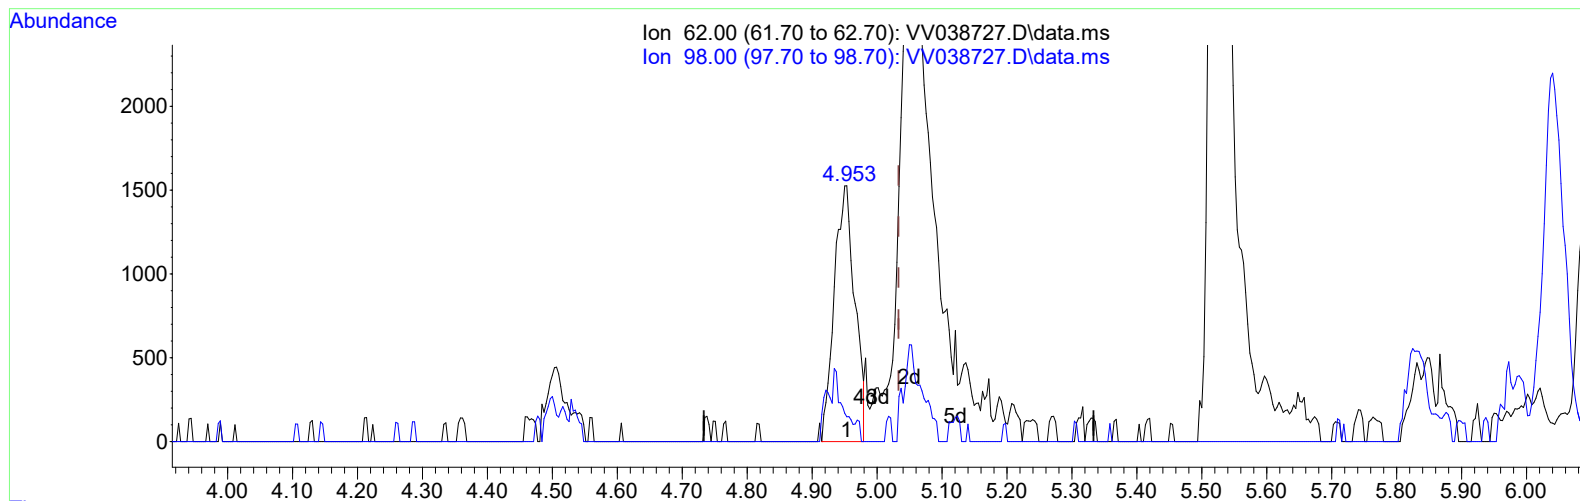

(27) 1,2-Dichloroethane (T)




4.953min (-0.080) 0.76 ug/L

response 3338

Ion	Exp%	Act%
62.00	100.00	100.00
98.00	9.40	9.70
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

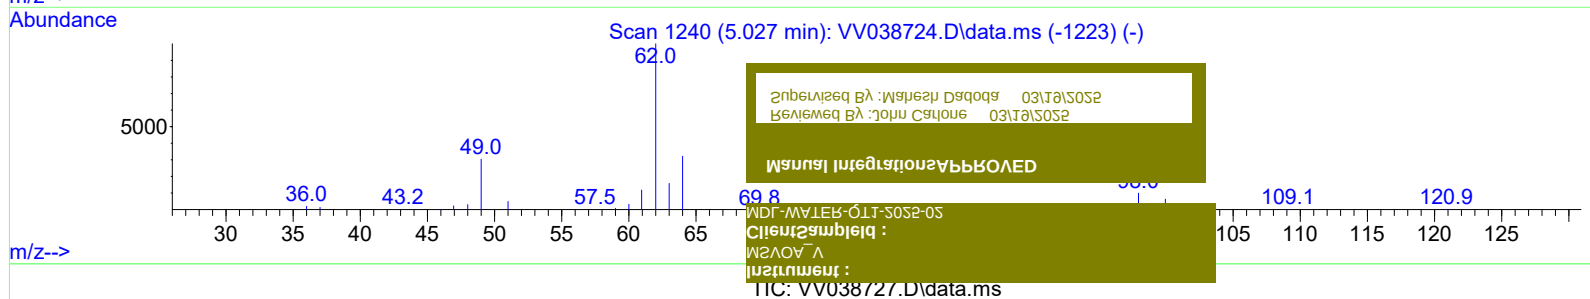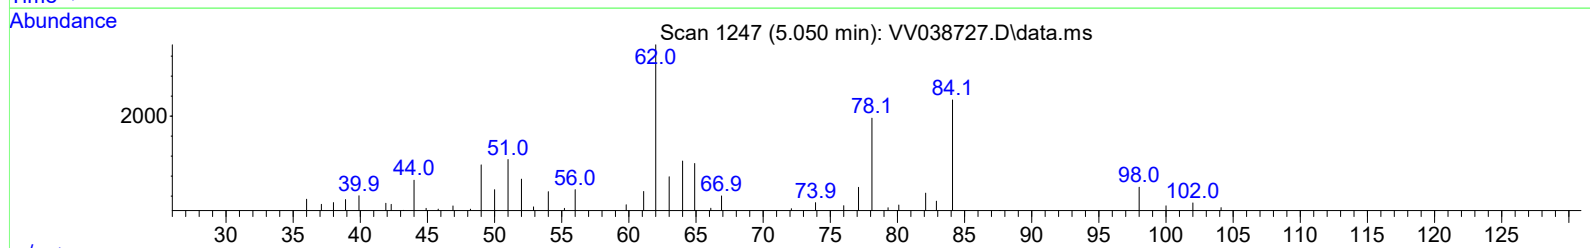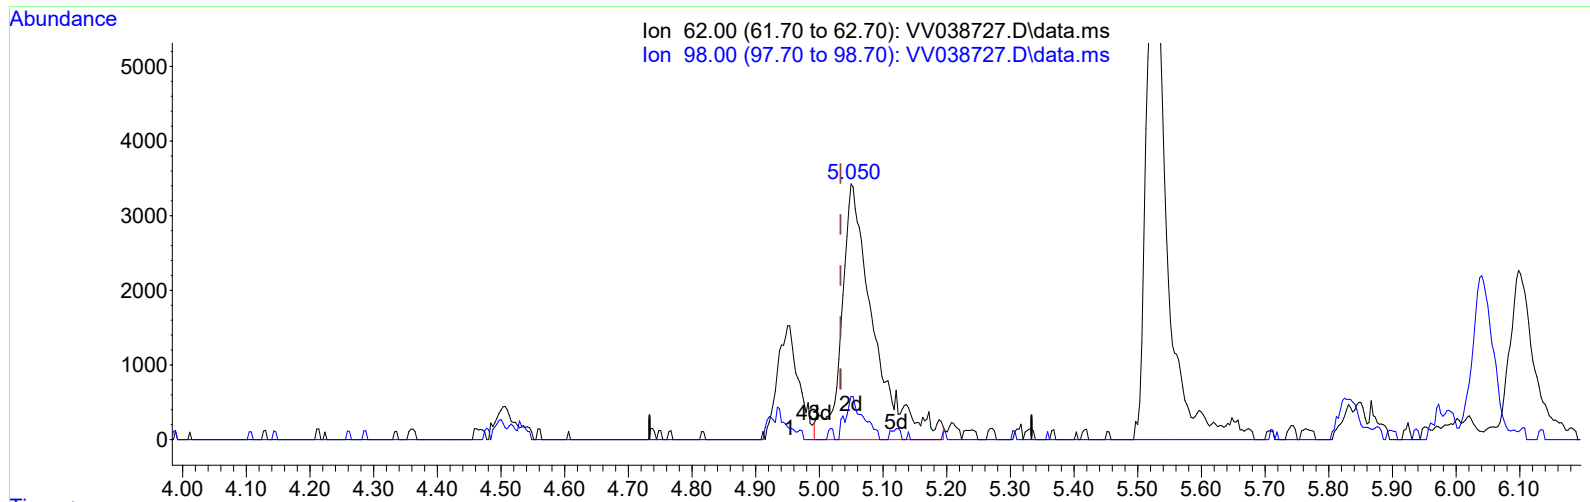

(27) 1,2-Dichloroethane (T)




5.050min (+ 0.016) 2.73 ug/L m

response 11971

Ion	Exp%	Act%
62.00	100.00	100.00
98.00	9.40	16.87#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

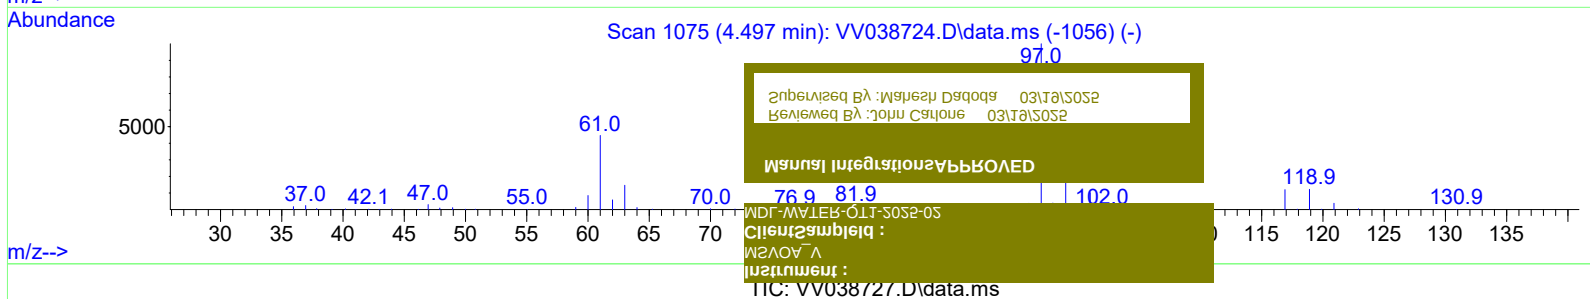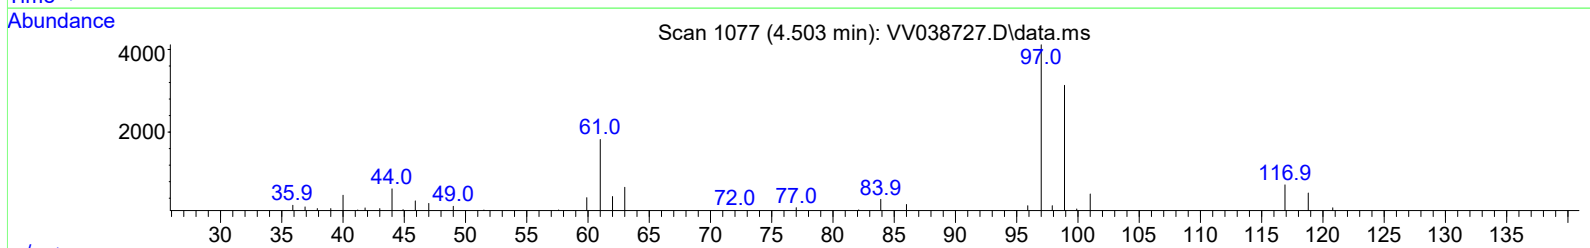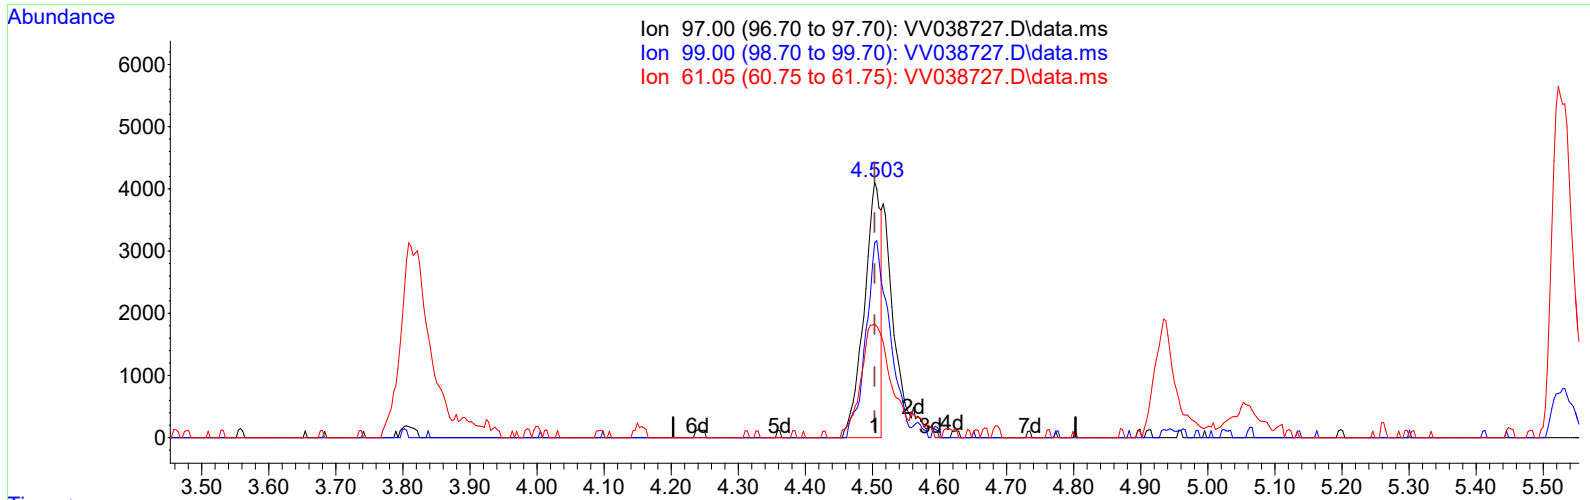

(30) 1,1,1-Trichloroethane (T)




4.503min (+ 0.000) 1.40 ug/L

response 7039

Ion	Exp%	Act%
97.00	100.00	100.00
99.00	65.40	110.78#
61.05	42.00	79.66#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

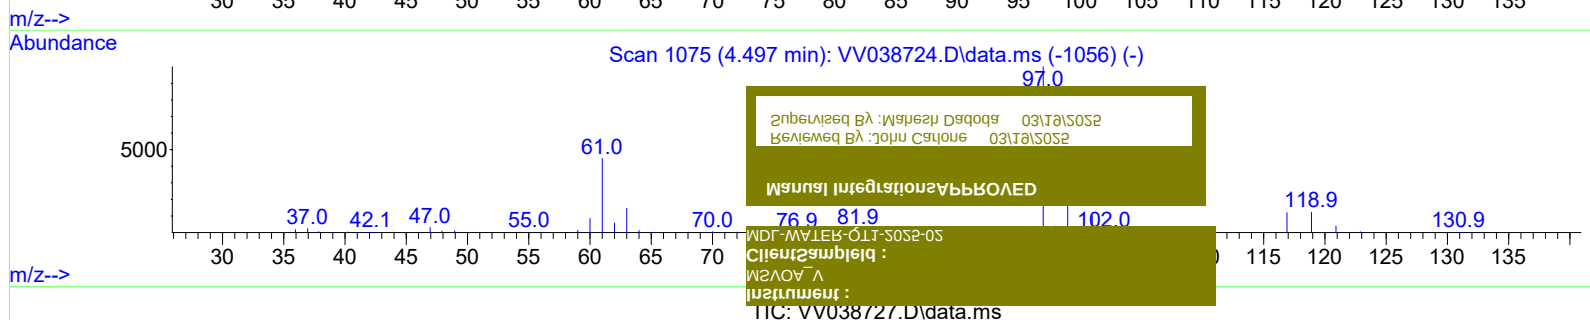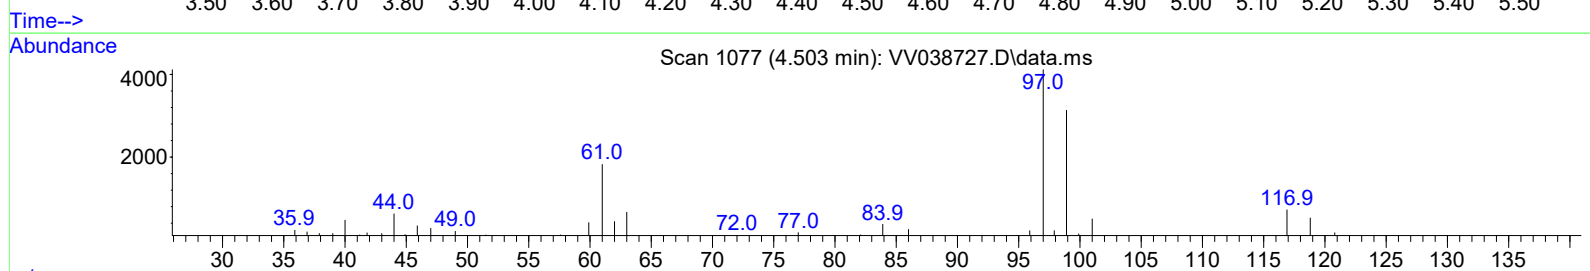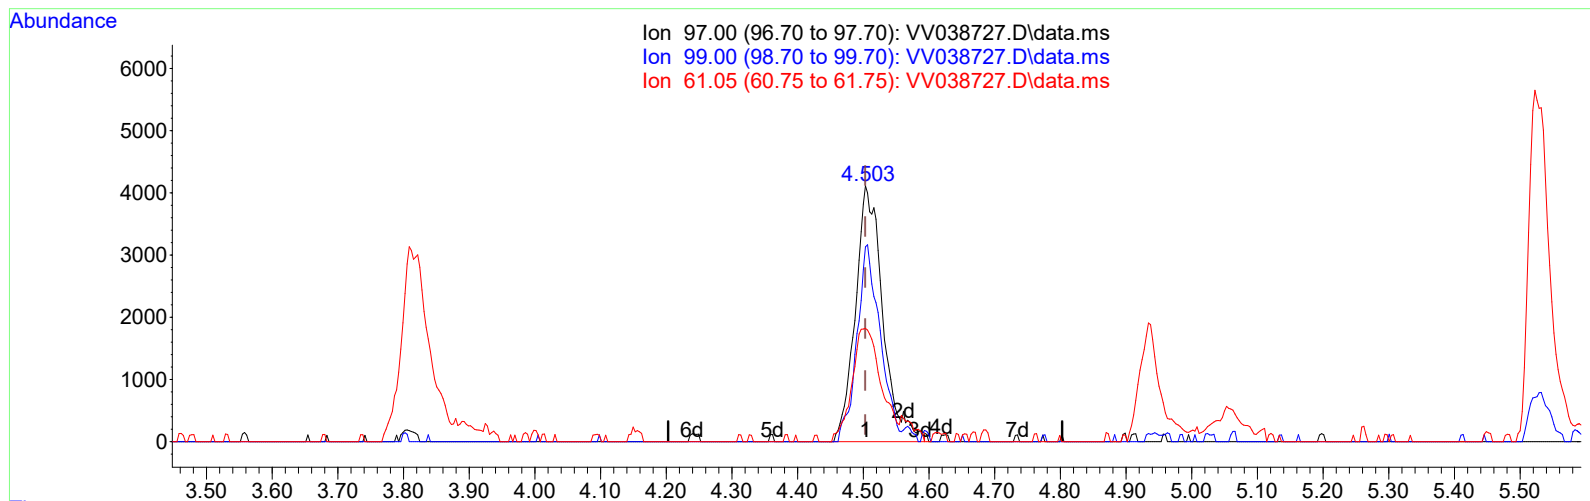

(30) 1,1,1-Trichloroethane (T)




4.503min (+ 0.000) 2.37 ug/L m

response 11951

Ion	Exp%	Act%
97.00	100.00	100.00
99.00	65.40	65.25
61.05	42.00	46.92
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

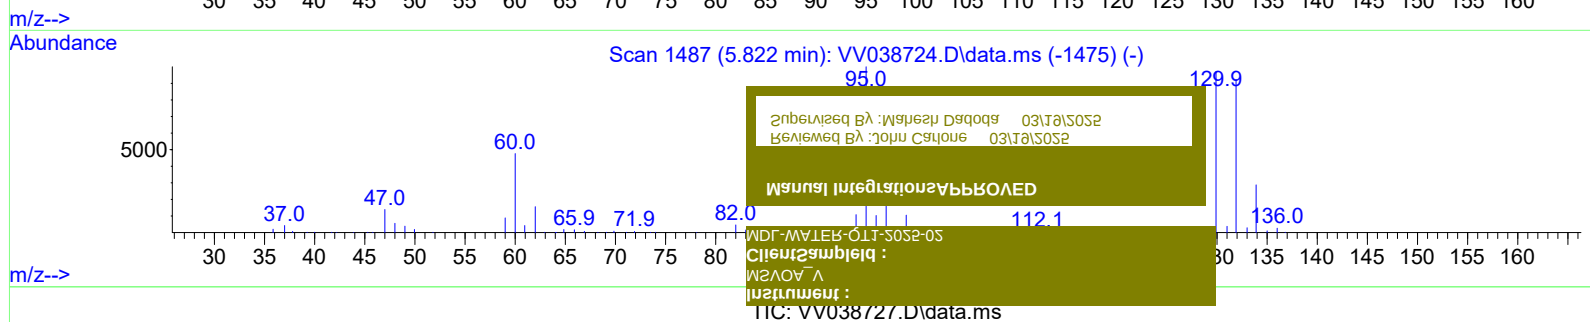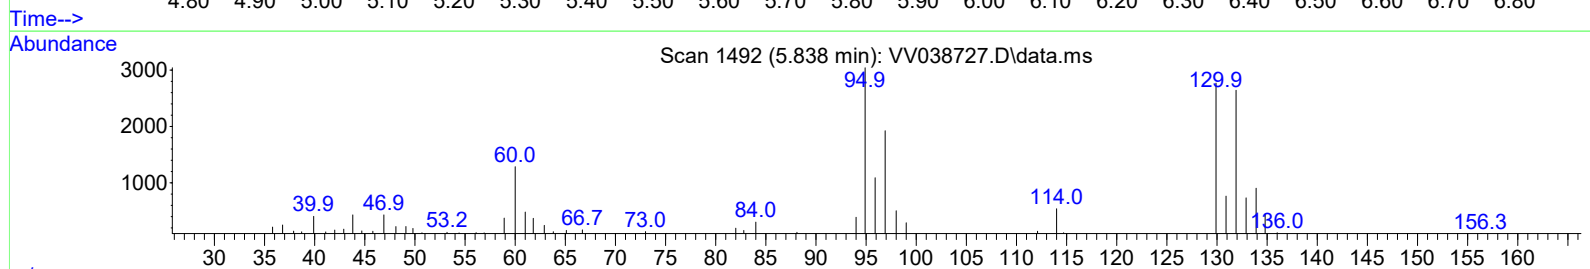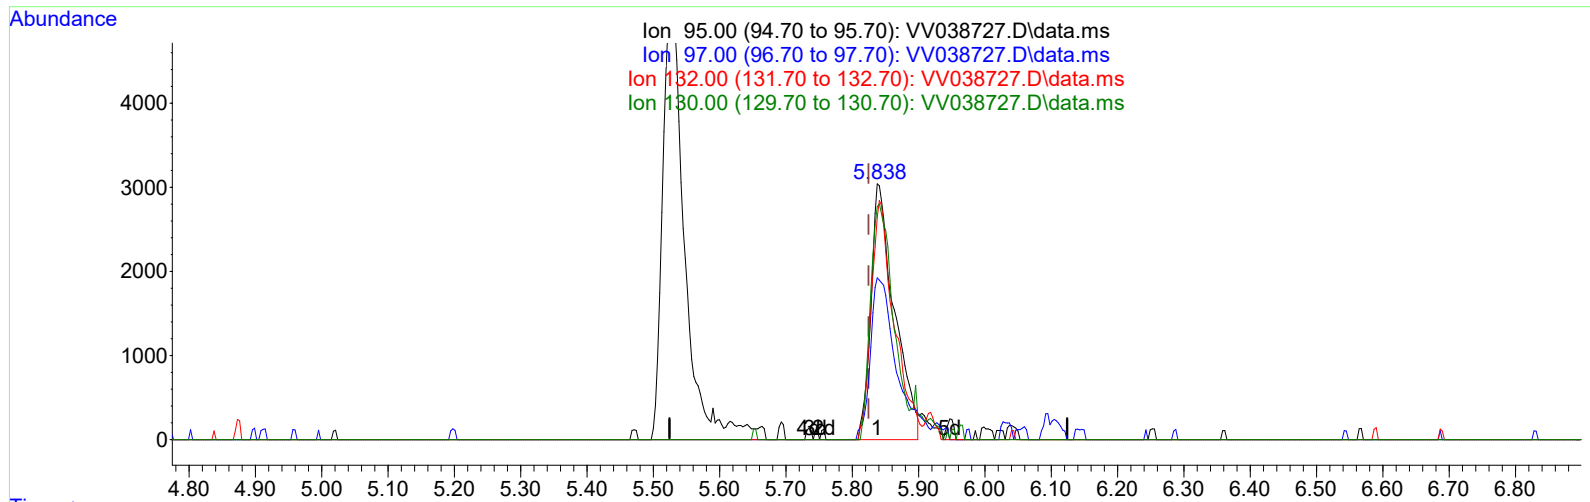

(34) Trichloroethene (T)




5.838min (+ 0.013) 2.32 ug/L

response 7451

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	65.20	63.27
132.00	96.60	86.88
130.00	101.20	91.06

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

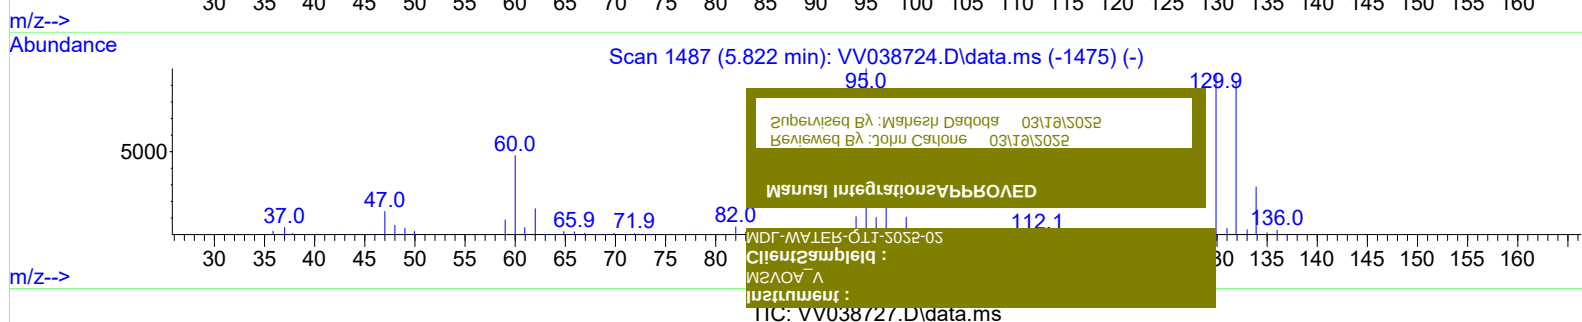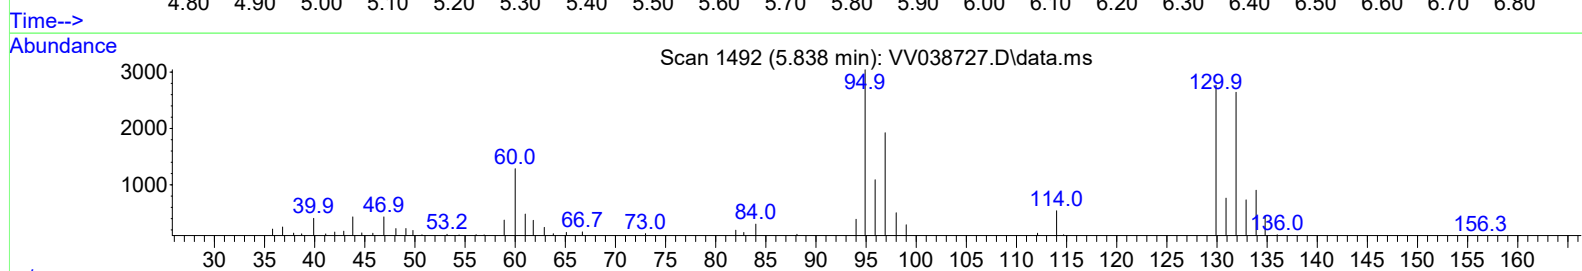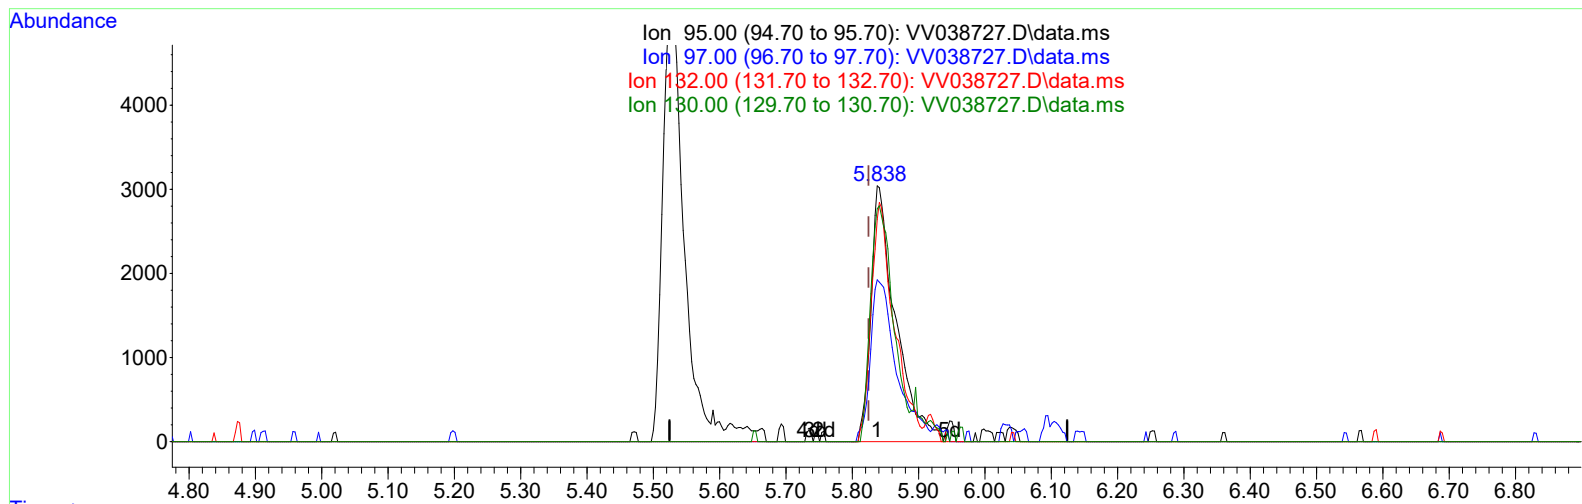

(34) Trichloroethene (T)




5.838min (+ 0.013) 2.46 ug/L m

response 7898

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	65.20	63.27
132.00	96.60	86.88
130.00	101.20	91.06

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

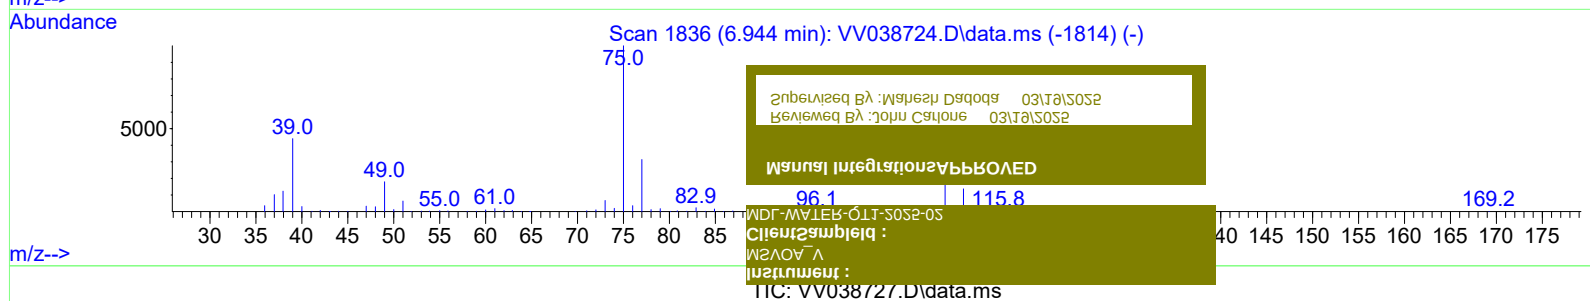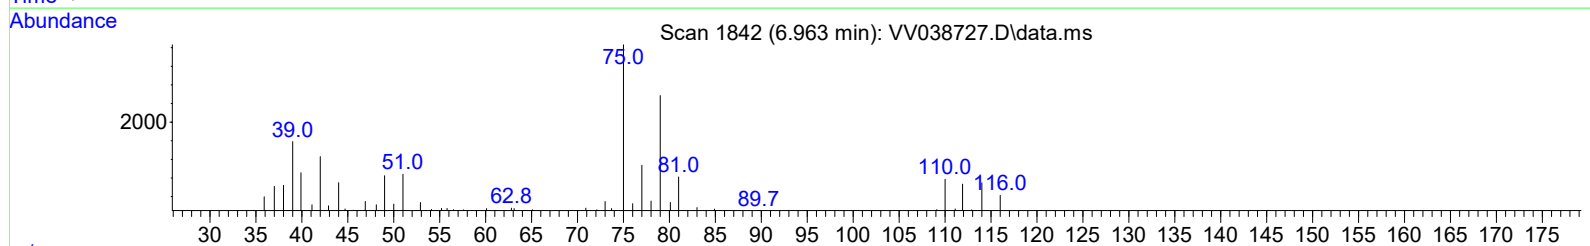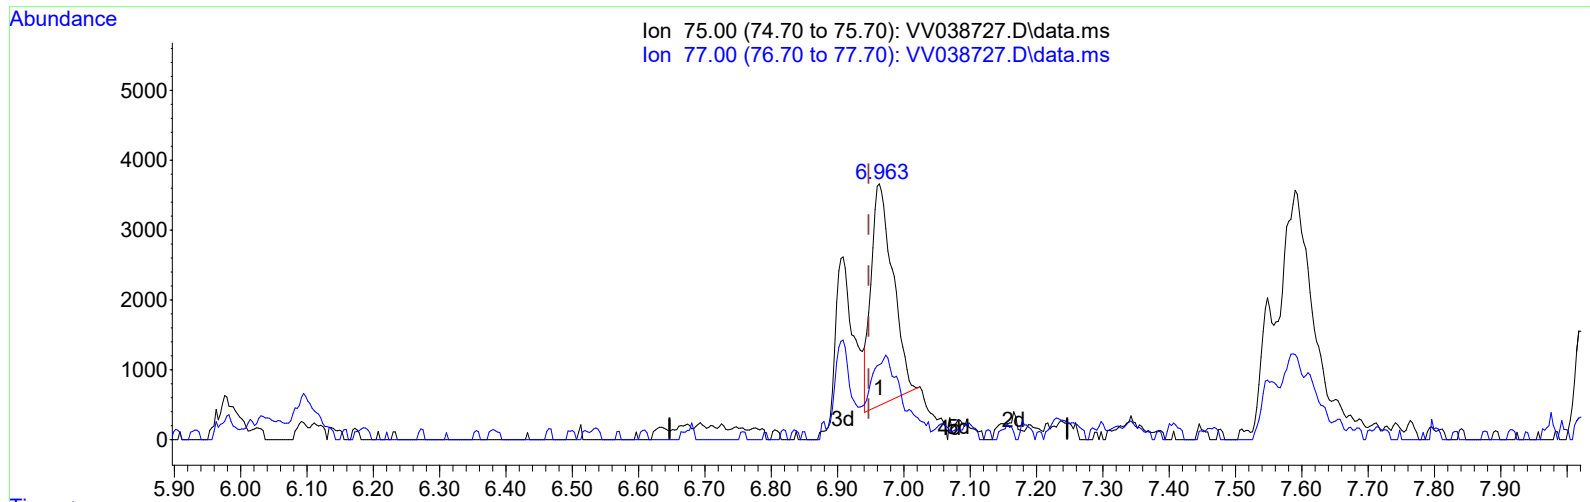

(39) cis-1,3-Dichloropropene (T)




6.963min (+ 0.016) 1.45 ug/L

response 7216

Ion	Exp%	Act%
75.00	100.00	100.00
77.00	31.30	29.33
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

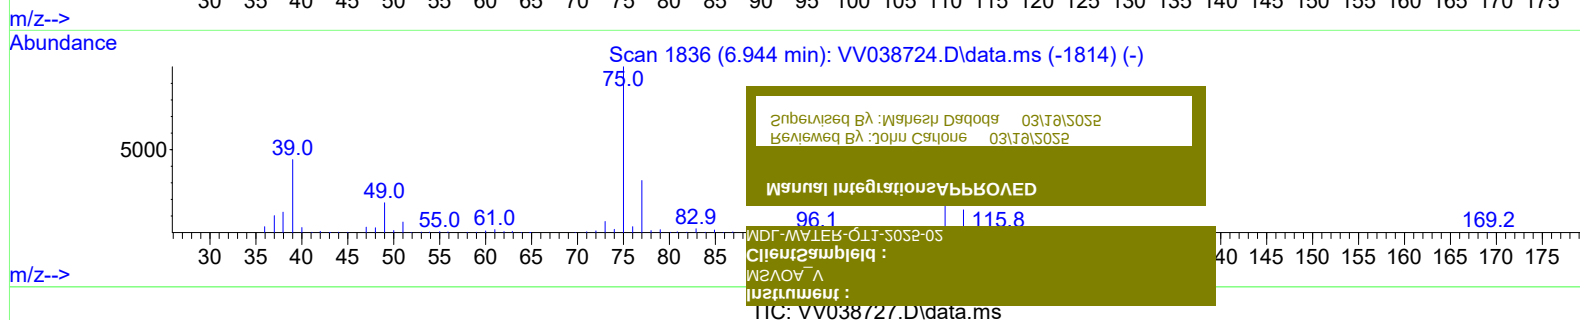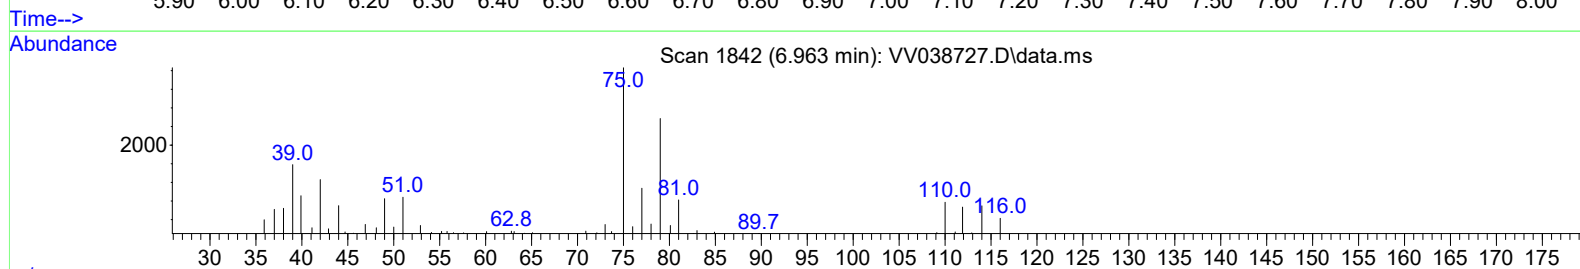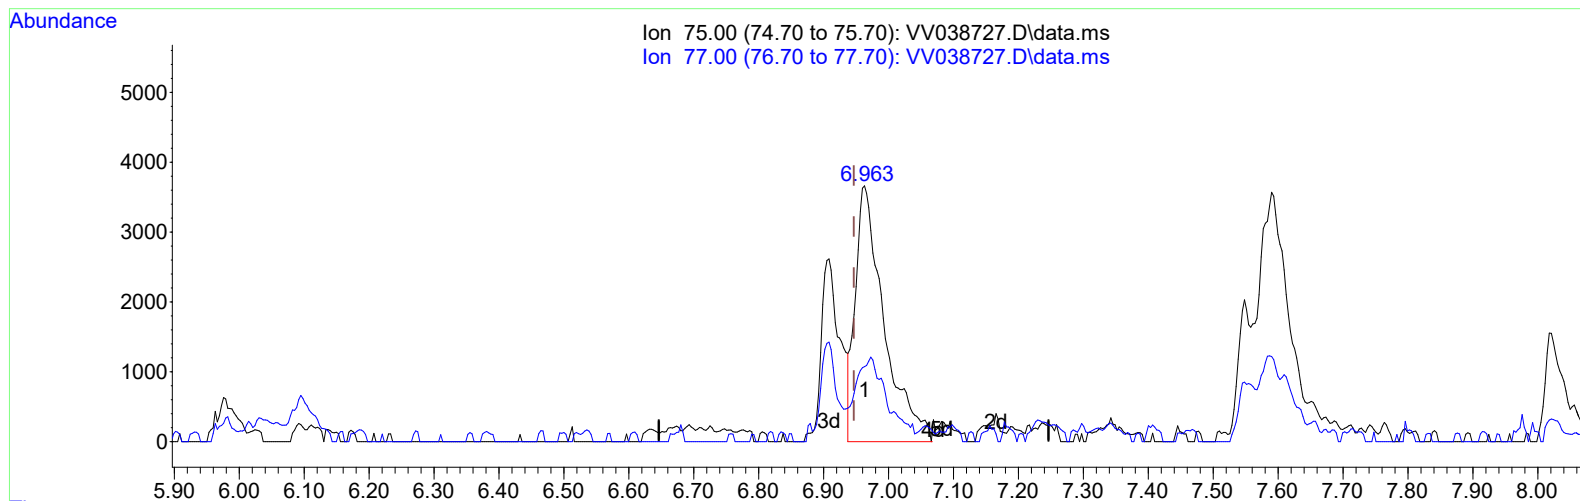

(39) cis-1,3-Dichloropropene (T)




6.963min (+ 0.016) 2.25 ug/L m

response 11235

Ion	Exp%	Act%
75.00	100.00	100.00
77.00	31.30	29.33
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

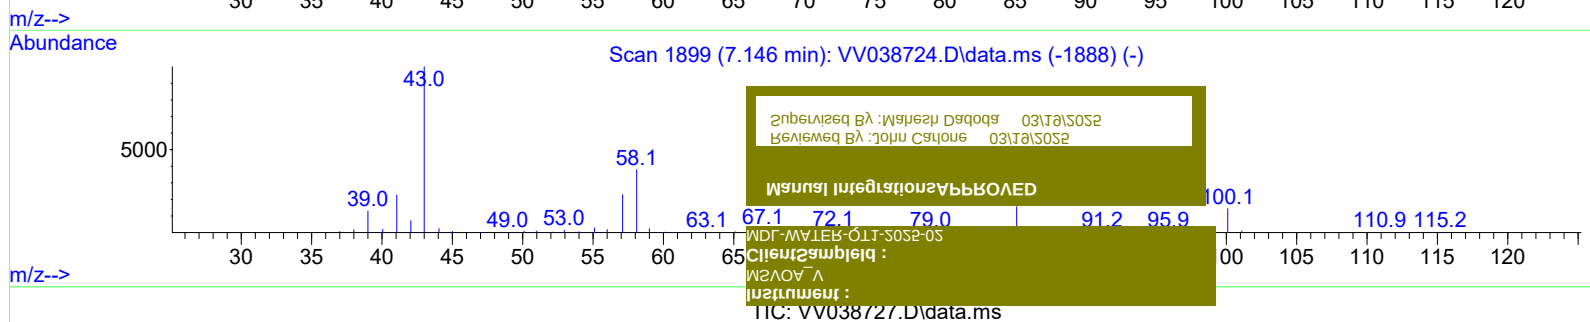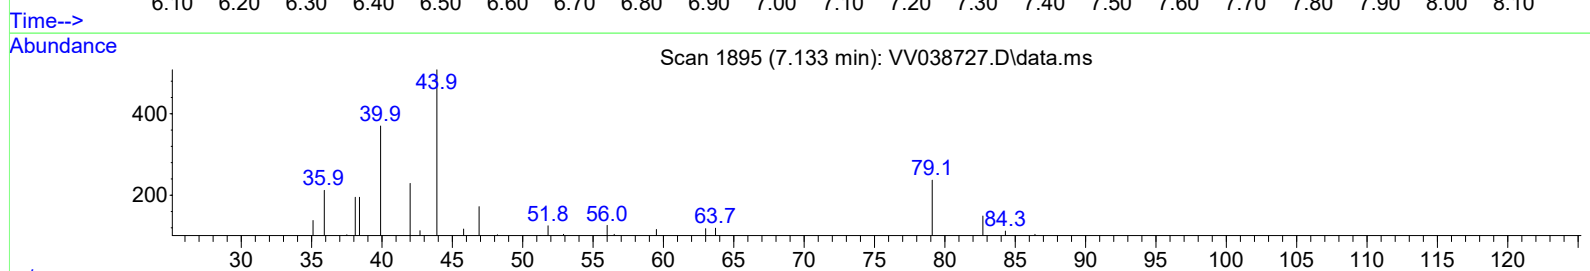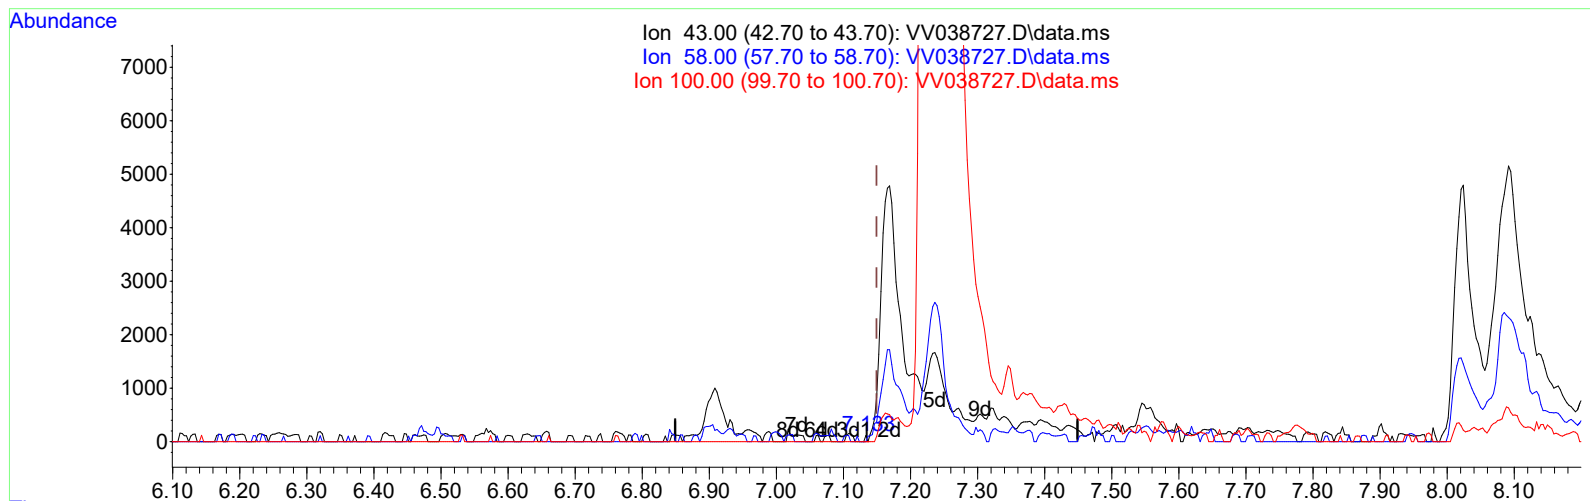

(40) 4-Methyl-2-pentanone (T)




7.133min (-0.016) 0.01 ug/L

response 22

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	40.90	0.00#
100.00	17.10	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

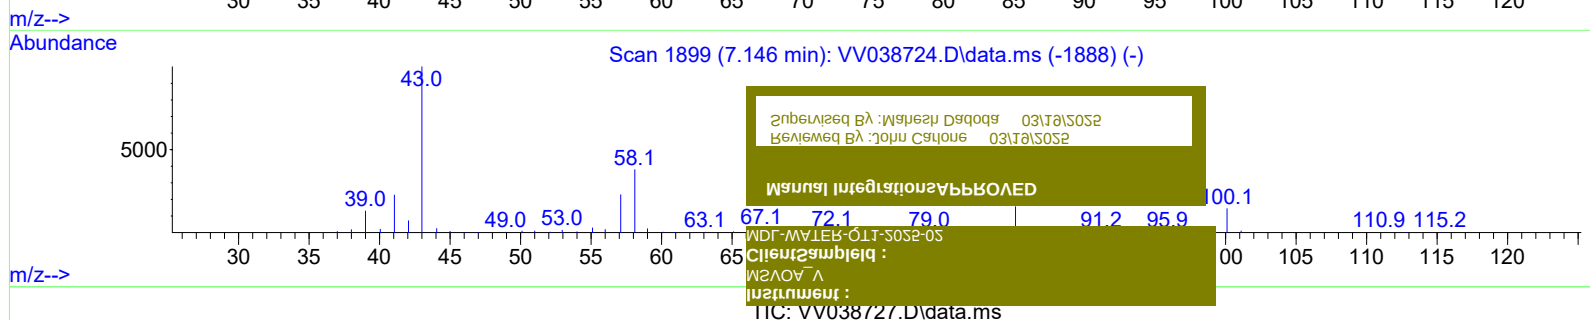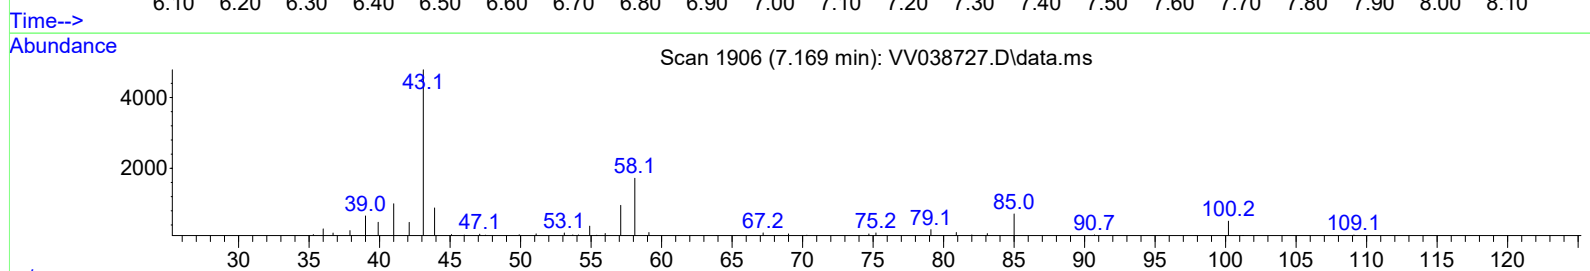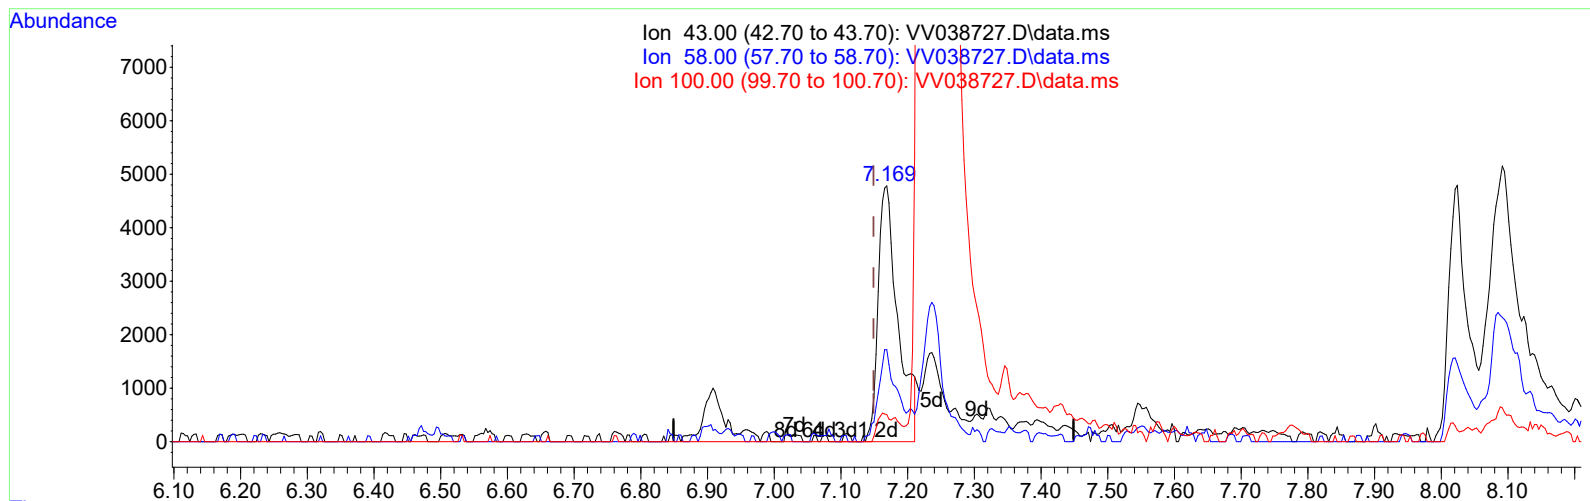

(40) 4-Methyl-2-pentanone (T)




7.169min (+ 0.019) 3.23 ug/L m

response 9973

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	40.90	0.00#
100.00	17.10	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

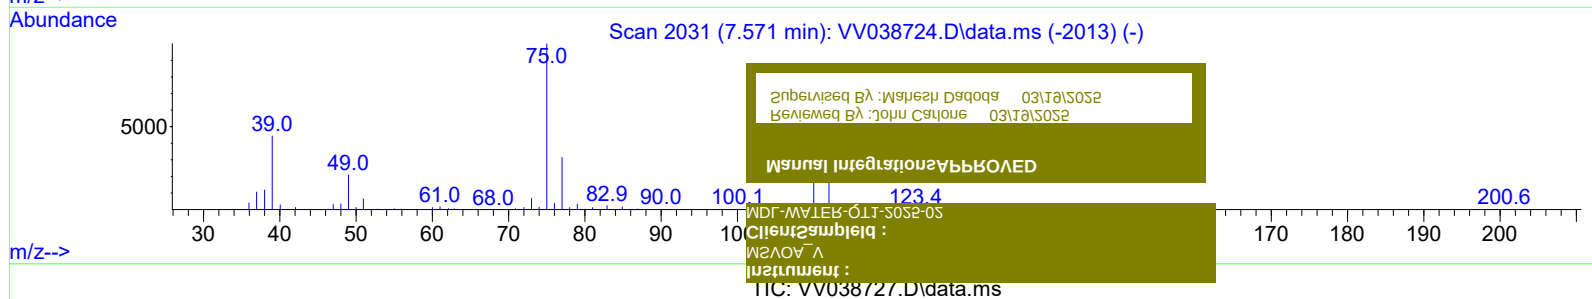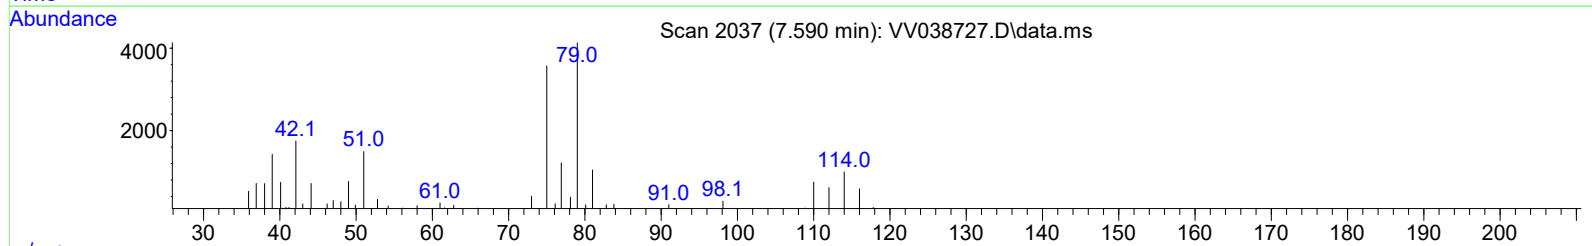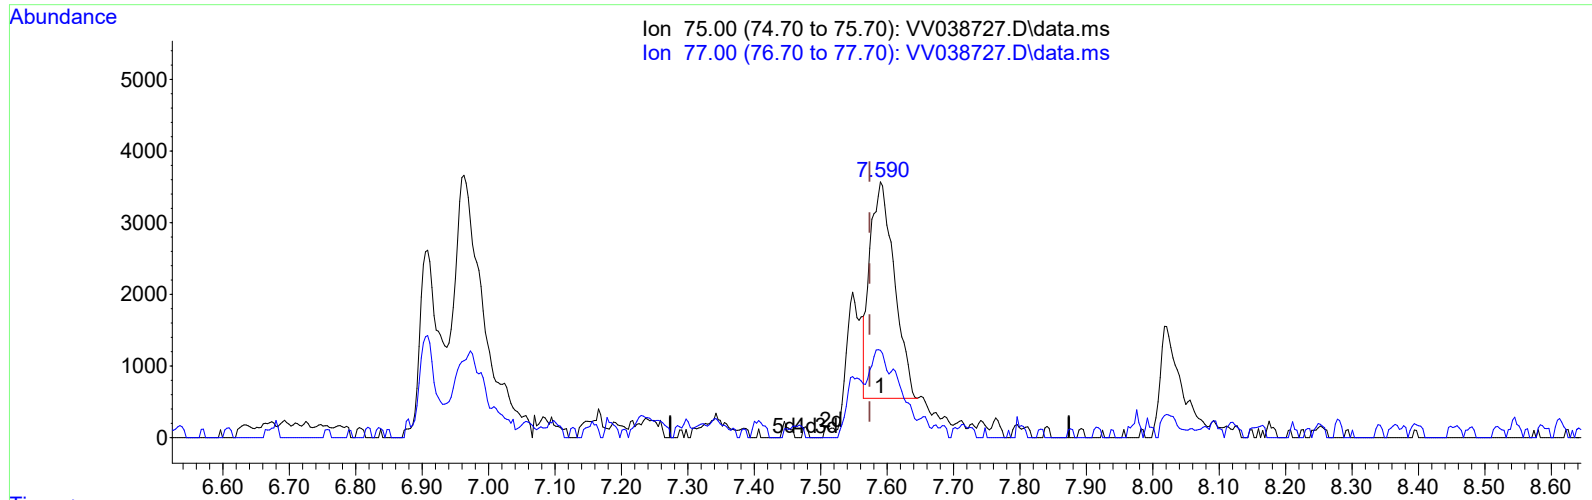

(44) trans-1,3-Dichloropropene (T)




7.590min (+ 0.016) 1.63 ug/L

response 7687

Ion	Exp%	Act%
75.00	100.00	100.00
77.00	32.40	34.15
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

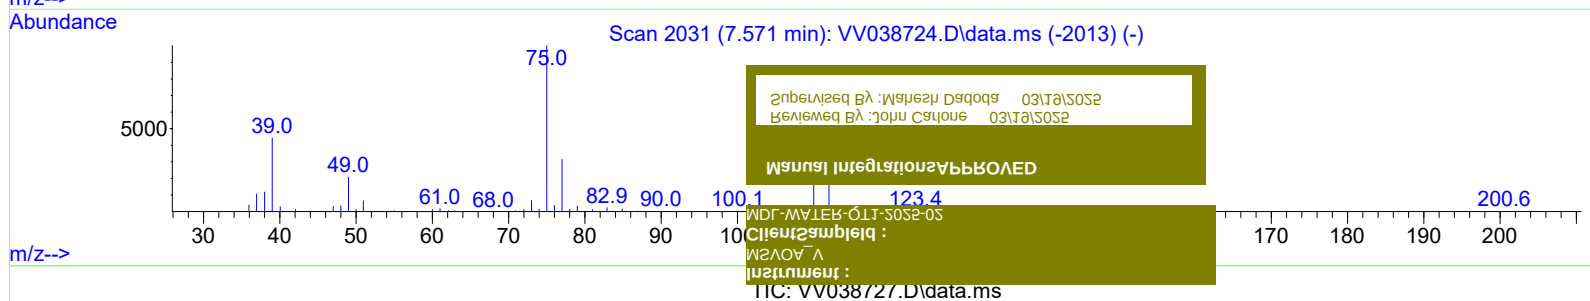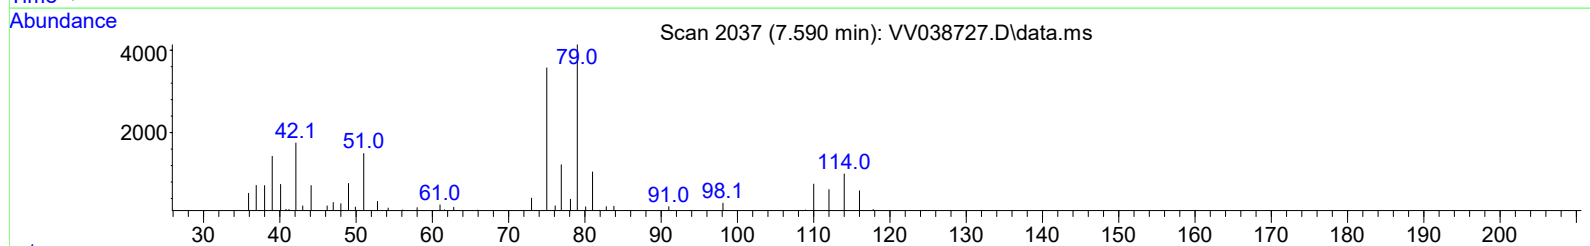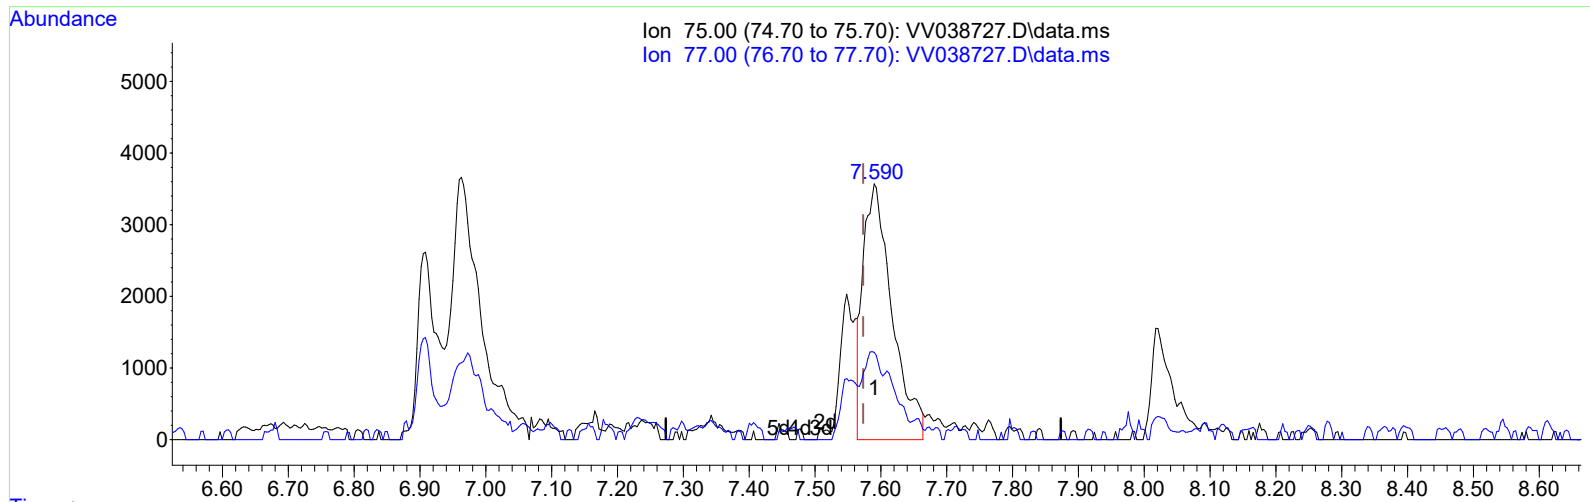

(44) trans-1,3-Dichloropropene (T)




7.590min (+ 0.016) 2.31 ug/L m

response 10912

Ion	Exp%	Act%
75.00	100.00	100.00
77.00	32.40	34.15
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

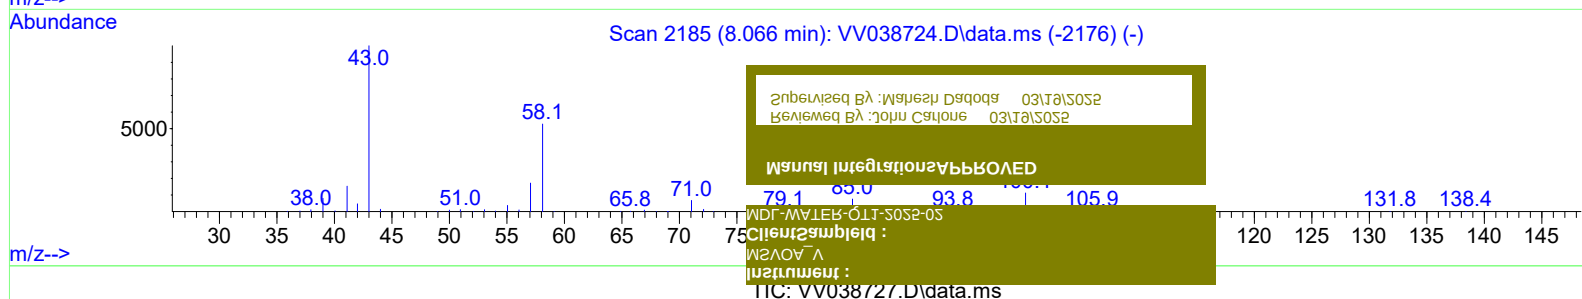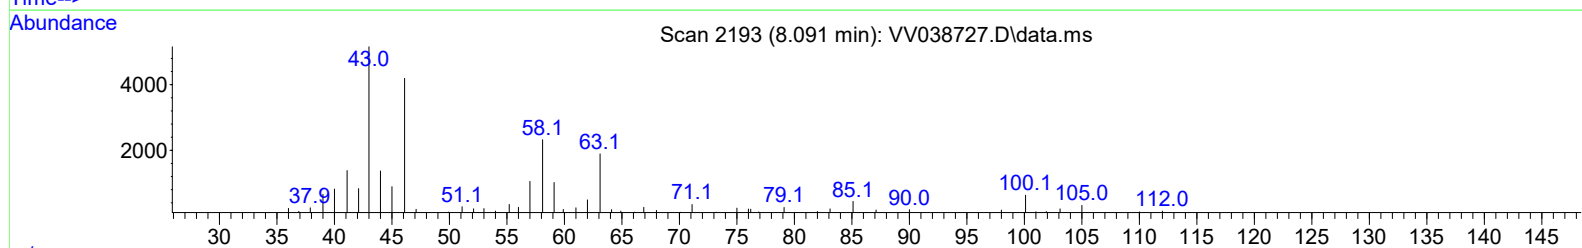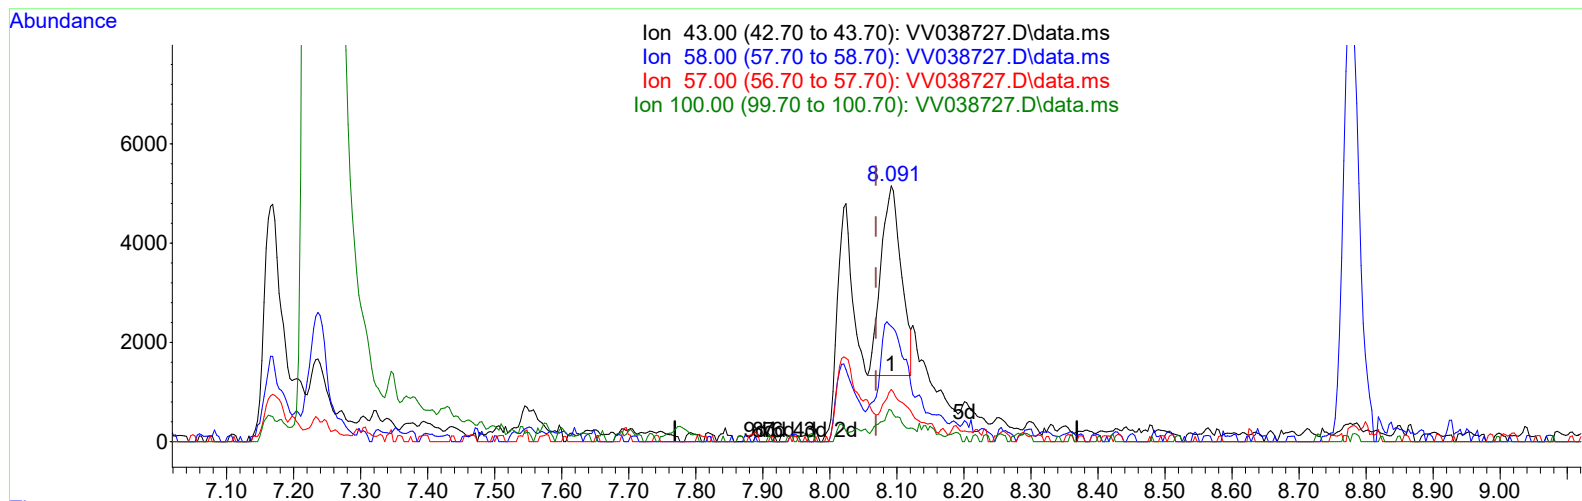

(48) 2-Hexanone (T)




8.091min (+ 0.023) 3.76 ug/L

response 8061

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	60.00	59.42
57.00	19.40	17.81
100.00	13.70	8.05#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038727.D
Acq On : 18 Mar 2025 10:26
Operator : SY/MD
Sample : Q1546-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 17 15:08:07 2025
Response via : Initial Calibration

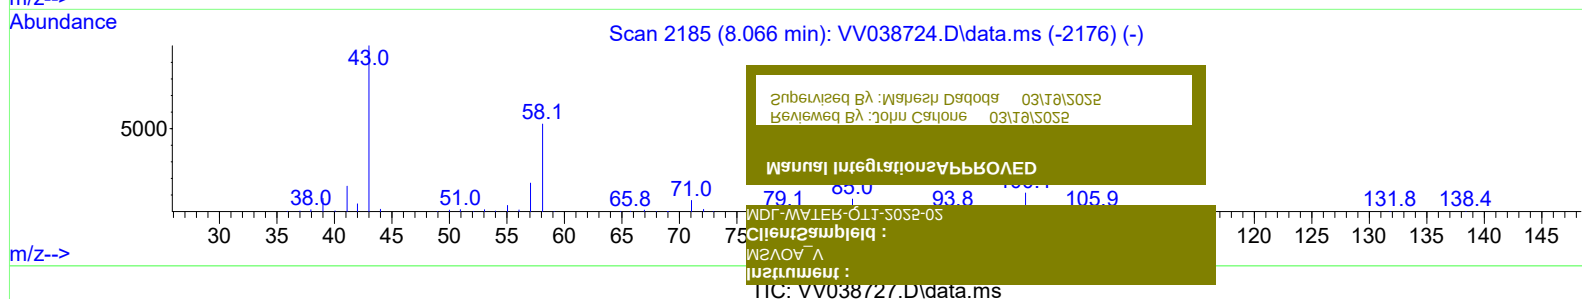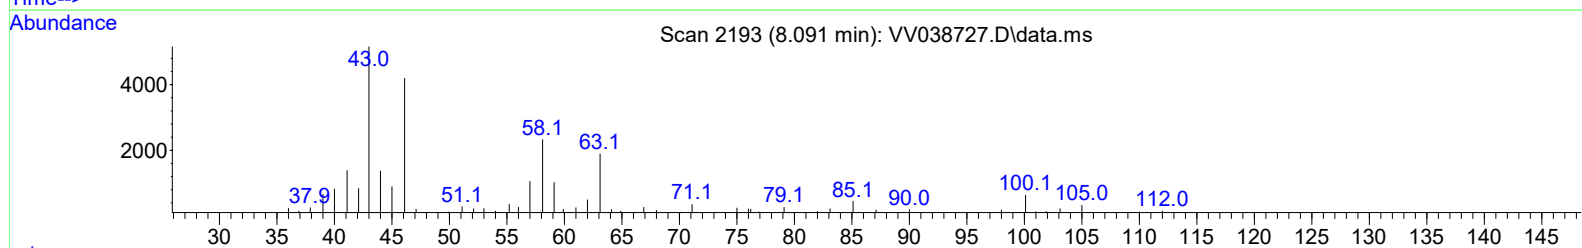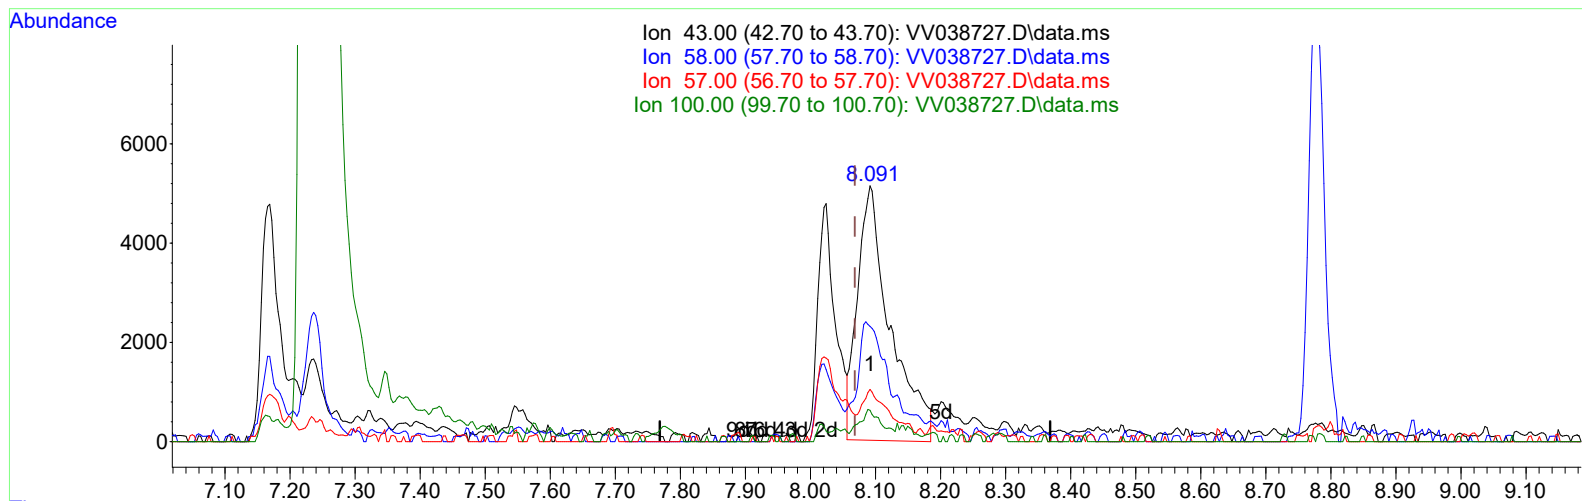

(48) 2-Hexanone (T)

8.091min (+ 0.023) 8.37 ug/L m

response 17941

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	60.00	26.70#
57.00	19.40	8.00#
100.00	13.70	3.62#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
 Data File : VV038727.D
 Acq On : 18 Mar 2025 10:26
 Operator : SY/MD
 Sample : Q1546-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 17 15:08:07 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	366491	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	393451	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	171804	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	170196	46.13	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	92.26%	
7) Chloroethane-d5	1.529	69	143014	46.24	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	92.48%	
11) 1,1-Dichloroethene-d2	2.053	65	74600	45.09	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	90.18%	
21) 2-Butanone-d5	3.786	46	113724	85.56	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	85.56%	
24) Chloroform-d	4.240	84	310627	46.57	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.14%	
26) 1,2-Dichloroethane-d4	4.931	65	189944	48.94	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.88%	
32) Benzene-d6	4.950	84	599560	48.13	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.26%	
36) 1,2-Dichloropropane-d6	5.979	67	201152	50.00	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	100.00%	
41) Toluene-d8	7.236	98	500592	46.25	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.50%	
43) trans-1,3-Dichloroprop...	7.548	79	75976	45.83	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.66%	
47) 2-Hexanone-d5	8.021	63	76873	92.37	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	106.00%	
56) 1,1,2,2-Tetrachloroeth...	10.143	84	229419			
Spiked Amount	50.000	Range 65 - 120	Recovery	=		
66) 1,2-Dichlorobenzene-d4	11.551	152	173811			
Spiked Amount	50.000	Range 80 - 120	Recovery	=		
Target Compounds						
2) Dichlorodifluoromethane	1.105	85	6789			
3) Chloromethane	1.214	50	8673	2.34	ug/L	94
5) Vinyl chloride	1.281	62	9972	2.59	ug/L #	70
6) Bromomethane	1.484	94	5412	2.69	ug/L	88
8) Chloroethane	1.545	64	6416	2.62	ug/L	97
9) Trichlorofluoromethane	1.709	101	11297	2.32	ug/L	92
10) 1,1,2-Trichloro-1,2,2-...	2.063	101	8950	3.06	ug/L #	83
12) 1,1-Dichloroethene	2.063	96	8405	3.06	ug/L #	1
13) Acetone	2.111	43	6209	4.75	ug/L	98
14) Carbon disulfide	2.236	76	21046	2.46	ug/L	100
15) Methyl Acetate	2.381	43	5749	2.20	ug/L #	75
17) trans-1,2-Dichloroethene	2.693	96	6373	2.20	ug/L	99
18) Methyl tert-butyl Ether	2.699	73	17385	2.14	ug/L #	78
19) 1,1-Dichloroethane	3.105	63	13643	2.24	ug/L	98
20) cis-1,2-Dichloroethene	3.818	96	7409	2.34	ug/L	95
22) 2-Butanone	3.918	43	9051m	5.89	ug/L	
23) Bromochloromethane	4.166	128	4026m	2.37	ug/L	
27) 1,2-Dichloroethane	5.050	62	11971m	2.73	ug/L	
29) Cyclohexane	4.568	56	9950	2.06	ug/L #	77

Submitted by: Magesh Dabodu 03/18/2025
 Reviewed by: John Canine 03/18/2025

Manual Integrations APPROVED

MDT-MATEB-011-5052-05
 Client Sampled:
 MSVOA_V
 Instrument:

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
 Data File : VV038727.D
 Acq On : 18 Mar 2025 10:26
 Operator : SY/MD
 Sample : Q1546-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 18 10:47:45 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 17 15:08:07 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
30) 1,1,1-Trichloroethane	4.503	97	11951m	2.37	ug/L	
31) Carbon tetrachloride	4.728	117	10286	2.37	ug/L	95
33) Benzene	5.008	78	28044	2.24	ug/L	100
34) Trichloroethene	5.838	95	7898m	2.46	ug/L	
35) Methylcyclohexane	6.043	83	8536	1.81	ug/L #	80
37) 1,2-Dichloropropane	6.098	63	6724	1.93	ug/L	97
38) Bromodichloromethane	6.436	83	10910	2.38	ug/L	93
39) cis-1,3-Dichloropropene	6.963	75	11235m	2.25	ug/L	
40) 4-Methyl-2-pentanone	7.169	43	9973m	3.23	ug/L	
42) Toluene	7.320	91	27579	2.16	ug/L	96
44) trans-1,3-Dichloropropene	7.590	75	10912m	2.31	ug/L	
45) 1,1,2-Trichloroethane	7.773	97	6958	2.12	ug/L	94
46) Tetrachloroethene	7.905	164	5088	2.23	ug/L	97
48) 2-Hexanone	8.091	43	17941m	8.37	ug/L	
49) Dibromochloromethane	8.178	129	7377	2.25	ug/L	94
50) 1,2-Dibromoethane	8.284	107	6784	2.12	ug/L	97
51) Chlorobenzene	8.815	112	19775	2.27	ug/L	90
52) Ethylbenzene	8.950	91	25581	1.82	ug/L	99
53) m,p-Xylene	9.075	106	8833	1.73	ug/L	91
54) o-Xylene	9.474	106	8585	1.73	ug/L	94
55) Styrene	9.503	104	11577	1.33	ug/L	97
57) 1,1,2,2-Tetrachloroethane	10.169	83	11992	2.45	ug/L #	97
59) Bromoform	9.667	173	3825	2.40	ug/L #	92
60) Isopropylbenzene	9.863	105	21910	2.03	ug/L	96
61) 1,2,3-Trichloropropane	10.207	75	7543	2.63	ug/L	93
62) 1,3,5-Trimethylbenzene	10.471	105	16571	1.98	ug/L	100
63) 1,2,4-Trimethylbenzene	10.850	105	15612	1.84	ug/L	98
64) 1,3-Dichlorobenzene	11.117	146	11986	Reviewed By: Matthew DeBodas 03/18/2025 Reviewed By: John Carione 03/18/2025 Manual Integrations APPROVED		
65) 1,4-Dichlorobenzene	11.201	146	13274			
67) 1,2-Dichlorobenzene	11.570	146	13807			
68) 1,2-Dibromo-3-chloropr...	12.371	75	2208	2.20	ug/L	95
69) 1,3,5-Trichlorobenzene	12.583	180	7346	MDT-MATEB-01T-5052-05 Client Sample ID : MS/MS V Instrument :		
70) 1,2,4-trichlorobenzene	13.204	180	6412			
71) Naphthalene	13.448	128	17476			
72) 1,2,3-Trichlorobenzene	13.676	180	6206			

(#) = qualifier out of range (m) = manual integration (+) = signals summed