
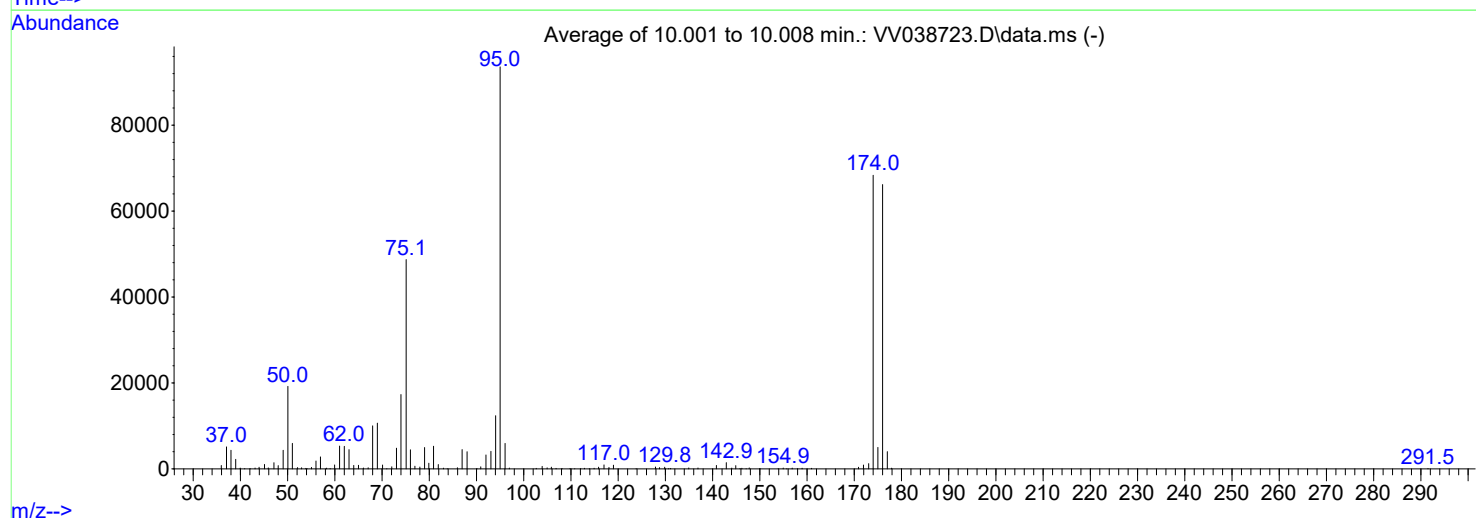


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031825\
Data File : VV038723.D
Acq On : 18 Mar 2025 07:53
Operator : SY/MD
Sample : BFB201
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB201

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
Title : VOC Analysis
Last Update : Mon Mar 17 15:08:07 2025

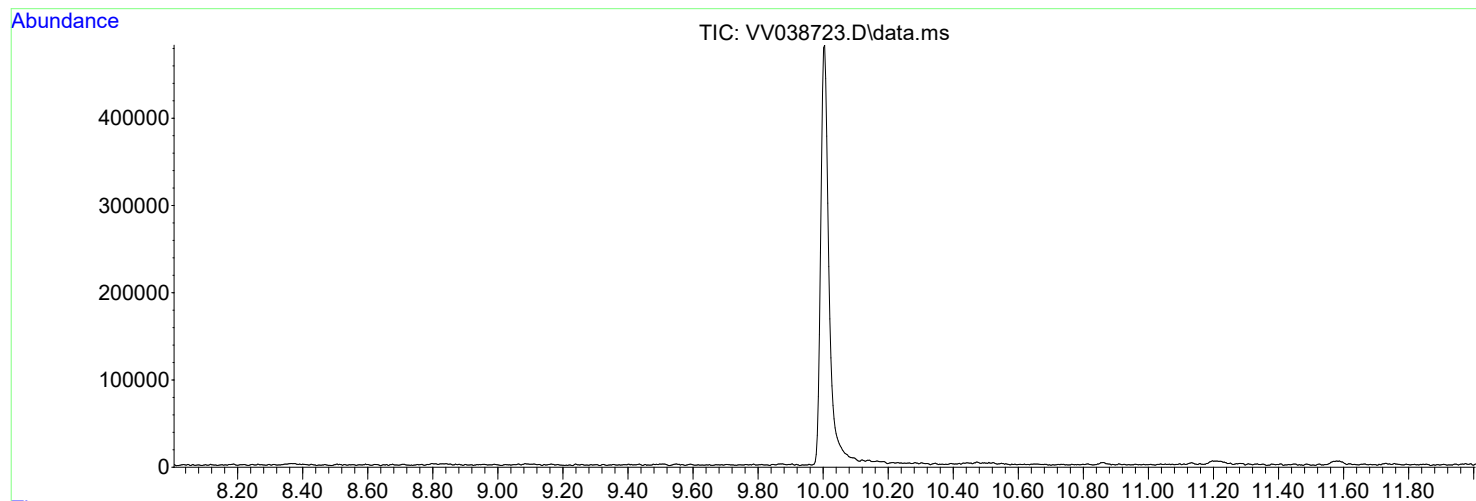

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	19205	PASS
75	95	30	80	52.1	48715	PASS
95	95	100	100	100.0	93568	PASS
96	95	5	9	6.3	5924	PASS
173	174	0.00	2	1.8	1226	PASS
174	95	50	120	73.0	68341	PASS
175	174	5	9	7.3	4998	PASS
176	174	95	105	96.8	66181	PASS
177	176	5	10	6.1	4012	PASS

m/z	Abundance
35.90	143.0
37.00	163.0
38.10	165.0
40.00	312.0
41.30	101.0
44.00	688.0
49.70	157.0
56.90	133.0
58.00	120.0
64.90	123.0
71.30	100.0
76.90	164.0
78.00	102.0
81.90	107.0

BEBS01
Client Sample :
MS/MS
Instrument :

m/z	Abundance
36.00	984.0
37.10	5541.0
38.00	4839.0
39.00	2347.0
40.00	477.0
40.90	198.0
42.10	100.0
43.10	216.0
43.90	911.0
45.10	1051.0
45.90	310.0
47.10	1388.0
48.00	740.0
49.00	4373.0
50.00	20024.0
51.00	6331.0
52.10	308.0
52.90	211.0
53.80	196.0
55.00	376.0
56.00	2051.0
57.00	2975.0
58.30	183.0
59.00	115.0
60.00	958.0
61.00	5633.0
62.00	5391.0
63.00	4841.0
64.00	788.0
65.10	927.0
66.00	212.0
67.10	312.0
68.00	10692.0
69.00	11161.0
70.10	993.0
71.00	144.0
72.10	518.0
73.00	4842.0
74.00	17656.0
75.10	50096.0
76.00	4651.0
77.00	816.0
78.00	482.0
79.00	5381.0
79.90	1276.0
80.90	5372.0
81.90	1179.0
83.00	245.0
86.00	231.0
86.90	4849.0
88.00	3995.0
90.10	102.0
90.90	529.0
92.00	3224.0
93.10	4283.0
94.10	12956.0
95.00	95376.0
96.10	6317.0
96.90	169.0
102.60	139.0
103.90	598.0
104.90	229.0
105.90	451.0
106.80	120.0
112.10	112.0
112.90	120.0
113.90	111.0
115.00	193.0
115.80	437.0
117.00	897.0
118.10	334.0
119.00	921.0
127.90	485.0
128.80	288.0
129.80	456.0
130.70	194.0
131.10	180.0
134.90	184.0
136.90	204.0
140.80	786.0
142.90	1466.0
144.10	266.0
144.90	849.0
146.20	148.0
147.10	104.0
147.70	238.0
153.90	148.0
154.90	194.0
155.70	104.0
156.80	191.0
158.90	142.0
161.00	175.0

BEBSOT
ClientSampleId :
MS/MS
Instrument :

170.90	351.0
171.90	852.0
173.10	1369.0
174.00	68264.0
175.00	4923.0
176.00	66232.0
177.00	4005.0
177.90	194.0
291.50	105.0

BEBSOT
Client :
MSAOA
Instrument :

m/z	Abundance
36.00	930.0
37.10	5508.0
38.00	4582.0
39.00	2322.0
39.90	516.0
41.40	117.0
43.10	211.0
44.00	1099.0
45.10	1068.0
45.90	245.0
47.10	1499.0
48.00	802.0
49.00	4540.0
50.10	19864.0
51.00	6025.0
52.10	323.0
52.90	279.0
53.90	182.0
55.10	348.0
56.00	1874.0
57.00	3006.0
58.30	180.0
59.00	103.0
59.90	931.0
61.00	5492.0
62.00	5460.0
63.00	4515.0
64.00	842.0
65.10	1005.0
66.10	215.0
67.10	267.0
68.00	10331.0
69.00	11071.0
70.10	931.0
71.20	132.0
72.10	462.0
73.10	4923.0
74.00	17712.0
75.10	49976.0
76.00	4592.0
77.00	828.0
78.00	576.0
79.00	5054.0
79.90	1362.0
80.90	5339.0
81.90	1160.0
83.00	174.0
86.00	274.0
87.00	4632.0
88.00	4127.0
90.90	496.0
92.00	3417.0
93.10	4127.0
94.00	12864.0
95.00	96440.0
96.10	6006.0
96.90	215.0
102.60	136.0
103.90	597.0
105.00	261.0
105.80	398.0
106.80	138.0
108.20	117.0
109.80	107.0
112.00	109.0
112.90	146.0
114.90	143.0
115.80	408.0
117.00	965.0
118.00	352.0
119.00	894.0
127.90	481.0
128.80	332.0
129.90	401.0
131.10	160.0
135.00	222.0
136.90	221.0
140.80	833.0
142.90	1485.0
144.10	182.0
144.90	805.0
145.90	143.0
146.20	153.0
147.80	237.0
150.00	135.0
155.00	195.0
156.80	203.0
159.00	178.0
160.90	140.0
170.90	398.0
171.90	966.0
173.00	1214.0

BEBSOT
Client Sample ID :
MS/MS
Instrument :

174.00	70328.0
175.00	5210.0
176.00	68400.0
177.00	4123.0
177.90	179.0
291.50	102.0

BEBST
Client :
MSAOA
Instrument :

m/z	Abundance
36.00	886.0
37.10	4802.0
38.00	4062.0
39.00	1997.0
40.00	497.0
41.40	135.0
42.00	113.0
43.10	192.0
44.00	1224.0
45.10	976.0
45.90	144.0
47.10	1442.0
48.00	747.0
49.10	4076.0
50.00	17728.0
51.00	5457.0
52.10	291.0
53.00	312.0
54.10	220.0
55.10	309.0
56.00	1587.0
57.00	2782.0
58.20	171.0
59.90	859.0
61.00	4816.0
62.00	4900.0
63.00	4104.0
64.00	814.0
65.00	959.0
66.10	202.0
66.90	236.0
68.00	9036.0
69.00	9699.0
70.10	796.0
71.20	131.0
71.90	487.0
73.10	4702.0
74.00	16544.0
75.10	46072.0
76.00	4082.0
77.00	739.0
78.00	545.0
79.00	4482.0
79.90	1320.0
80.90	5095.0
81.90	1021.0
82.90	108.0
83.80	109.0
85.90	289.0
87.00	3998.0
88.00	3863.0
90.90	427.0
92.00	3081.0
93.00	3834.0
94.00	11321.0
95.00	88888.0
96.00	5449.0
97.00	205.0
102.70	106.0
103.90	567.0
105.00	258.0
105.80	352.0
106.90	112.0
108.00	177.0
109.80	120.0
110.80	102.0
112.80	166.0
114.80	122.0
115.90	355.0
117.00	926.0
118.00	342.0
119.00	773.0
123.80	133.0
127.90	362.0
128.70	256.0
129.90	332.0
135.00	265.0
136.90	224.0
140.80	785.0
142.90	1405.0
143.90	128.0
144.90	635.0
145.70	142.0
146.20	142.0
147.80	226.0
150.00	161.0
154.90	201.0
156.90	175.0
158.00	135.0
159.00	169.0
160.90	109.0
170.90	401.0

BEBS01
ClientSampleId :
MS2A047
Instrument :

172.00	891.0
173.00	1094.0
174.00	66432.0
175.00	4860.0
176.00	63912.0
177.00	3908.0
177.90	153.0

BEB50T
ClientSampleId :
MS\OVL
Instrument :