

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034753.D
 Acq On : 20 Mar 2024 10:59
 Operator : SY/MD
 Sample : P1755-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 21 02:18:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 21 02:16:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	335526	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	315888	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	147328	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	117464	40.384	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.760%
7) Chloroethane-d5	1.532	69	102079	45.047	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.100%
11) 1,1-Dichloroethene-d2	2.060	65	55360	42.085	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.160%
21) 2-Butanone-d5	3.789	46	179849	92.461	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.460%
24) Chloroform-d	4.249	84	242437	47.141	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.280%
26) 1,2-Dichloroethane-d4	4.941	65	163759	48.728	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.460%
32) Benzene-d6	4.957	84	467430	49.030	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.060%
36) 1,2-Dichloropropane-d6	5.986	67	145878	50.139	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.280%
41) Toluene-d8	7.243	98	410687	47.602	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.200%
43) trans-1,3-Dichloroprop...	7.551	79	64652	44.251	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.500%
47) 2-Hexanone-d5	8.024	63	110505	76.060	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.060%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	193527	50.545	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.080%
66) 1,2-Dichlorobenzene-d4	11.558	152	154371	51.262	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.520%
Target Compounds						
39) cis-1,3-Dichloropropene	6.915	75	4649	1.118	ug/L	Qvalue # 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034753.D
Acq On : 20 Mar 2024 10:59
Operator : SY/MD
Sample : P1755-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 21 02:18:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 02:16:15 2024
Response via : Initial Calibration

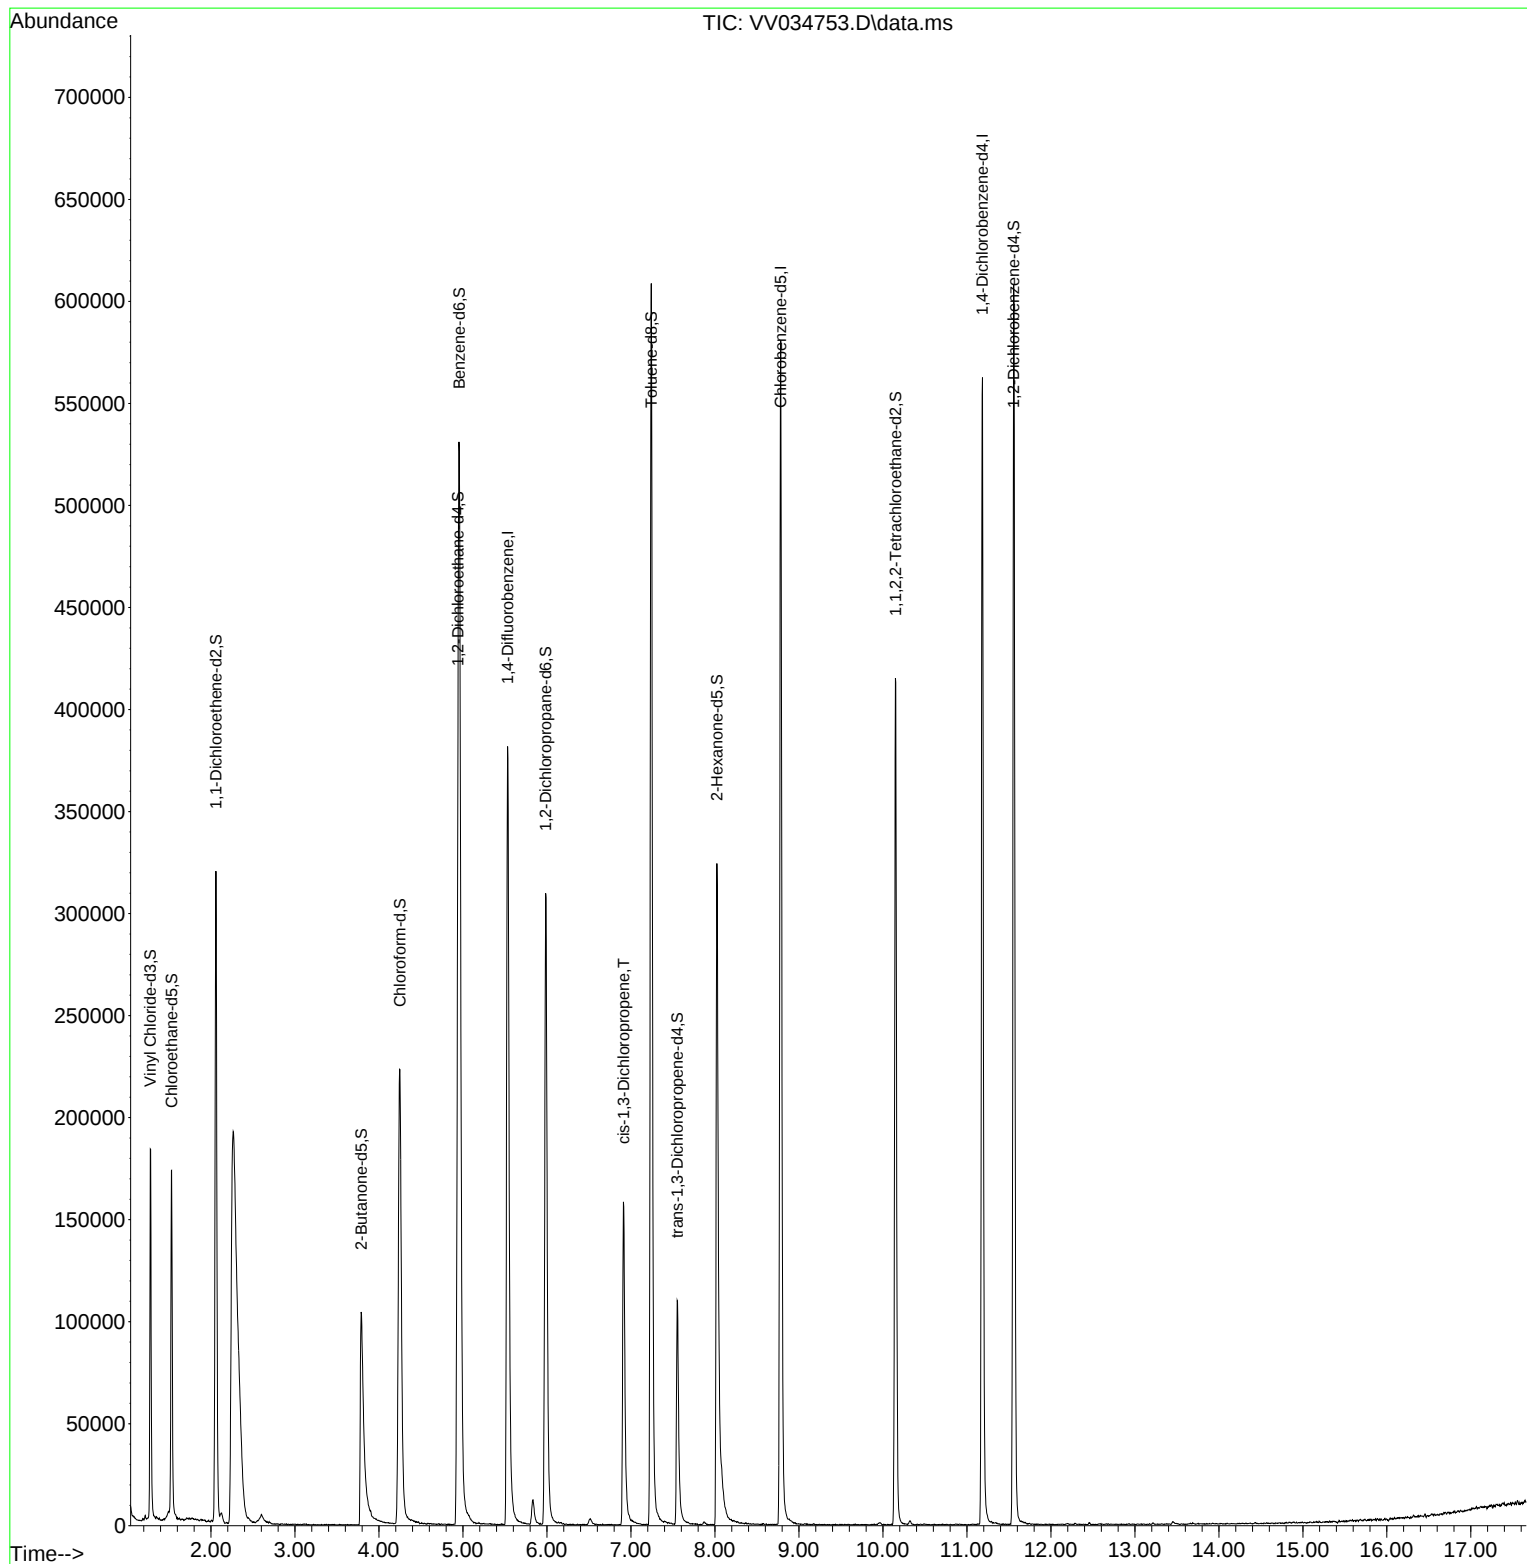

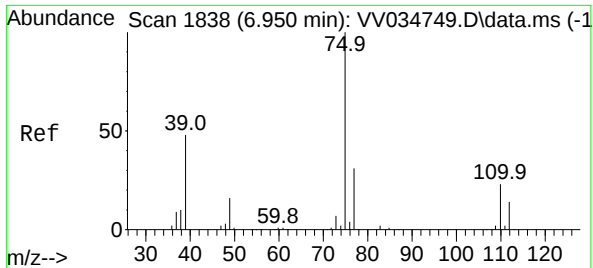

#39
 cis-1,3-Dichloropropene
 Concen: 1.118 ug/L
 RT: 6.915 min Scan# 11
 Delta R.T. -0.035 min
 Lab File: VV034753.D
 Acq: 20 Mar 2024 10:59

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 4649
 Ion Ratio Lower Upper
 75 100
 77 46.1 20.9 38.9#

