

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034755.D
 Acq On : 20 Mar 2024 11:46
 Operator : SY/MD
 Sample : P1755-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 21 02:18:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 21 02:16:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	335352	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	314223	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	147100	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	117269	40.338	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.680%		
7) Chloroethane-d5	1.532	69	100411	44.334	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.660%		
11) 1,1-Dichloroethene-d2	2.060	65	55200	41.985	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.980%		
21) 2-Butanone-d5	3.789	46	181782	93.503	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	93.500%		
24) Chloroform-d	4.249	84	234719	45.664	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.320%		
26) 1,2-Dichloroethane-d4	4.940	65	156224	46.510	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.020%		
32) Benzene-d6	4.960	84	448826	47.328	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.660%		
36) 1,2-Dichloropropane-d6	5.985	67	139261	48.118	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.240%		
41) Toluene-d8	7.243	98	395542	46.090	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.180%		
43) trans-1,3-Dichloroprop...	7.555	79	63626	43.779	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.560%		
47) 2-Hexanone-d5	8.024	63	106986	74.028	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	74.030%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	187746	49.295	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.580%		
66) 1,2-Dichlorobenzene-d4	11.561	152	152881	50.846	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.700%		
Target Compounds					Qvalue	
13) Acetone	2.117	43	223857	95.782	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034755.D
Acq On : 20 Mar 2024 11:46
Operator : SY/MD
Sample : P1755-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 21 02:18:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 02:16:15 2024
Response via : Initial Calibration

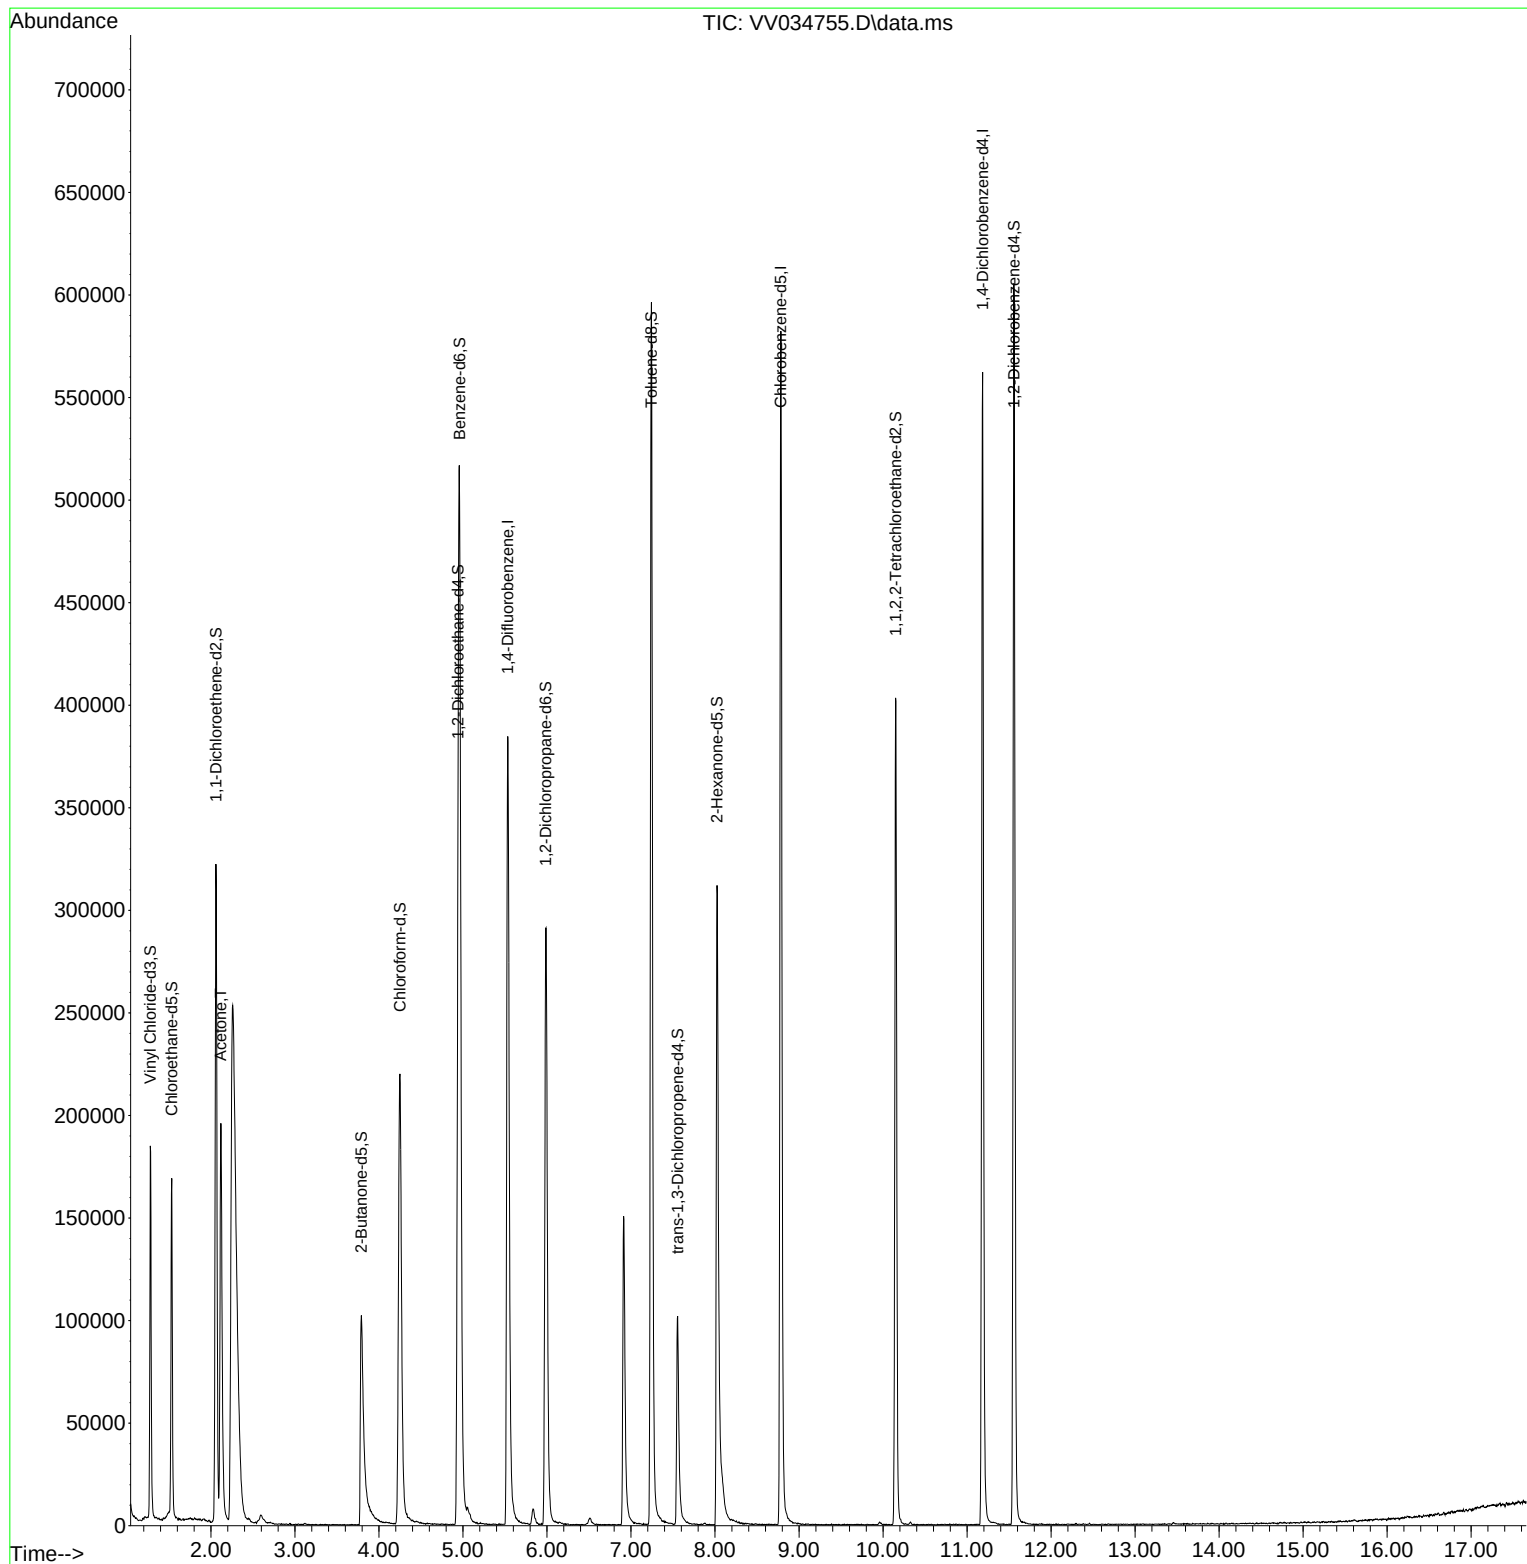

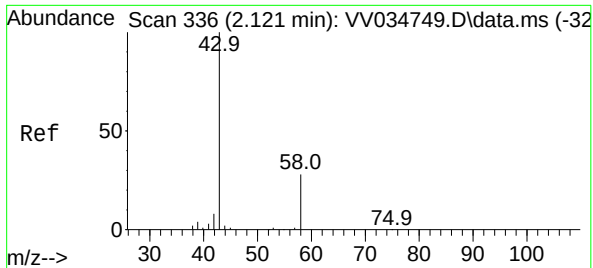

#13
 Acetone
 Concen: 95.782 ug/L
 RT: 2.117 min Scan# 34
 Delta R.T. -0.003 min
 Lab File: VV034755.D
 Acq: 20 Mar 2024 11:46

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 43 Resp: 223857
 Ion Ratio Lower Upper
 43 100
 58 28.7 0.0 57.2

