

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034757.D
 Acq On : 20 Mar 2024 12:33
 Operator : SY/MD
 Sample : P1755-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 21 02:19:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 21 02:16:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	337185	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	308367	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	147410	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	121730	41.645	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.280%		
7) Chloroethane-d5	1.529	69	105783	46.452	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.900%		
11) 1,1-Dichloroethene-d2	2.060	65	55789	42.202	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.400%		
21) 2-Butanone-d5	3.786	46	179522	91.839	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	91.840%		
24) Chloroform-d	4.249	84	245963	47.591	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.180%		
26) 1,2-Dichloroethane-d4	4.941	65	169226	50.107	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.220%		
32) Benzene-d6	4.960	84	477471	51.305	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.600%		
36) 1,2-Dichloropropane-d6	5.986	67	145300	51.158	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.320%		
41) Toluene-d8	7.243	98	405346	48.129	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.260%		
43) trans-1,3-Dichloroprop...	7.555	79	67119	47.060	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.120%		
47) 2-Hexanone-d5	8.024	63	110099	77.629	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	77.630%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	190513	50.971	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	101.940%		
66) 1,2-Dichlorobenzene-d4	11.558	152	155514	51.613	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.220%		
Target Compounds						
					Qvalue	
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	1961	0.720	ug/L #	20
13) Acetone	2.118	43	20619	8.774	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034757.D
Acq On : 20 Mar 2024 12:33
Operator : SY/MD
Sample : P1755-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 21 02:19:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 02:16:15 2024
Response via : Initial Calibration

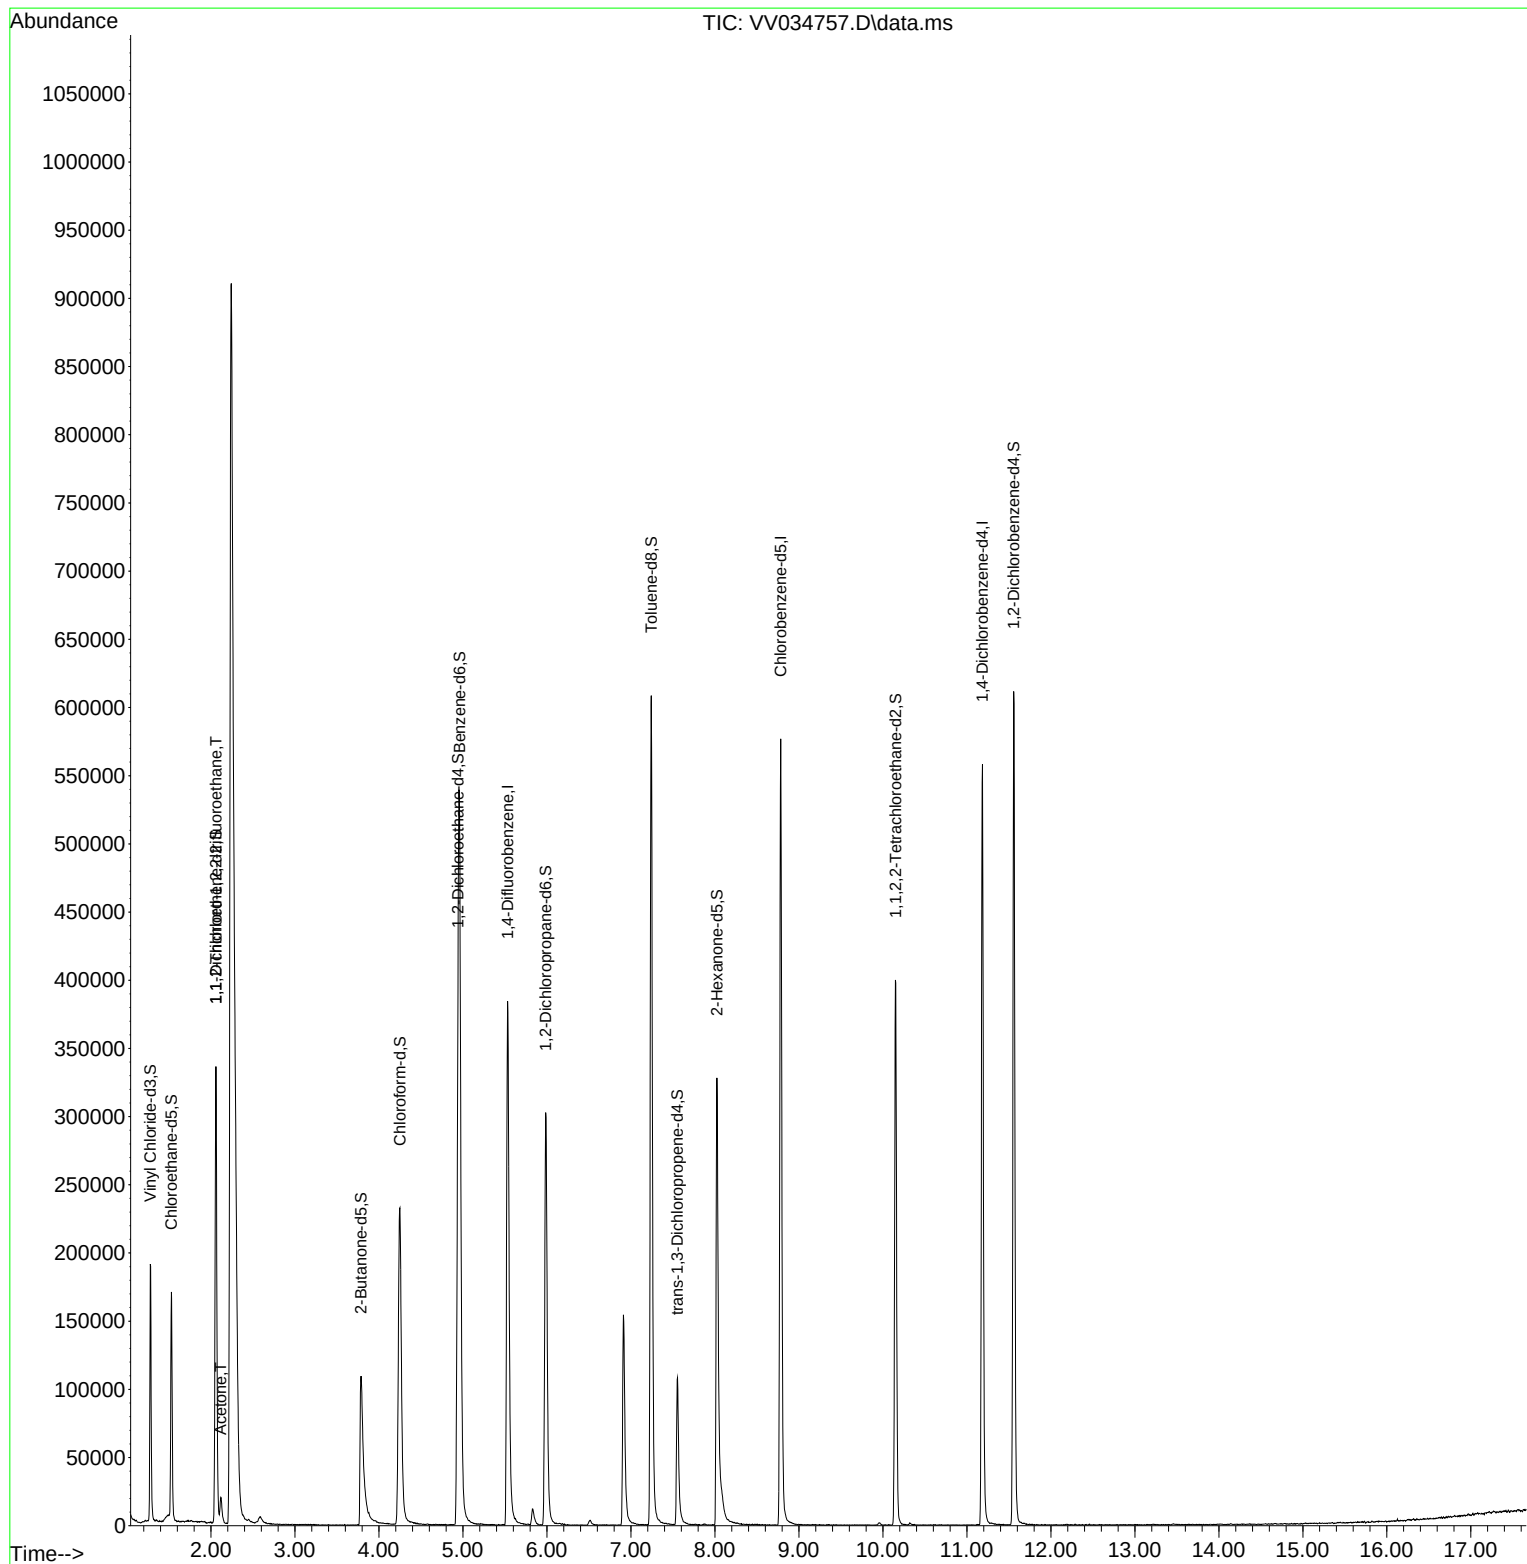

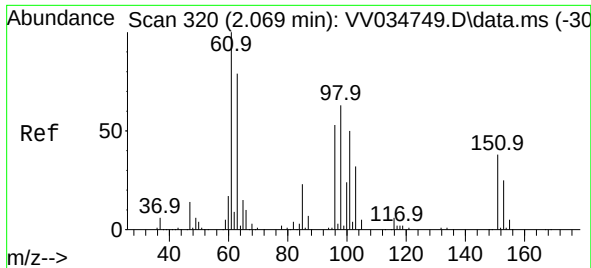

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.720 ug/L

RT: 2.060 min Scan# 317

Delta R.T. -0.009 min

Lab File: VV034757.D

Acq: 20 Mar 2024 12:33

Instrument :

MSVOA_V

ClientSampleId :





Tgt Ion:101 Resp: 1961

Ion Ratio Lower Upper

101 100

85 3.5 37.4 56.0#

151 0.0 61.4 92.2#

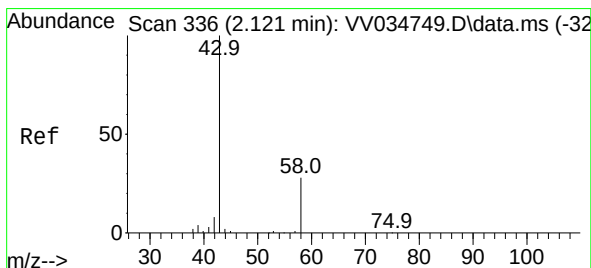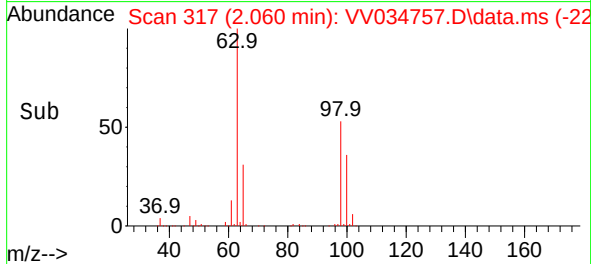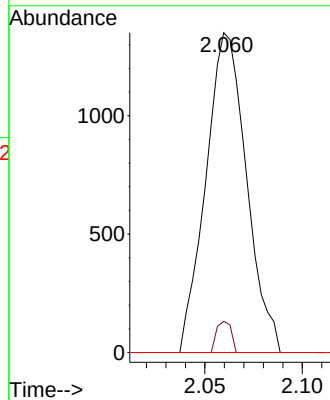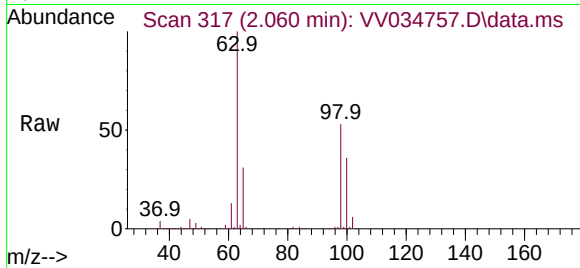

#13

Acetone

Concen: 8.774 ug/L

RT: 2.118 min Scan# 335

Delta R.T. -0.003 min

Lab File: VV034757.D

Acq: 20 Mar 2024 12:33

Tgt Ion: 43 Resp: 20619

Ion Ratio Lower Upper

43 100

58 30.0 0.0 57.2

