




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034758.D
Acq On : 20 Mar 2024 12:57
Operator : SY/MD
Sample : P1755-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKX1

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:19:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 02:16:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/22/2024
Supervised By :Semsettin Yesilyurt 03/22/2024

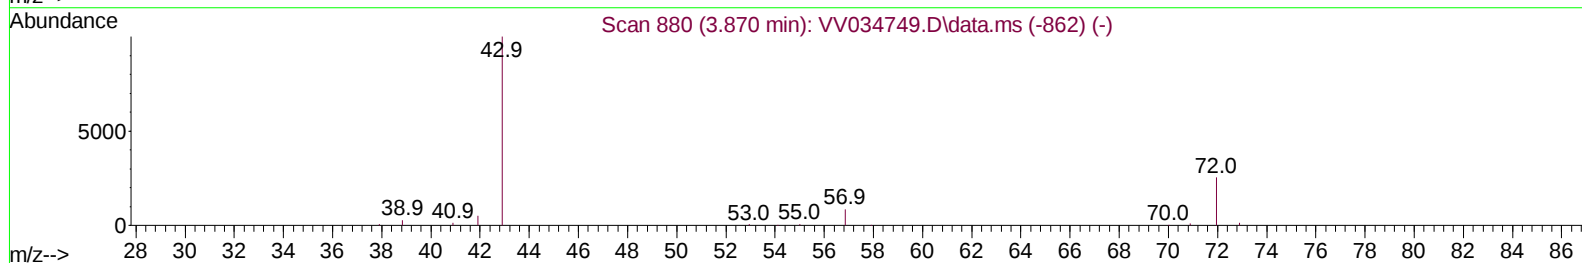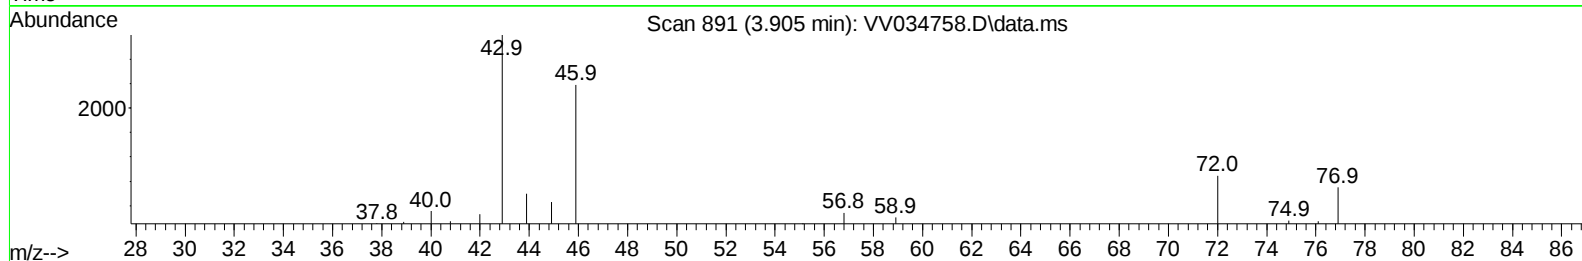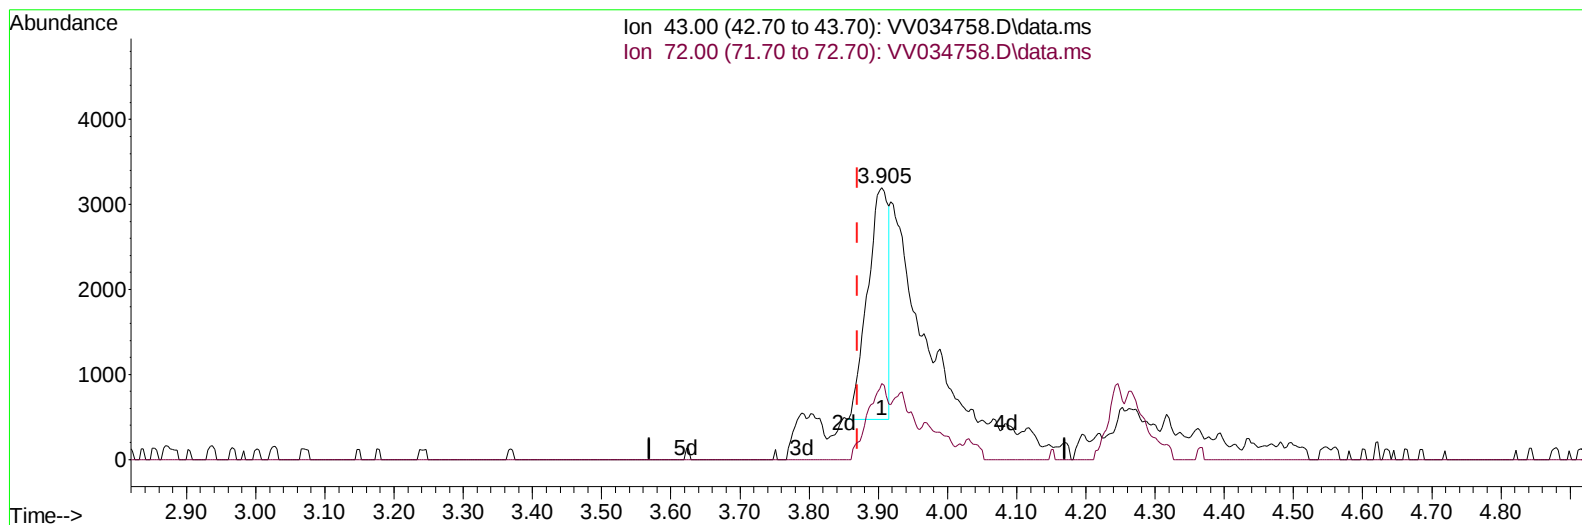

TIC: VV034758.D\data.ms

(22) 2-Butanone (T)

3.905min (+ 0.036) 2.49 ug/L

response 5672

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	22.90	33.96
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034758.D
Acq On : 20 Mar 2024 12:57
Operator : SY/MD
Sample : P1755-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKX1

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:19:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 02:16:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/22/2024
Supervised By :Semsettin Yesilyurt 03/22/2024

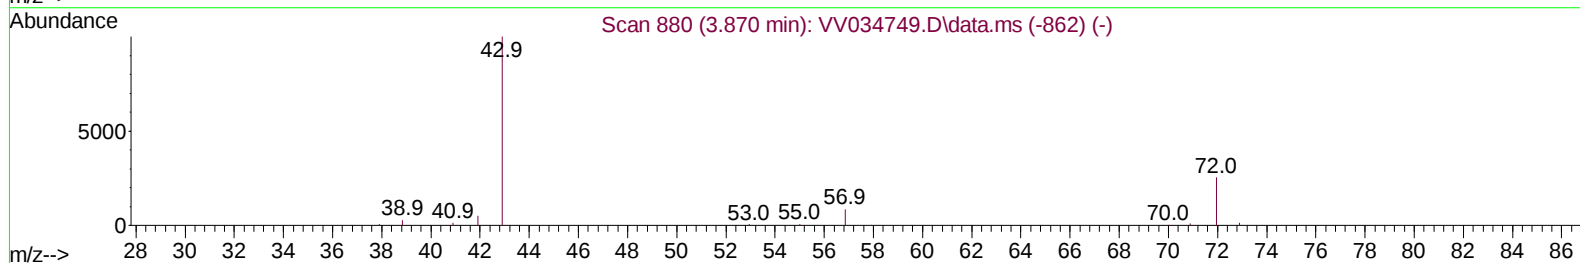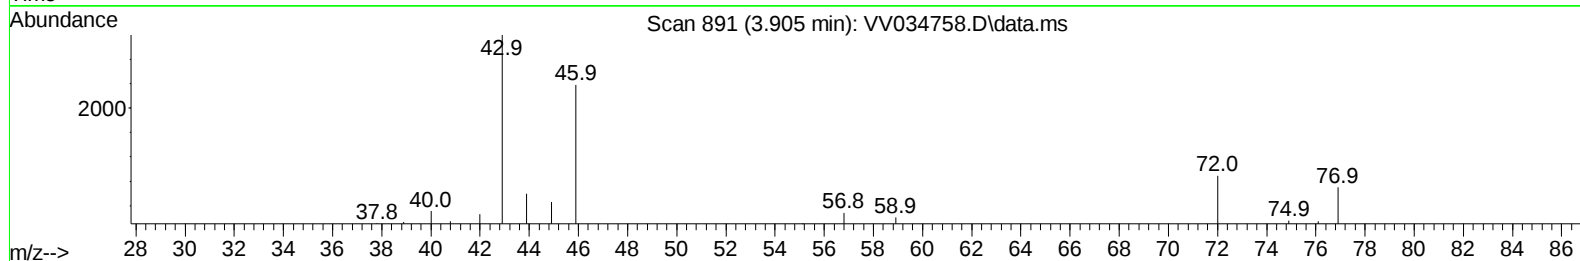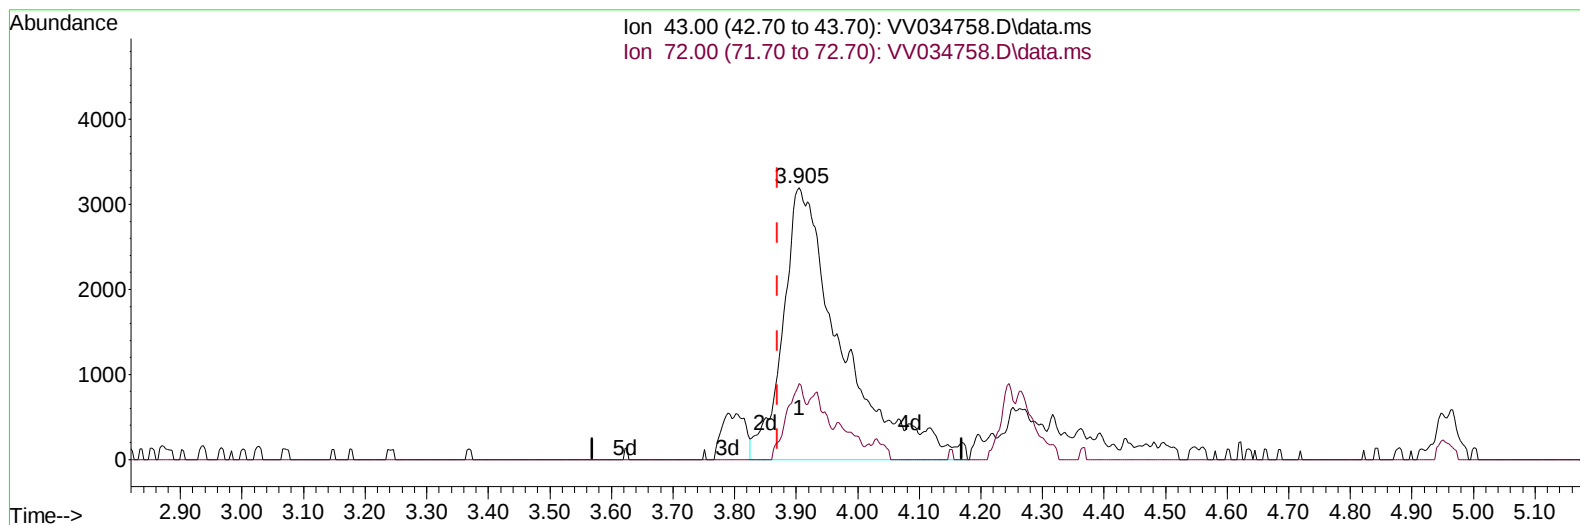

TIC: VV034758.D\data.ms

(22) 2-Butanone (T)

3.905min (+ 0.036) 9.28 ug/L m

response 21165

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	22.90	9.10#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034758.D
 Acq On : 20 Mar 2024 12:57
 Operator : SY/MD
 Sample : P1755-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX1

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:19:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 21 02:16:15 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/22/2024
 Supervised By :Semsettin Yesilyurt 03/22/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.532	114		331422	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117		310755	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		145514	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		112089	39.014	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery =	78.020%		
7) Chloroethane-d5	1.532	69		97925	43.749	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery =	87.500%		
11) 1,1-Dichloroethene-d2	2.060	65		52761	40.606	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery =	81.220%		
21) 2-Butanone-d5	3.789	46		184753	96.158	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery =	96.160%		
24) Chloroform-d	4.249	84		231841	45.639	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	91.280%		
26) 1,2-Dichloroethane-d4	4.941	65		158707	47.809	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	95.620%		
32) Benzene-d6	4.957	84		447909	47.758	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery =	95.520%		
36) 1,2-Dichloropropane-d6	5.986	67		141490	49.434	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery =	98.860%		
41) Toluene-d8	7.243	98		396380	46.703	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery =	93.400%		
43) trans-1,3-Dichloroprop...	7.551	79		63447	44.143	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery =	88.280%		
47) 2-Hexanone-d5	8.024	63		111123	77.749	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery =	77.750%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84		188418	50.023	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery =	100.040%		
66) 1,2-Dichlorobenzene-d4	11.561	152		150690	50.663	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery =	101.320%		
Target Compounds							
13) Acetone	2.121	43		111269	48.173	ug/L	99
22) 2-Butanone	3.905	43		21165m	9.279	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034758.D
Acq On : 20 Mar 2024 12:57
Operator : SY/MD
Sample : P1755-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKX1

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:19:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 02:16:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/22/2024
Supervised By :Semsettin Yesilyurt 03/22/2024

