

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW032024\
 Data File : VW034751.D
 Acq On : 20 Mar 2024 10:11
 Operator : SY/MD
 Sample : P1755-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKW1

Quant Time: Mar 21 02:17:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 21 02:16:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	363483	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	325825	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	151197	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	128262	40.705	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.400%		
7) Chloroethane-d5	1.529	69	106727	43.476	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.960%		
11) 1,1-Dichloroethene-d2	2.060	65	59309	41.619	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.240%		
21) 2-Butanone-d5	3.786	46	177119	84.054	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.050%		
24) Chloroform-d	4.246	84	251822	45.200	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.400%		
26) 1,2-Dichloroethane-d4	4.937	65	170538	46.842	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.680%		
32) Benzene-d6	4.957	84	490538	49.884	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.760%		
36) 1,2-Dichloropropane-d6	5.986	67	150667	50.206	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.420%		
41) Toluene-d8	7.239	98	416248	46.775	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.560%		
43) trans-1,3-Dichloroprop...	7.551	79	66047	43.827	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.660%		
47) 2-Hexanone-d5	8.024	63	102468	68.378	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	68.380%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	185224	46.901	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.800%		
66) 1,2-Dichlorobenzene-d4	11.558	152	157537	50.974	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.940%		
Target Compounds					Qvalue	
13) Acetone	2.118	43	279285	110.250	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034751.D
Acq On : 20 Mar 2024 10:11
Operator : SY/MD
Sample : P1755-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKW1

Quant Time: Mar 21 02:17:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 21 02:16:15 2024
Response via : Initial Calibration

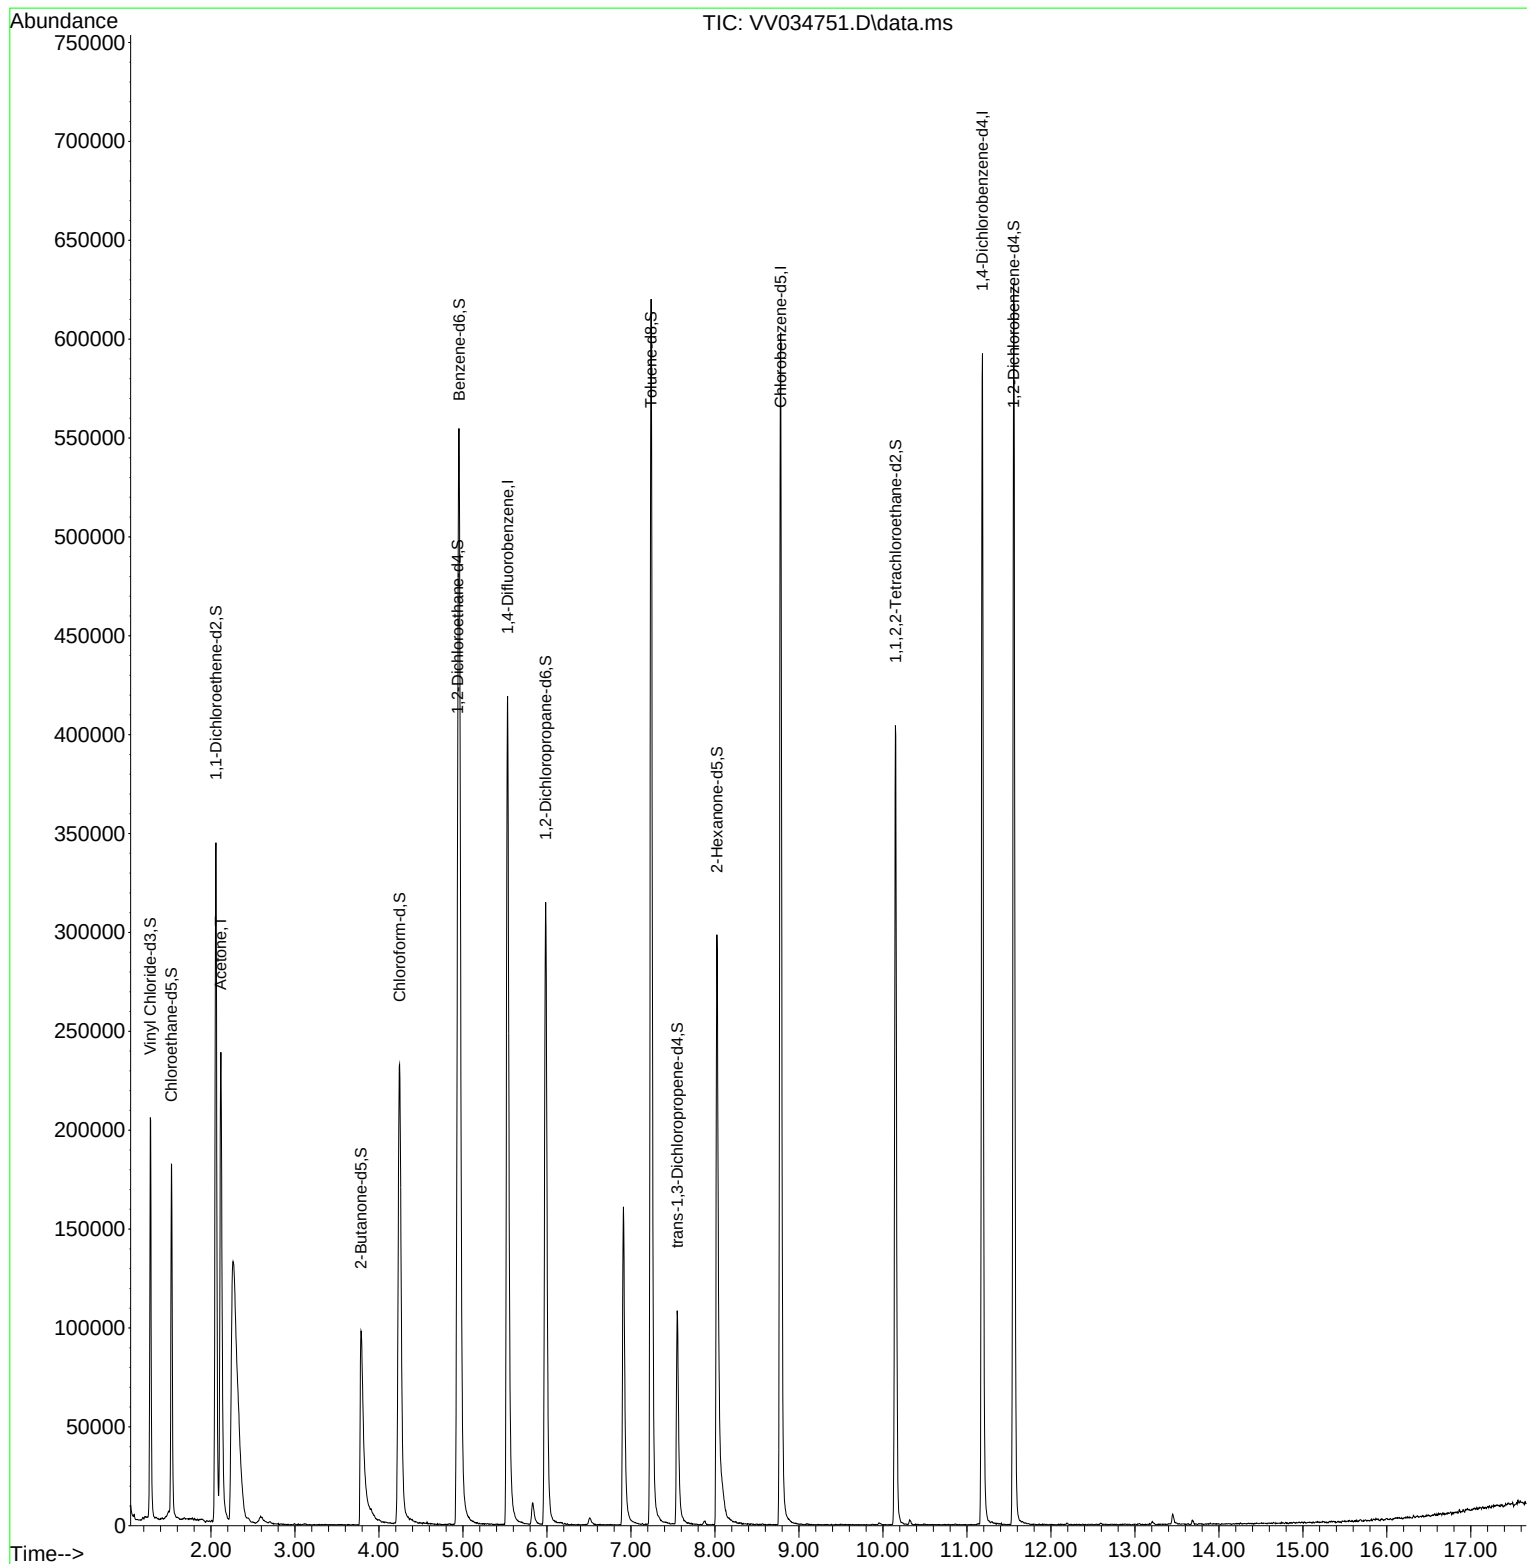

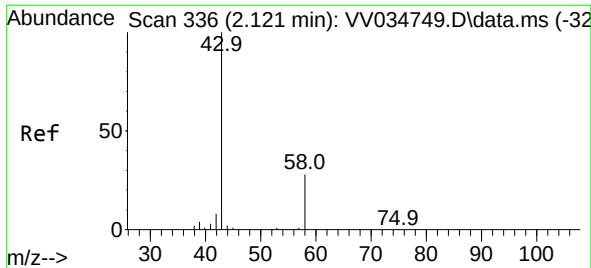

#13
 Acetone
 Concen: 110.250 ug/L
 RT: 2.118 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VV034751.D
 Acq: 20 Mar 2024 10:11

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKW1

Tgt Ion: 43 Resp: 279285
 Ion Ratio Lower Upper
 43 100
 58 29.3 0.0 57.2

