

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034750.D
 Acq On : 20 Mar 2024 09:42
 Operator : SY/MD
 Sample : VV0320WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	92	rVB	246114	257197	15.34%	2.166%
2	1.536	147	154	173	rVB	207950	243655	14.53%	2.052%
3	2.060	307	317	334	rBV	409495	604711	36.07%	5.092%
4	2.394	417	421	423	rBV2	614	498	0.03%	0.004%
5	2.452	431	439	448	rBV5	3148	5284	0.32%	0.044%
6	2.519	457	460	463	rBV	287	219	0.01%	0.002%
7	2.545	466	468	470	rBV	377	219	0.01%	0.002%
8	2.706	511	518	527	rBV4	2339	3496	0.21%	0.029%
9	2.892	573	576	577	rBV2	229	133	0.01%	0.001%
10	3.008	609	612	613	rBV	143	85	0.01%	0.001%
11	3.015	613	614	618	rVB	287	130	0.01%	0.001%
12	3.040	618	622	623	rBV	265	116	0.01%	0.001%
13	3.069	628	631	632	rBV	345	139	0.01%	0.001%
14	3.121	639	647	653	rVB3	878	1201	0.07%	0.010%
15	3.156	653	658	660	rBB2	232	155	0.01%	0.001%
16	3.214	673	676	677	rBV2	110	69	0.00%	0.001%
17	3.298	699	702	704	rBV2	150	101	0.01%	0.001%
18	3.368	718	724	726	rBV2	228	259	0.02%	0.002%
19	3.429	740	743	746	rBV2	135	114	0.01%	0.001%
20	3.494	760	763	766	rVB2	206	117	0.01%	0.001%
21	3.526	766	773	775	rBV2	193	231	0.01%	0.002%
22	3.664	813	816	818	rBV	146	113	0.01%	0.001%
23	3.754	837	844	848	rBV2	353	407	0.02%	0.003%
24	3.793	848	856	901	rBV	114352	347510	20.73%	2.926%
25	4.249	981	998	1030	rBV	261425	673554	40.18%	5.671%
26	4.561	1092	1095	1097	rBV3	599	424	0.03%	0.004%
27	4.706	1138	1140	1142	rBV	186	98	0.01%	0.001%
28	4.889	1195	1197	1198	rBV	321	124	0.01%	0.001%
29	4.957	1201	1218	1254	rBV2	625411	1676462	100.00%	14.116%
30	5.394	1350	1354	1355	rBV2	279	205	0.01%	0.002%
31	5.439	1365	1368	1369	rBV2	367	223	0.01%	0.002%
32	5.471	1376	1378	1381	rVB2	410	185	0.01%	0.002%
33	5.532	1383	1397	1439	rBV	413382	867631	51.75%	7.305%
34	5.834	1480	1491	1507	rBV4	13678	30350	1.81%	0.256%
35	5.986	1525	1538	1572	rBV	344550	722440	43.09%	6.083%
36	6.275	1626	1628	1636	rVB5	566	580	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034750.D
 Acq On : 20 Mar 2024 09:42
 Operator : SY/MD
 Sample : VV0320WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.304	1636	1637	1639	rBV2	240	107	0.01%	0.001%
38	6.323	1640	1643	1646	rVB2	349	194	0.01%	0.002%
39	6.368	1654	1657	1661	rBV2	125	96	0.01%	0.001%
40	6.400	1665	1667	1670	rBV	256	142	0.01%	0.001%
41	6.416	1670	1672	1674	rBV	166	98	0.01%	0.001%
42	6.442	1676	1680	1681	rBV2	442	302	0.02%	0.003%
43	6.506	1698	1700	1702	rVB	170	72	0.00%	0.001%
44	6.523	1702	1705	1707	rBV2	134	79	0.00%	0.001%
45	6.609	1729	1732	1734	rBV	117	71	0.00%	0.001%
46	6.658	1744	1747	1750	rBV	234	200	0.01%	0.002%
47	6.725	1764	1768	1770	rBV	116	89	0.01%	0.001%
48	6.912	1815	1826	1856	rBV	179762	347749	20.74%	2.928%
49	7.243	1918	1929	1962	rBV	709635	1269781	75.74%	10.691%
50	7.551	2016	2025	2049	rBV	124725	229731	13.70%	1.934%
51	7.780	2093	2096	2097	rBV2	592	360	0.02%	0.003%
52	7.899	2130	2133	2134	rBV3	390	236	0.01%	0.002%
53	7.937	2143	2145	2146	rBV	152	65	0.00%	0.001%
54	7.976	2155	2157	2160	rVB2	234	111	0.01%	0.001%
55	7.992	2160	2162	2163	rBV	210	79	0.00%	0.001%
56	8.024	2163	2172	2217	rBV	354261	724956	43.24%	6.104%
57	8.452	2302	2305	2308	rBV2	560	339	0.02%	0.003%
58	8.674	2371	2374	2377	rBV2	151	100	0.01%	0.001%
59	8.690	2377	2379	2380	rBV	249	110	0.01%	0.001%
60	8.783	2397	2408	2431	rBV	624993	1027489	61.29%	8.651%
61	9.053	2490	2492	2496	rBV2	250	152	0.01%	0.001%
62	9.172	2528	2529	2533	rVB	375	129	0.01%	0.001%
63	9.307	2568	2571	2573	rBV	132	76	0.00%	0.001%
64	9.320	2573	2575	2583	rVB2	189	166	0.01%	0.001%
65	9.362	2583	2588	2591	rBV2	160	157	0.01%	0.001%
66	9.493	2621	2629	2633	rBV3	1726	2481	0.15%	0.021%
67	9.670	2680	2684	2691	rVV4	529	491	0.03%	0.004%
68	9.773	2714	2716	2719	rBV2	136	68	0.00%	0.001%
69	9.821	2728	2731	2733	rBV	143	103	0.01%	0.001%
70	9.876	2741	2748	2758	rVB4	2013	3063	0.18%	0.026%
71	9.947	2767	2770	2775	rBV2	278	247	0.01%	0.002%
72	10.149	2821	2833	2858	rBV	444497	715286	42.67%	6.023%
73	10.339	2888	2892	2893	rBV	511	261	0.02%	0.002%
74	10.452	2925	2927	2929	rVV	236	116	0.01%	0.001%
75	10.484	2929	2937	2945	rVV4	2341	3687	0.22%	0.031%
76	10.529	2948	2951	2953	rBV	169	97	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034750.D
 Acq On : 20 Mar 2024 09:42
 Operator : SY/MD
 Sample : VV0320WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.548	2954	2957	2960	rVB	316	208	0.01%	0.002%
78	10.641	2983	2986	2989	rBV	160	107	0.01%	0.001%
79	10.661	2990	2992	2995	rVB	222	87	0.01%	0.001%
80	10.738	3013	3016	3019	rVB2	194	108	0.01%	0.001%
81	10.860	3047	3054	3063	rBV3	1822	2908	0.17%	0.024%
82	11.133	3131	3139	3144	rBV4	2280	3315	0.20%	0.028%
83	11.182	3144	3154	3180	rVV	603826	957759	57.13%	8.064%
84	11.558	3259	3271	3300	rBV	702204	1102960	65.79%	9.287%
85	11.792	3341	3344	3346	rBV2	309	169	0.01%	0.001%
86	11.886	3367	3373	3375	rBV3	277	254	0.02%	0.002%
87	12.066	3426	3429	3432	rBV2	275	179	0.01%	0.002%
88	12.159	3455	3458	3463	rVB	376	289	0.02%	0.002%
89	12.365	3520	3522	3523	rBV	457	156	0.01%	0.001%
90	12.503	3561	3565	3568	rBV	311	236	0.01%	0.002%
91	12.535	3573	3575	3577	rBV	297	83	0.00%	0.001%
92	12.590	3582	3592	3596	rBV6	2370	3090	0.18%	0.026%
93	13.175	3771	3774	3777	rBV	474	290	0.02%	0.002%
94	13.207	3777	3784	3795	rBV6	4185	6647	0.40%	0.056%
95	13.448	3850	3859	3874	rBV2	12987	22301	1.33%	0.188%
96	13.587	3900	3902	3903	rBV2	266	97	0.01%	0.001%
97	13.686	3925	3933	3944	rVB5	4689	7067	0.42%	0.060%
98	13.850	3982	3984	3985	rBV	267	90	0.01%	0.001%
99	14.169	4080	4083	4085	rBV2	415	245	0.01%	0.002%
100	14.397	4151	4154	4157	rBV2	688	457	0.03%	0.004%




Sum of corrected areas: 11876673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034750.D
Acq On : 20 Mar 2024 09:42
Operator : SY/MD
Sample : VV0320WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

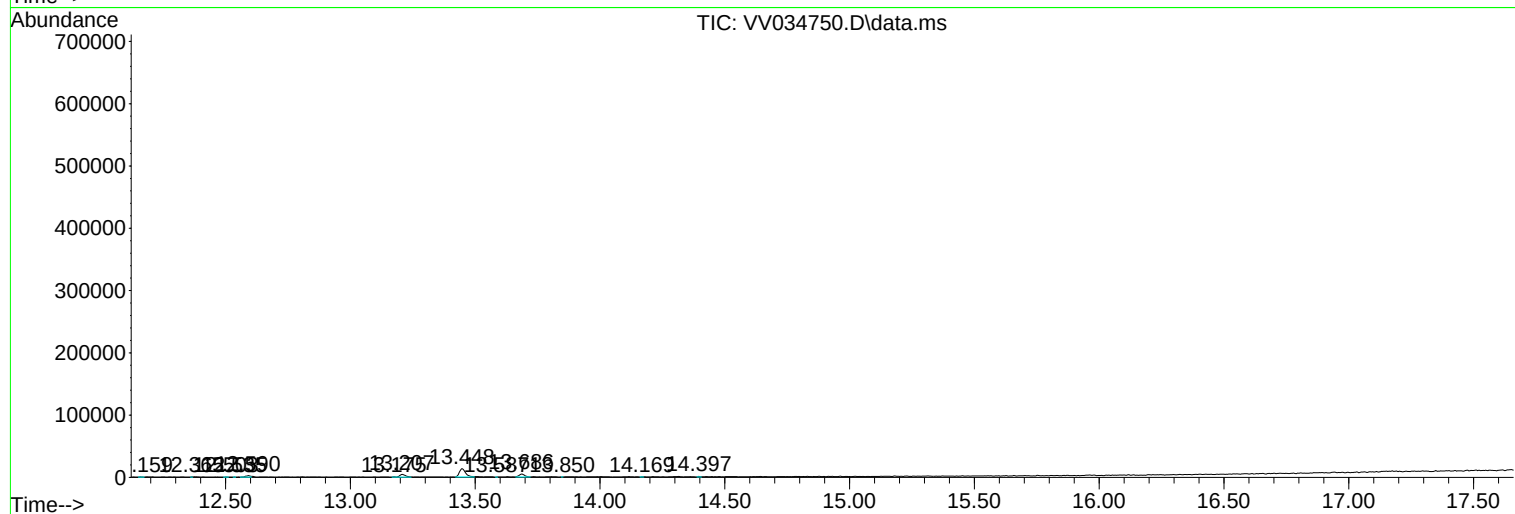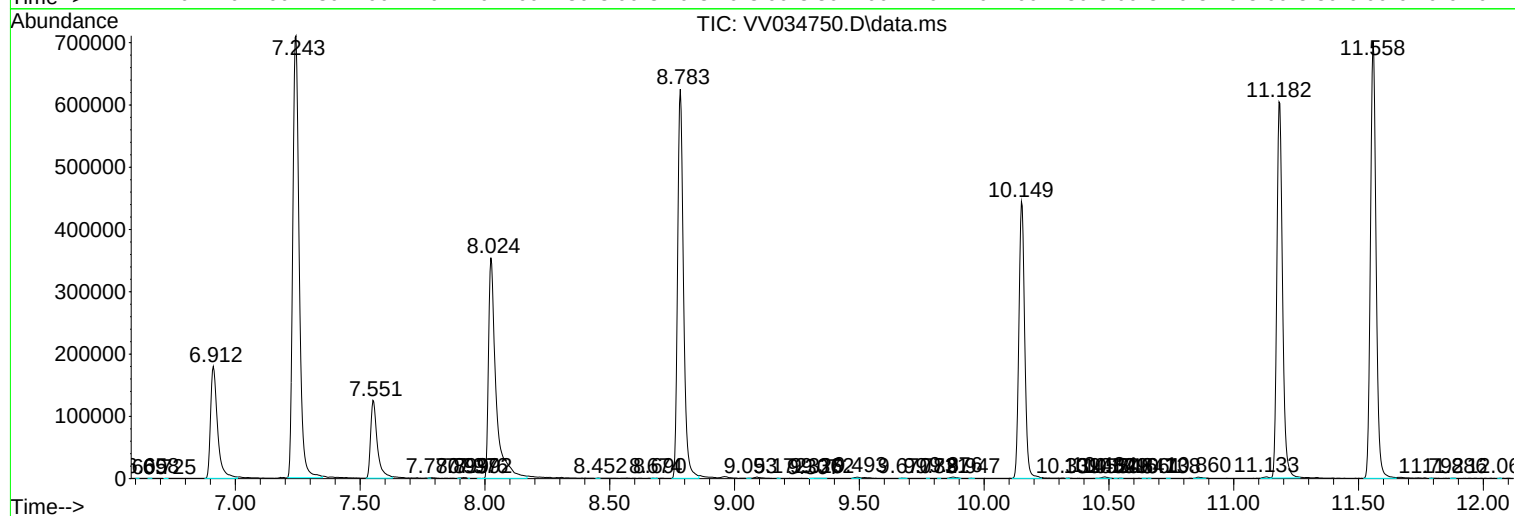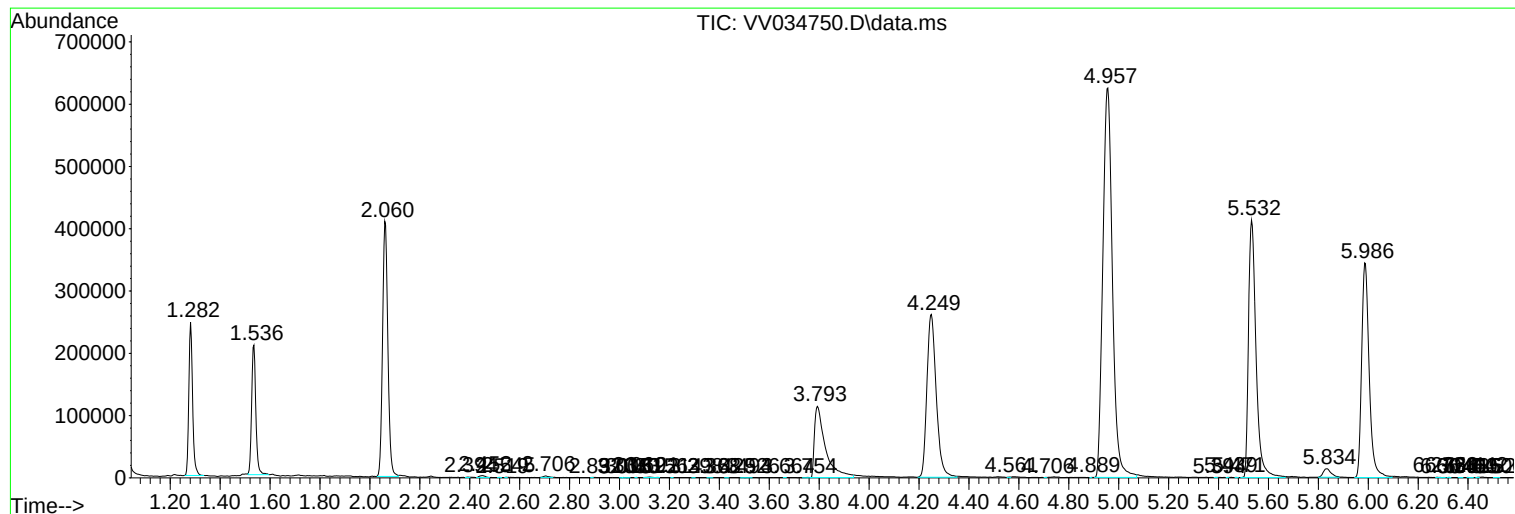

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034750.D
Acq On : 20 Mar 2024 09:42
Operator : SY/MD
Sample : VV0320WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034750.D
Acq On : 20 Mar 2024 09:42
Operator : SY/MD
Sample : VV0320WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc