

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034763.D
 Acq On : 20 Mar 2024 14:57
 Operator : SY/MD
 Sample : P1778-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	184546	196025	13.32%	1.848%
2	1.532	146	153	165	rVB	172527	195659	13.30%	1.844%
3	2.060	307	317	330	rBV	331506	479120	32.56%	4.516%
4	2.272	369	383	385	rBV6	3559	6647	0.45%	0.063%
5	2.642	496	498	500	rVB	379	146	0.01%	0.001%
6	2.667	503	506	507	rBV3	256	142	0.01%	0.001%
7	2.854	562	564	567	rBV	233	120	0.01%	0.001%
8	3.031	617	619	620	rBV	275	121	0.01%	0.001%
9	3.249	683	687	690	rBV2	192	142	0.01%	0.001%
10	3.458	749	752	754	rBV2	206	139	0.01%	0.001%
11	3.484	758	760	764	rVV	226	171	0.01%	0.002%
12	3.503	764	766	770	rVV2	219	159	0.01%	0.001%
13	3.542	774	778	780	rBV	237	124	0.01%	0.001%
14	3.670	815	818	822	rVB2	324	212	0.01%	0.002%
15	3.696	822	826	829	rVB2	193	164	0.01%	0.002%
16	3.715	829	832	838	rBV2	144	178	0.01%	0.002%
17	3.793	847	856	890	rBV	110382	325887	22.15%	3.072%
18	4.246	982	997	1025	rBV	228426	591425	40.19%	5.575%
19	4.616	1109	1112	1113	rBV3	260	179	0.01%	0.002%
20	4.635	1116	1118	1121	rVB2	437	218	0.01%	0.002%
21	4.693	1130	1136	1140	rBV2	425	378	0.03%	0.004%
22	4.850	1181	1185	1187	rBV	225	213	0.01%	0.002%
23	4.953	1201	1217	1256	rBV2	552098	1471549	100.00%	13.871%
24	5.474	1378	1379	1383	rBV3	402	204	0.01%	0.002%
25	5.532	1386	1397	1428	rBV	388047	803868	54.63%	7.577%
26	5.831	1481	1490	1509	rBV2	10259	23168	1.57%	0.218%
27	5.924	1517	1519	1521	rVB3	335	130	0.01%	0.001%
28	5.989	1526	1539	1570	rVV	316817	653906	44.44%	6.164%
29	6.211	1605	1608	1610	rBV3	506	286	0.02%	0.003%
30	6.259	1621	1623	1626	rBV	361	239	0.02%	0.002%
31	6.297	1633	1635	1640	rVB	204	112	0.01%	0.001%
32	6.320	1640	1642	1648	rVB2	304	217	0.01%	0.002%
33	6.349	1648	1651	1654	rBV	201	145	0.01%	0.001%
34	6.387	1660	1663	1664	rBV	241	121	0.01%	0.001%
35	6.448	1677	1682	1685	rBV2	202	166	0.01%	0.002%
36	6.731	1767	1770	1774	rVB2	300	202	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034763.D
 Acq On : 20 Mar 2024 14:57
 Operator : SY/MD
 Sample : P1778-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.754	1774	1777	1780	rBV2	246	162	0.01%	0.002%
38	6.911	1815	1826	1859	rBV	170890	332597	22.60%	3.135%
39	7.243	1918	1929	1955	rBV	619565	1102246	74.90%	10.390%
40	7.497	2005	2008	2013	rVB3	368	294	0.02%	0.003%
41	7.551	2016	2025	2050	rBV	114371	213309	14.50%	2.011%
42	7.937	2142	2145	2149	rBV	163	123	0.01%	0.001%
43	8.024	2163	2172	2220	rBV	336093	695443	47.26%	6.555%
44	8.500	2317	2320	2323	rVB2	416	249	0.02%	0.002%
45	8.516	2323	2325	2326	rBV	267	108	0.01%	0.001%
46	8.554	2333	2337	2341	rVB3	491	422	0.03%	0.004%
47	8.673	2372	2374	2375	rBV	351	130	0.01%	0.001%
48	8.728	2389	2391	2395	rVB2	421	223	0.02%	0.002%
49	8.783	2395	2408	2438	rBV	564063	942914	64.08%	8.888%
50	9.014	2478	2480	2488	rVB3	658	556	0.04%	0.005%
51	9.056	2488	2493	2496	rBV	527	421	0.03%	0.004%
52	9.104	2502	2508	2512	rBV2	394	373	0.03%	0.004%
53	9.127	2513	2515	2526	rVB2	373	371	0.03%	0.003%
54	9.239	2546	2550	2556	rBV2	442	411	0.03%	0.004%
55	9.268	2556	2559	2561	rVV	188	113	0.01%	0.001%
56	9.288	2563	2565	2567	rVV	266	163	0.01%	0.002%
57	9.352	2580	2585	2589	rBV	351	369	0.03%	0.003%
58	9.429	2603	2609	2612	rBV2	184	168	0.01%	0.002%
59	9.452	2612	2616	2620	rVB	149	130	0.01%	0.001%
60	9.474	2620	2623	2628	rBV2	335	308	0.02%	0.003%
61	9.532	2638	2641	2646	rVB2	178	114	0.01%	0.001%
62	9.673	2681	2685	2687	rBV	268	140	0.01%	0.001%
63	9.686	2687	2689	2694	rVB2	220	127	0.01%	0.001%
64	9.744	2703	2707	2709	rVB2	189	121	0.01%	0.001%
65	9.767	2709	2714	2718	rBV2	282	322	0.02%	0.003%
66	9.828	2731	2733	2737	rBV2	275	136	0.01%	0.001%
67	9.863	2742	2744	2748	rVB2	264	154	0.01%	0.001%
68	9.889	2748	2752	2754	rBV	196	126	0.01%	0.001%
69	9.918	2758	2761	2767	rVB2	191	209	0.01%	0.002%
70	9.947	2767	2770	2773	rBV2	272	143	0.01%	0.001%
71	10.017	2789	2792	2796	rBV	227	207	0.01%	0.002%
72	10.149	2822	2833	2855	rBV	416008	670965	45.60%	6.325%
73	10.275	2867	2872	2874	rBV2	327	334	0.02%	0.003%
74	10.323	2883	2887	2894	rVB2	685	942	0.06%	0.009%
75	10.355	2894	2897	2903	rBV2	218	229	0.02%	0.002%
76	10.452	2924	2927	2934	rVB2	250	257	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034763.D
 Acq On : 20 Mar 2024 14:57
 Operator : SY/MD
 Sample : P1778-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.487	2934	2938	2939	rBV	354	233	0.02%	0.002%
78	10.532	2949	2952	2954	rBV2	256	116	0.01%	0.001%
79	10.548	2954	2957	2959	rBV2	269	138	0.01%	0.001%
80	10.667	2992	2994	2997	rBV	191	121	0.01%	0.001%
81	10.760	3020	3023	3028	rBV	185	158	0.01%	0.001%
82	10.869	3054	3057	3062	rVB2	256	258	0.02%	0.002%
83	10.979	3088	3091	3095	rBV2	188	165	0.01%	0.002%
84	11.030	3102	3107	3110	rBV2	315	361	0.02%	0.003%
85	11.069	3117	3119	3124	rBV2	170	145	0.01%	0.001%
86	11.185	3143	3155	3178	rBV	558101	882173	59.95%	8.315%
87	11.490	3247	3250	3256	rBV2	277	208	0.01%	0.002%
88	11.561	3259	3272	3298	rBV	634193	1004479	68.26%	9.468%
89	11.773	3336	3338	3341	rBV	419	313	0.02%	0.003%
90	11.812	3349	3350	3355	rBV3	231	149	0.01%	0.001%
91	11.943	3389	3391	3393	rBV	245	105	0.01%	0.001%
92	12.120	3443	3446	3447	rBV	191	120	0.01%	0.001%
93	12.287	3495	3498	3501	rBV2	361	221	0.02%	0.002%
94	12.554	3577	3581	3583	rBV	187	152	0.01%	0.001%
95	12.853	3670	3674	3677	rBV2	266	200	0.01%	0.002%
96	13.262	3798	3801	3802	rBV	326	200	0.01%	0.002%
97	13.332	3821	3823	3825	rBV2	321	158	0.01%	0.001%
98	13.345	3825	3827	3832	rVB	258	184	0.01%	0.002%
99	13.458	3860	3862	3864	rVV	473	227	0.02%	0.002%
100	13.834	3977	3979	3981	rBV	747	256	0.02%	0.002%




Sum of corrected areas: 10608851

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034763.D
Acq On : 20 Mar 2024 14:57
Operator : SY/MD
Sample : P1778-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

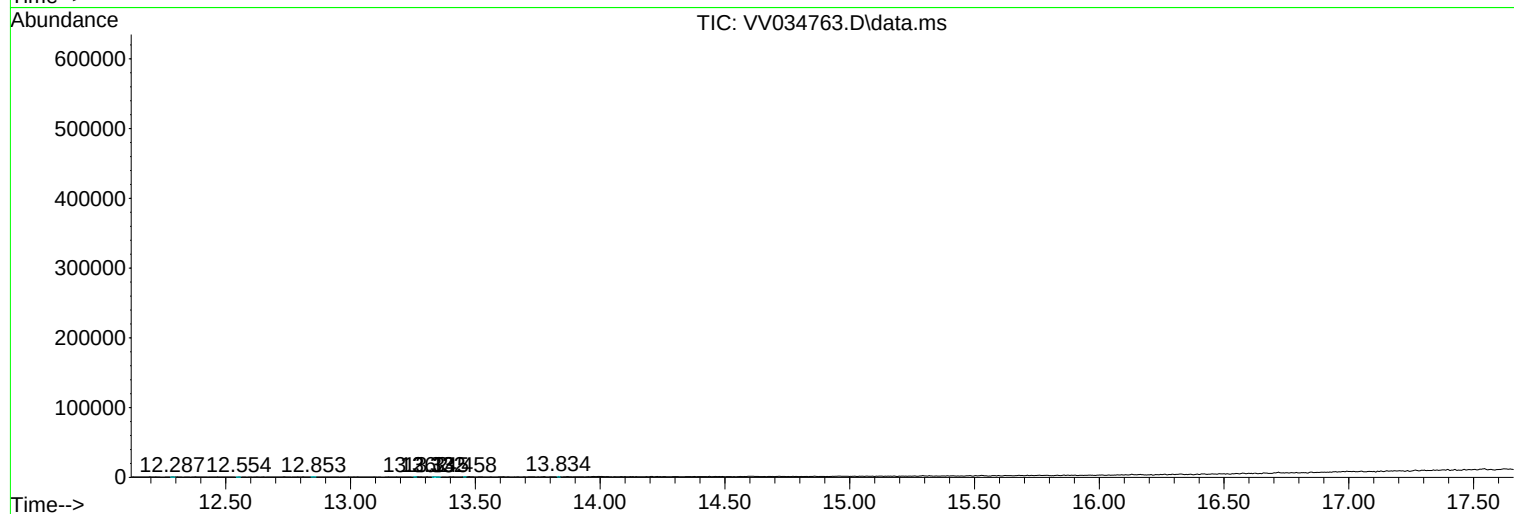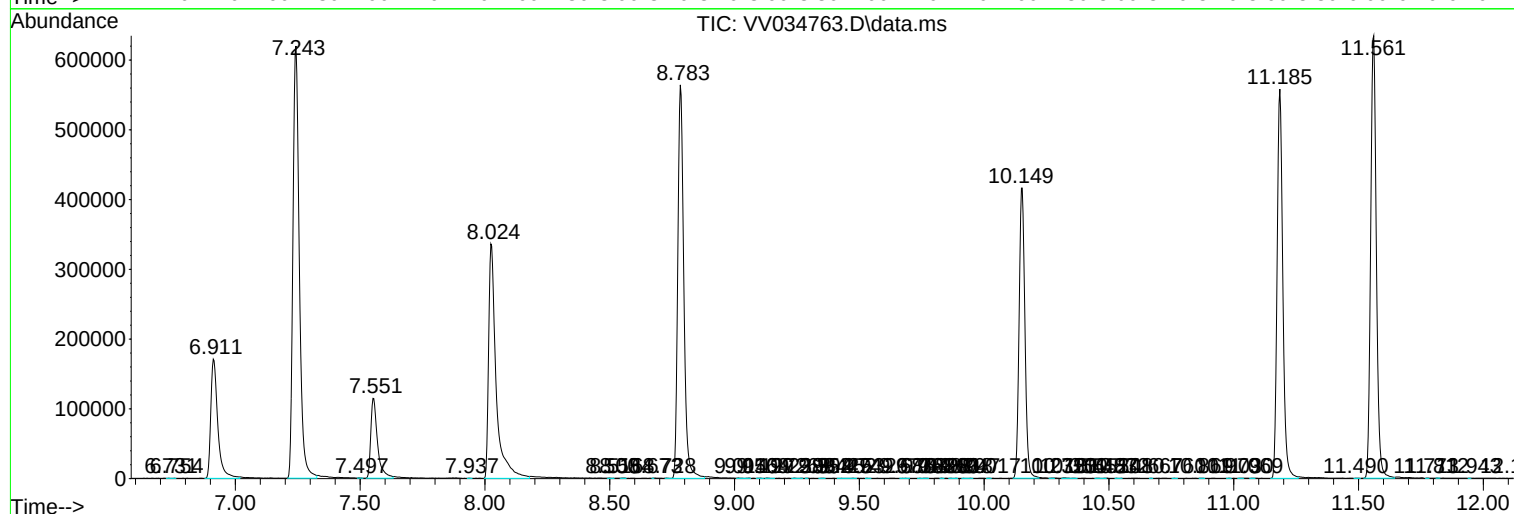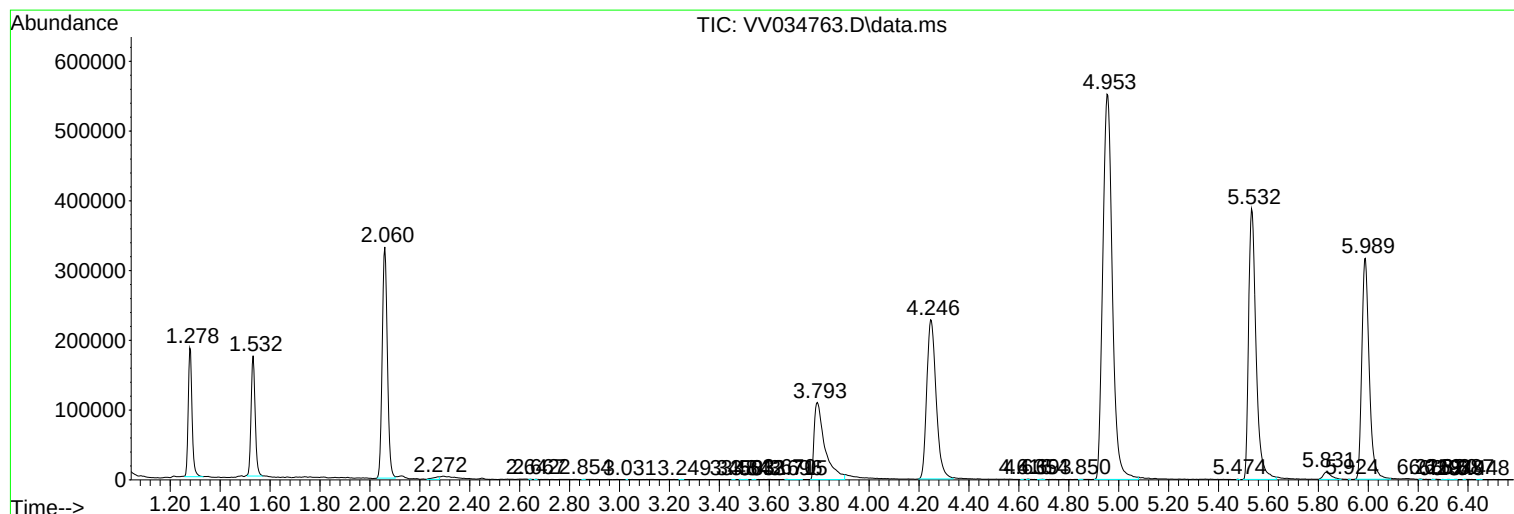

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034763.D
Acq On : 20 Mar 2024 14:57
Operator : SY/MD
Sample : P1778-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034763.D
Acq On : 20 Mar 2024 14:57
Operator : SY/MD
Sample : P1778-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------