

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034766.D
 Acq On : 20 Mar 2024 16:08
 Operator : SY/MD
 Sample : P1757-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	177089	184946	0.11%	0.041%
2	1.529	145	152	167	rVB	161474	190123	0.11%	0.042%
3	2.060	306	317	330	rBV	284569	413870	0.24%	0.092%
4	2.240	368	373	375	rBV3	1273	1151	0.00%	0.000%
5	2.387	415	419	421	rBV2	334	262	0.00%	0.000%
6	2.452	431	439	447	rVV5	2332	3272	0.00%	0.001%
7	2.516	450	459	469	rVB4	3202	5661	0.00%	0.001%
8	2.584	477	480	483	rVB3	429	295	0.00%	0.000%
9	2.690	506	513	515	rBV2	864	785	0.00%	0.000%
10	2.767	536	537	543	rVV2	273	215	0.00%	0.000%
11	2.815	548	552	554	rVV3	520	373	0.00%	0.000%
12	2.896	574	577	583	rVB3	424	332	0.00%	0.000%
13	2.950	592	594	598	rBV2	253	210	0.00%	0.000%
14	3.243	682	685	690	rBV2	375	257	0.00%	0.000%
15	3.490	757	762	765	rBB3	265	228	0.00%	0.000%
16	3.670	806	818	834	rVB5	6983	16721	0.01%	0.004%
17	3.786	845	854	895	rBV	105073	300339	0.17%	0.066%
18	4.111	951	955	956	rBV2	286	221	0.00%	0.000%
19	4.249	980	998	1031	rBV2	236911	695330	0.40%	0.154%
20	4.529	1083	1085	1089	rBV	247	214	0.00%	0.000%
21	4.587	1089	1103	1119	rVB8	5093	13384	0.01%	0.003%
22	4.648	1119	1122	1124	rBV3	613	399	0.00%	0.000%
23	4.738	1134	1150	1169	rBV2	16301	41727	0.02%	0.009%
24	4.844	1178	1183	1185	rBV2	616	480	0.00%	0.000%
25	4.886	1193	1196	1201	rVB2	600	340	0.00%	0.000%
26	4.957	1201	1218	1221	rBV2	572911	1133360	0.66%	0.251%
27	5.008	1223	1234	1280	rVB	5849975	12959015	7.49%	2.868%
28	5.474	1376	1379	1383	rBV3	687	598	0.00%	0.000%
29	5.532	1386	1397	1440	rVB	391795	815340	0.47%	0.180%
30	5.838	1482	1492	1506	rBV6	4561	9918	0.01%	0.002%
31	5.944	1519	1525	1526	rBV3	488	413	0.00%	0.000%
32	5.985	1526	1538	1571	rVV	304493	646305	0.37%	0.143%
33	6.281	1627	1630	1634	rBV4	967	808	0.00%	0.000%
34	6.442	1677	1680	1686	rBV2	469	522	0.00%	0.000%
35	6.503	1693	1699	1701	rBV3	391	406	0.00%	0.000%
36	6.513	1701	1702	1711	rVB3	275	216	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034766.D
 Acq On : 20 Mar 2024 16:08
 Operator : SY/MD
 Sample : P1757-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.567	1715	1719	1723	rVB3	251	245	0.00%	0.000%
38	6.690	1753	1757	1759	rBV2	319	228	0.00%	0.000%
39	6.767	1777	1781	1784	rBV	354	213	0.00%	0.000%
40	6.911	1815	1826	1859	rBV	174036	330970	0.19%	0.073%
41	7.088	1878	1881	1888	rVB5	772	961	0.00%	0.000%
42	7.243	1915	1929	1953	rBV	639449	1123978	0.65%	0.249%
43	7.551	2016	2025	2047	rBV	121668	221109	0.13%	0.049%
44	7.664	2058	2060	2065	rBV2	507	398	0.00%	0.000%
45	7.706	2070	2073	2077	rBV4	431	260	0.00%	0.000%
46	7.747	2083	2086	2088	rBV2	490	262	0.00%	0.000%
47	7.844	2111	2116	2117	rBV2	412	292	0.00%	0.000%
48	7.879	2117	2127	2132	rBV4	2651	4667	0.00%	0.001%
49	7.911	2133	2137	2151	rVB5	3708	5528	0.00%	0.001%
50	8.024	2163	2172	2213	rBV	360429	674420	0.39%	0.149%
51	8.262	2243	2246	2249	rBV4	425	321	0.00%	0.000%
52	8.329	2265	2267	2270	rVB3	640	322	0.00%	0.000%
53	8.390	2283	2286	2291	rBV3	542	551	0.00%	0.000%
54	8.519	2322	2326	2330	rBV3	331	278	0.00%	0.000%
55	8.538	2330	2332	2336	rVB2	398	224	0.00%	0.000%
56	8.815	2398	2418	2473	rBV	22289482	36836755	21.30%	8.153%
57	9.181	2530	2532	2536	rBV4	645	374	0.00%	0.000%
58	9.442	2610	2613	2616	rBV2	445	292	0.00%	0.000%
59	9.487	2621	2627	2629	rBV4	1045	1196	0.00%	0.000%
60	9.561	2644	2650	2654	rBV3	403	464	0.00%	0.000%
61	9.603	2660	2663	2665	rBV2	352	221	0.00%	0.000%
62	9.709	2693	2696	2700	rBV3	415	455	0.00%	0.000%
63	9.728	2700	2702	2704	rVV3	379	237	0.00%	0.000%
64	9.879	2745	2749	2753	rVB2	384	333	0.00%	0.000%
65	9.902	2753	2756	2761	rBV2	314	296	0.00%	0.000%
66	9.969	2774	2777	2783	rVB3	415	414	0.00%	0.000%
67	10.152	2822	2834	2863	rBV	466902	749332	0.43%	0.166%
68	10.271	2869	2871	2877	rVB3	476	290	0.00%	0.000%
69	10.326	2879	2888	2892	rBV3	3862	5088	0.00%	0.001%
70	10.365	2892	2900	2915	rVB	24503	39703	0.02%	0.009%
71	10.435	2919	2922	2924	rBV3	649	416	0.00%	0.000%
72	10.487	2930	2938	2951	rBV3	8596	14389	0.01%	0.003%
73	10.796	3029	3034	3036	rBV2	565	365	0.00%	0.000%
74	10.866	3050	3056	3062	rVB5	636	785	0.00%	0.000%
75	10.976	3082	3090	3092	rBV3	445	590	0.00%	0.000%
76	11.033	3106	3108	3111	rBV2	466	343	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034766.D
 Acq On : 20 Mar 2024 16:08
 Operator : SY/MD
 Sample : P1757-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	11.123	3120	3136	3149	rBV	27419745	44153239	25.53%	9.772%
78	11.230	3149	3169	3190	rVB3	71752145	144883174	83.77%	32.066%
79	11.609	3263	3287	3302	rBV3	78016513	172945834	100.00%	38.277%
80	12.278	3490	3495	3496	rBV3	3219	2543	0.00%	0.001%
81	12.332	3503	3512	3536	rVB	180976	284216	0.16%	0.063%
82	12.522	3560	3571	3582	rBV3	21659	50051	0.03%	0.011%
83	12.583	3582	3590	3609	rVV2	25866	46269	0.03%	0.010%
84	12.686	3611	3622	3638	rVV	133850	211158	0.12%	0.047%
85	12.937	3692	3700	3709	rBV6	4046	7366	0.00%	0.002%
86	13.011	3720	3723	3727	rBV5	758	616	0.00%	0.000%
87	13.069	3737	3741	3744	rBV3	741	705	0.00%	0.000%
88	13.201	3768	3782	3807	rBV	15247476	22705832	13.13%	5.025%
89	13.532	3882	3885	3889	rBV3	701	679	0.00%	0.000%
90	13.680	3915	3931	3965	rBV	5940110	8947560	5.17%	1.980%
91	14.094	4052	4060	4076	rBV4	11849	23439	0.01%	0.005%
92	14.278	4114	4117	4120	rBV4	740	482	0.00%	0.000%
93	14.368	4141	4145	4148	rBV3	818	609	0.00%	0.000%
94	14.516	4189	4191	4194	rVB2	818	412	0.00%	0.000%
95	14.599	4210	4217	4219	rBV6	740	835	0.00%	0.000%
96	14.638	4227	4229	4234	rVB3	507	338	0.00%	0.000%
97	14.660	4234	4236	4239	rBV2	556	388	0.00%	0.000%
98	14.760	4254	4267	4279	rBV3	19608	34325	0.02%	0.008%
99	15.336	4437	4446	4462	rBV4	41927	66788	0.04%	0.015%
100	15.474	4486	4489	4493	rBV3	983	698	0.00%	0.000%




Sum of corrected areas: 451823157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034766.D
Acq On : 20 Mar 2024 16:08
Operator : SY/MD
Sample : P1757-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

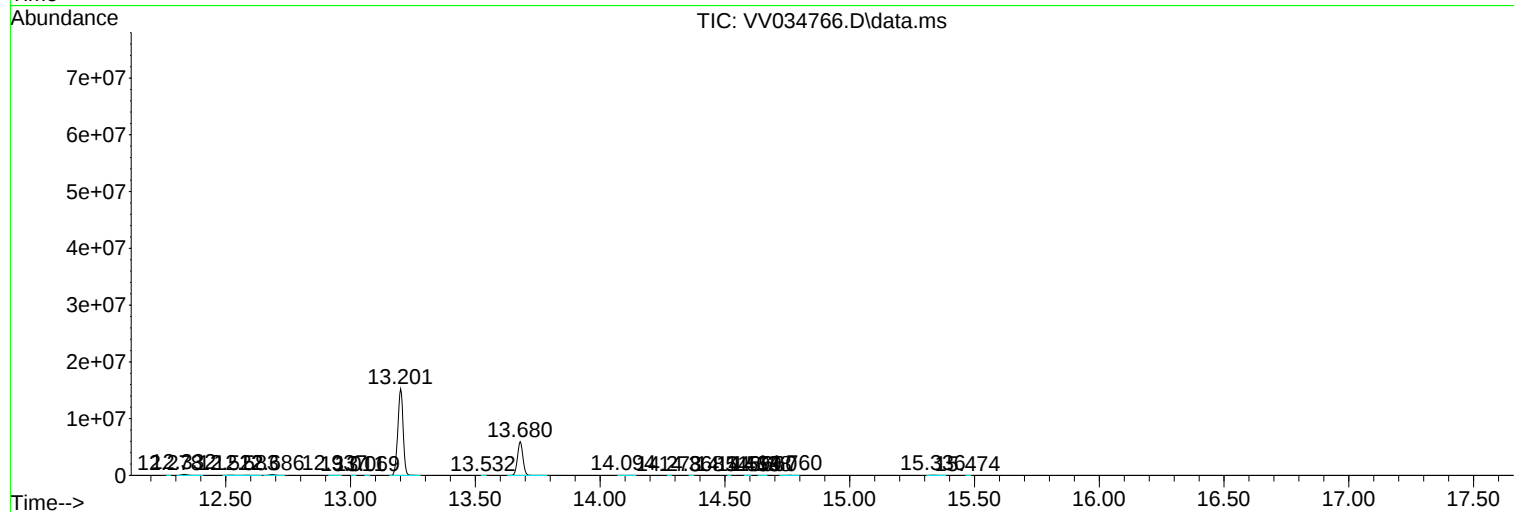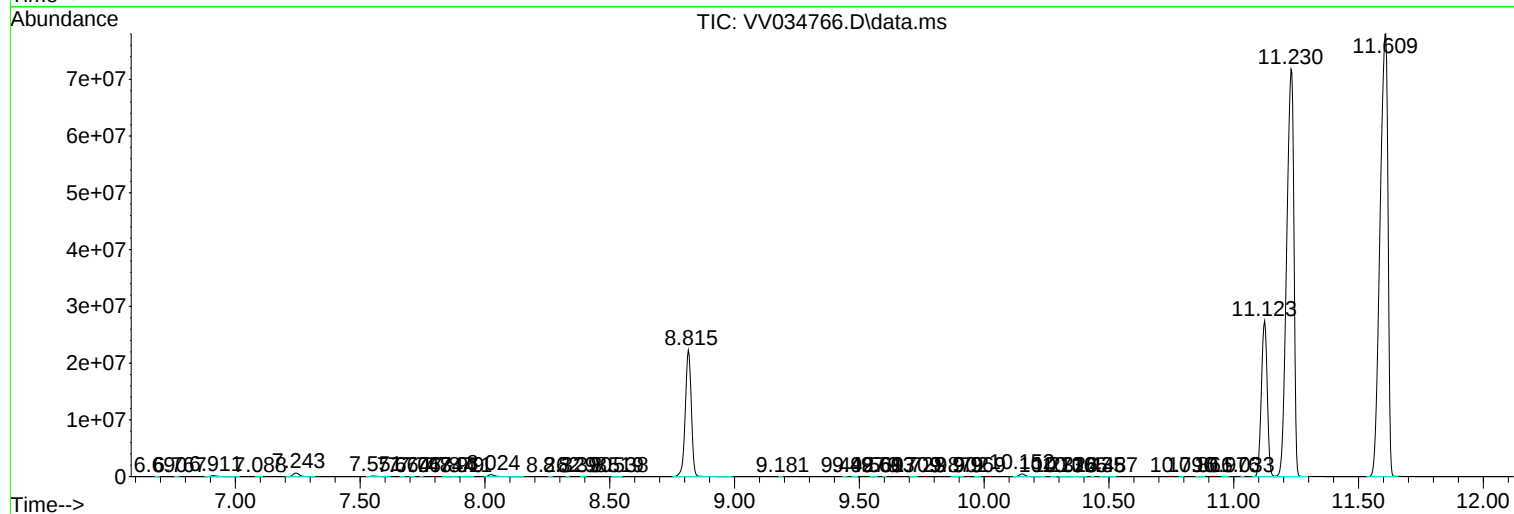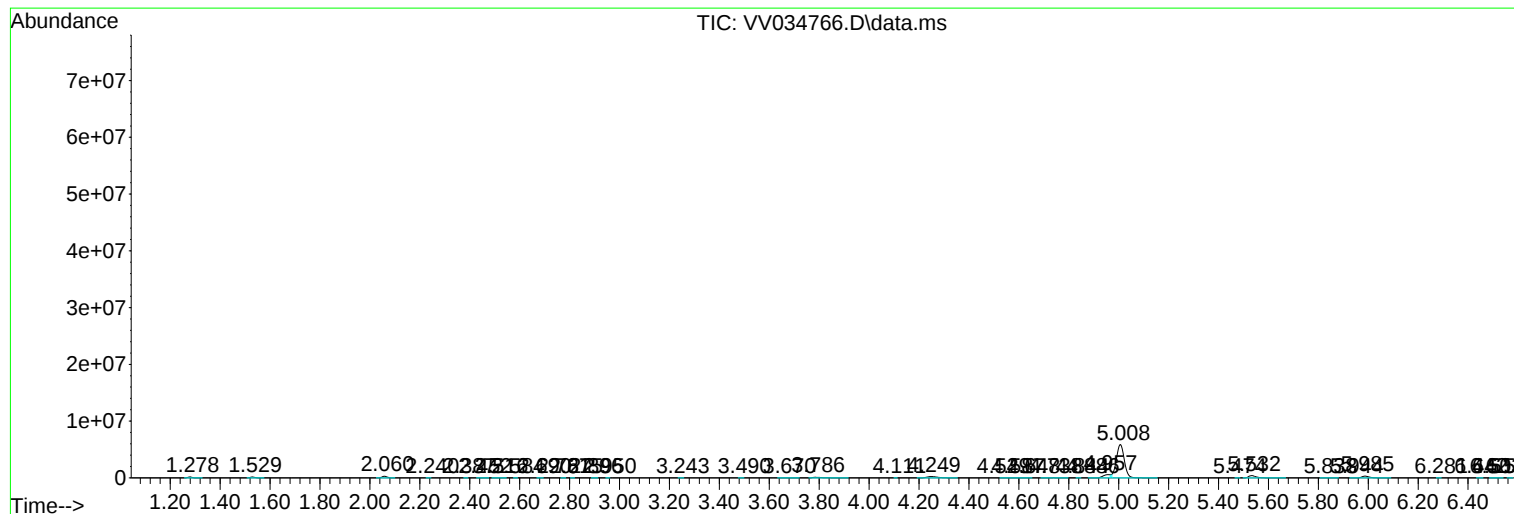

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034766.D
Acq On : 20 Mar 2024 16:08
Operator : SY/MD
Sample : P1757-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034766.D
Acq On : 20 Mar 2024 16:08
Operator : SY/MD
Sample : P1757-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc