

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034767.D
 Acq On : 20 Mar 2024 16:56
 Operator : SY/MD
 Sample : VIBLK273
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK273

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	176728	187498	13.20%	1.759%
2	1.529	146	152	175	rVB	173405	204740	14.41%	1.921%
3	2.059	307	317	333	rBV	247618	363522	25.59%	3.411%
4	2.449	431	438	450	rVB4	3892	6440	0.45%	0.060%
5	2.506	452	456	457	rBV	247	184	0.01%	0.002%
6	2.561	463	473	476	rBV2	917	1358	0.10%	0.013%
7	2.645	497	499	506	rVB2	325	222	0.02%	0.002%
8	2.703	511	517	523	rVV6	1535	2329	0.16%	0.022%
9	2.767	533	537	540	rBV2	399	263	0.02%	0.002%
10	2.850	559	563	565	rBV	218	148	0.01%	0.001%
11	2.953	593	595	600	rBV2	292	222	0.02%	0.002%
12	3.088	634	637	639	rVV2	317	212	0.01%	0.002%
13	3.121	643	647	654	rVB4	470	563	0.04%	0.005%
14	3.153	654	657	659	rBV2	190	136	0.01%	0.001%
15	3.185	664	667	671	rVB2	329	244	0.02%	0.002%
16	3.214	671	676	680	rBV2	178	206	0.01%	0.002%
17	3.285	695	698	701	rBV	127	93	0.01%	0.001%
18	3.323	707	710	714	rVB	226	202	0.01%	0.002%
19	3.375	718	726	730	rBV2	262	305	0.02%	0.003%
20	3.545	775	779	780	rBV	135	94	0.01%	0.001%
21	3.667	813	817	820	rBV2	151	126	0.01%	0.001%
22	3.728	833	836	838	rBV2	290	185	0.01%	0.002%
23	3.751	841	843	847	rVB2	214	99	0.01%	0.001%
24	3.789	847	855	895	rBV	113461	332704	23.42%	3.122%
25	4.162	967	971	973	rBV3	379	309	0.02%	0.003%
26	4.246	982	997	1029	rBV	219707	569255	40.07%	5.342%
27	4.699	1135	1138	1144	rVB3	276	305	0.02%	0.003%
28	4.725	1144	1146	1150	rBV3	574	543	0.04%	0.005%
29	4.876	1190	1193	1200	rVB2	347	303	0.02%	0.003%
30	4.953	1200	1217	1258	rBV2	529003	1420529	100.00%	13.329%
31	5.429	1362	1365	1367	rBV3	328	212	0.01%	0.002%
32	5.487	1380	1383	1384	rBV2	261	147	0.01%	0.001%
33	5.532	1387	1397	1429	rBV	336432	705805	49.69%	6.623%
34	5.834	1480	1491	1509	rBV3	12358	27087	1.91%	0.254%
35	5.985	1526	1538	1572	rBV2	308682	644290	45.36%	6.046%
36	6.210	1605	1608	1611	rBV3	487	258	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034767.D
 Acq On : 20 Mar 2024 16:56
 Operator : SY/MD
 Sample : VIBLK273
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK273

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.255	1619	1622	1623	rBV	201	120	0.01%	0.001%
38	6.374	1655	1659	1664	rVV2	250	246	0.02%	0.002%
39	6.410	1668	1670	1673	rVB	253	122	0.01%	0.001%
40	6.436	1676	1678	1680	rBV2	209	92	0.01%	0.001%
41	6.455	1680	1684	1688	rBV3	324	326	0.02%	0.003%
42	6.513	1695	1702	1704	rBV	252	301	0.02%	0.003%
43	6.545	1707	1712	1715	rBV3	235	248	0.02%	0.002%
44	6.661	1745	1748	1750	rBV	183	106	0.01%	0.001%
45	6.741	1768	1773	1774	rBV	144	128	0.01%	0.001%
46	6.776	1777	1784	1786	rVB3	311	289	0.02%	0.003%
47	6.821	1795	1798	1801	rVB2	289	161	0.01%	0.002%
48	6.847	1801	1806	1809	rBV3	269	208	0.01%	0.002%
49	6.911	1816	1826	1857	rBV	158190	304964	21.47%	2.862%
50	7.243	1918	1929	1958	rBV	577091	1026455	72.26%	9.632%
51	7.554	2016	2026	2055	rBV	110047	207022	14.57%	1.943%
52	7.844	2114	2116	2119	rBV2	330	231	0.02%	0.002%
53	7.857	2119	2120	2125	rVB2	390	230	0.02%	0.002%
54	7.882	2125	2128	2129	rBV	339	215	0.02%	0.002%
55	7.969	2148	2155	2159	rBV2	298	309	0.02%	0.003%
56	7.992	2159	2162	2163	rBV	140	91	0.01%	0.001%
57	8.024	2163	2172	2218	rBV	352545	706677	49.75%	6.631%
58	8.426	2295	2297	2303	rVB2	335	141	0.01%	0.001%
59	8.554	2334	2337	2338	rBV	347	177	0.01%	0.002%
60	8.583	2343	2346	2349	rBV2	343	241	0.02%	0.002%
61	8.741	2393	2395	2397	rBV2	242	125	0.01%	0.001%
62	8.783	2397	2408	2435	rBV	516904	891276	62.74%	8.363%
63	9.056	2491	2493	2497	rVB3	419	192	0.01%	0.002%
64	9.146	2519	2521	2524	rVB	271	100	0.01%	0.001%
65	9.271	2558	2560	2564	rVB	257	133	0.01%	0.001%
66	9.287	2564	2565	2568	rVB2	227	93	0.01%	0.001%
67	9.316	2568	2574	2577	rBV2	261	308	0.02%	0.003%
68	9.445	2610	2614	2615	rBV	176	100	0.01%	0.001%
69	9.487	2623	2627	2628	rBV	1113	761	0.05%	0.007%
70	9.590	2654	2659	2663	rBV4	511	547	0.04%	0.005%
71	9.628	2669	2671	2676	rVB2	405	288	0.02%	0.003%
72	9.657	2676	2680	2682	rBV	237	174	0.01%	0.002%
73	9.680	2684	2687	2689	rVB	229	143	0.01%	0.001%
74	9.770	2713	2715	2718	rVB2	225	95	0.01%	0.001%
75	9.876	2739	2748	2758	rBV3	1082	1972	0.14%	0.019%
76	9.976	2777	2779	2781	rVB	354	97	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034767.D
Acq On : 20 Mar 2024 16:56
Operator : SY/MD
Sample : VIBLK273
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis

77	10.040	2793	2799	2810	rBV3	700	1130	0.08%	0.011%
78	10.152	2821	2834	2852	rBV	427634	677780	47.71%	6.360%
79	10.480	2929	2936	2938	rBV2	1042	1082	0.08%	0.010%
80	10.818	3038	3041	3043	rBV2	206	147	0.01%	0.001%
81	10.927	3072	3075	3078	rBV2	171	149	0.01%	0.001%
82	11.123	3126	3136	3145	rBV2	31929	50986	3.59%	0.478%
83	11.185	3145	3155	3189	rVB2	492780	988870	69.61%	9.279%
84	11.561	3260	3272	3297	rBV2	612486	1162924	81.87%	10.912%
85	11.857	3362	3364	3365	rBV	306	137	0.01%	0.001%
86	11.918	3380	3383	3386	rBV2	241	175	0.01%	0.002%
87	12.001	3406	3409	3415	rVB2	287	209	0.01%	0.002%
88	12.136	3449	3451	3452	rBV2	314	97	0.01%	0.001%
89	12.242	3482	3484	3487	rVB2	300	124	0.01%	0.001%
90	12.278	3493	3495	3498	rBV	240	121	0.01%	0.001%
91	12.303	3501	3503	3507	rVB	262	134	0.01%	0.001%
92	12.400	3529	3533	3535	rBV2	296	256	0.02%	0.002%
93	12.529	3567	3573	3576	rBV3	315	368	0.03%	0.003%
94	12.577	3586	3588	3589	rBV3	369	139	0.01%	0.001%
95	12.647	3607	3610	3613	rBV2	337	229	0.02%	0.002%
96	13.017	3723	3725	3728	rVB	339	156	0.01%	0.001%
97	13.059	3737	3738	3742	rVB2	206	94	0.01%	0.001%
98	13.201	3772	3782	3805	rBV2	60665	98687	6.95%	0.926%
99	13.564	3893	3895	3897	rBV	229	104	0.01%	0.001%
100	13.683	3922	3932	3947	rBV	35296	56407	3.97%	0.529%




Sum of corrected areas: 10657147

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034767.D
Acq On : 20 Mar 2024 16:56
Operator : SY/MD
Sample : VIBLK273
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

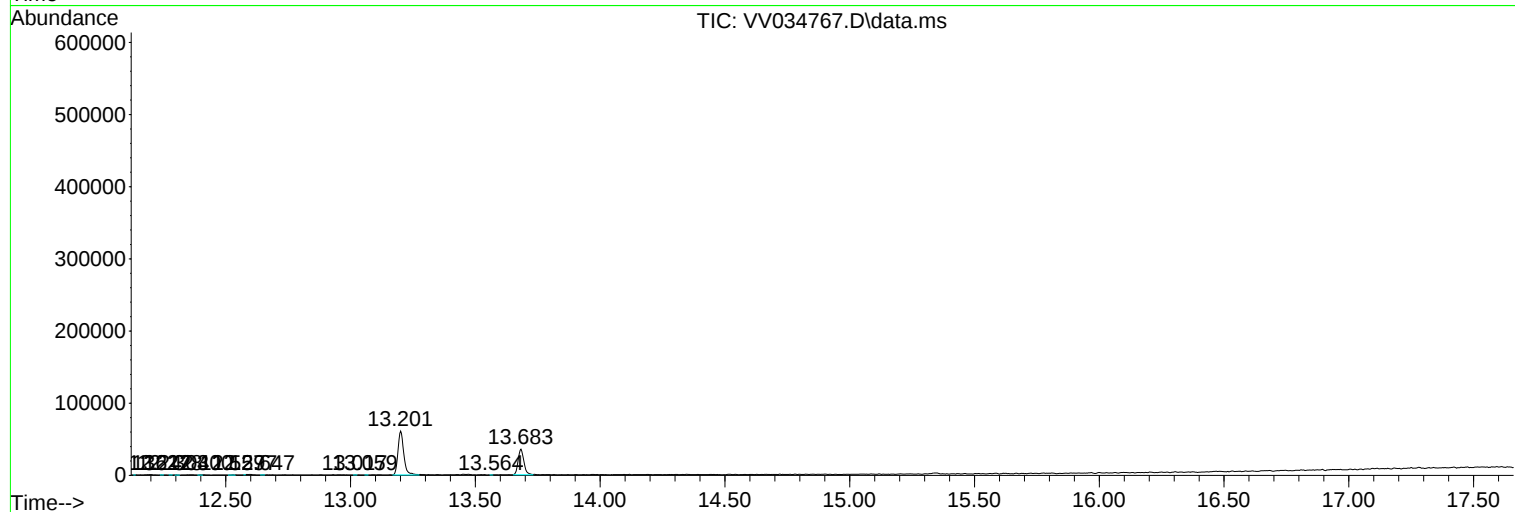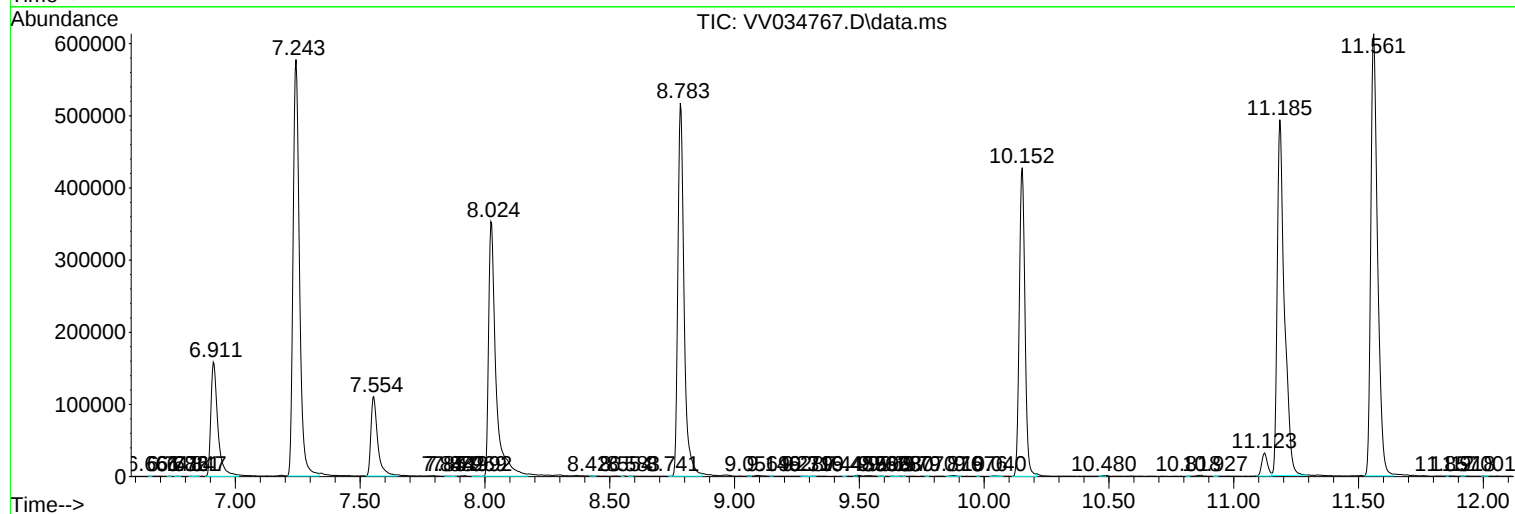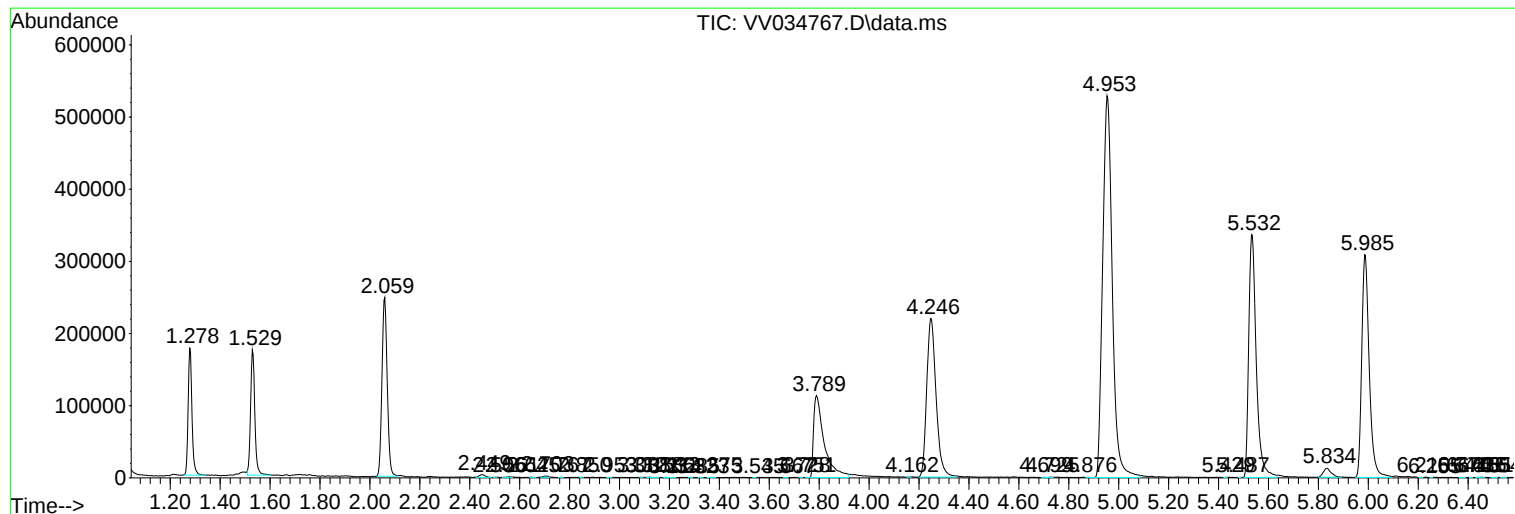

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034767.D
Acq On : 20 Mar 2024 16:56
Operator : SY/MD
Sample : VIBLK273
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034767.D
Acq On : 20 Mar 2024 16:56
Operator : SY/MD
Sample : VIBLK273
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------