

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034770.D
 Acq On : 20 Mar 2024 18:07
 Operator : SY/MD
 Sample : P1778-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	179867	191775	13.56%	1.814%
2	1.529	145	152	168	rVB	165292	198276	14.02%	1.876%
3	2.060	305	317	330	rBV	272345	401298	28.37%	3.797%
4	2.481	446	448	452	rBV2	470	279	0.02%	0.003%
5	2.558	461	472	481	rBV2	4694	9376	0.66%	0.089%
6	2.703	516	517	521	rVV2	345	159	0.01%	0.002%
7	2.773	537	539	543	rVB2	521	217	0.02%	0.002%
8	2.815	550	552	555	rBV	237	143	0.01%	0.001%
9	2.889	568	575	580	rBV6	1467	2057	0.15%	0.019%
10	2.976	599	602	606	rBB3	216	170	0.01%	0.002%
11	3.175	661	664	666	rBV2	304	213	0.02%	0.002%
12	3.301	700	703	705	rBV2	294	195	0.01%	0.002%
13	3.317	705	708	712	rVV2	328	236	0.02%	0.002%
14	3.346	712	717	721	rVV2	292	316	0.02%	0.003%
15	3.407	733	736	738	rBV2	230	134	0.01%	0.001%
16	3.452	746	750	754	rBV2	291	264	0.02%	0.002%
17	3.616	796	801	806	rVB3	357	285	0.02%	0.003%
18	3.670	814	818	824	rBV2	205	162	0.01%	0.002%
19	3.789	844	855	904	rBV2	122756	386252	27.31%	3.654%
20	4.146	964	966	970	rBV3	409	260	0.02%	0.002%
21	4.249	982	998	1030	rBV	222624	572664	40.49%	5.418%
22	4.632	1112	1117	1122	rBV3	370	419	0.03%	0.004%
23	4.799	1168	1169	1172	rVB2	368	135	0.01%	0.001%
24	4.818	1172	1175	1180	rVB2	424	343	0.02%	0.003%
25	4.953	1201	1217	1253	rBV2	535365	1414471	100.00%	13.382%
26	5.223	1299	1301	1304	rBV3	513	409	0.03%	0.004%
27	5.436	1364	1367	1369	rBV2	453	346	0.02%	0.003%
28	5.468	1374	1377	1382	rBV4	429	282	0.02%	0.003%
29	5.532	1386	1397	1430	rBV	389429	807479	57.09%	7.639%
30	5.831	1480	1490	1511	rBV4	13549	31127	2.20%	0.294%
31	5.989	1523	1539	1574	rBV	304129	630978	44.61%	5.970%
32	6.220	1607	1611	1616	rVB2	725	605	0.04%	0.006%
33	6.252	1616	1621	1625	rBV4	419	507	0.04%	0.005%
34	6.284	1629	1631	1633	rBV	323	207	0.01%	0.002%
35	6.506	1697	1700	1703	rBV2	239	182	0.01%	0.002%
36	6.587	1721	1725	1730	rVB2	195	188	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034770.D
 Acq On : 20 Mar 2024 18:07
 Operator : SY/MD
 Sample : P1778-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.722	1763	1767	1769	rBV2	181	125	0.01%	0.001%
38	6.792	1786	1789	1791	rBV	307	133	0.01%	0.001%
39	6.911	1816	1826	1853	rBV	164388	311141	22.00%	2.944%
40	7.169	1903	1906	1910	rVB2	366	232	0.02%	0.002%
41	7.243	1917	1929	1964	rBV	609015	1089104	77.00%	10.304%
42	7.551	2016	2025	2053	rBV	110419	208207	14.72%	1.970%
43	7.873	2120	2125	2131	rVB3	587	642	0.05%	0.006%
44	7.924	2138	2141	2143	rVB	300	143	0.01%	0.001%
45	7.992	2158	2162	2163	rBV	164	134	0.01%	0.001%
46	8.024	2163	2172	2223	rBV	340293	690818	48.84%	6.536%
47	8.519	2324	2326	2330	rVB2	391	197	0.01%	0.002%
48	8.673	2372	2374	2378	rVB	215	119	0.01%	0.001%
49	8.709	2383	2385	2387	rVB	327	160	0.01%	0.002%
50	8.725	2387	2390	2393	rBV2	278	162	0.01%	0.002%
51	8.783	2397	2408	2438	rBV	576822	970635	68.62%	9.183%
52	9.014	2477	2480	2483	rBV3	474	362	0.03%	0.003%
53	9.059	2492	2494	2495	rBV2	305	121	0.01%	0.001%
54	9.095	2502	2505	2506	rBV	400	185	0.01%	0.002%
55	9.214	2539	2542	2547	rVB3	493	326	0.02%	0.003%
56	9.268	2556	2559	2564	rVB2	259	201	0.01%	0.002%
57	9.297	2564	2568	2572	rBV2	255	278	0.02%	0.003%
58	9.368	2587	2590	2591	rBV	236	129	0.01%	0.001%
59	9.397	2597	2599	2604	rVB2	231	126	0.01%	0.001%
60	9.452	2613	2616	2619	rBV2	323	212	0.01%	0.002%
61	9.493	2626	2629	2634	rBV3	358	275	0.02%	0.003%
62	9.554	2644	2648	2652	rBV3	216	181	0.01%	0.002%
63	9.657	2677	2680	2684	rBV2	261	183	0.01%	0.002%
64	9.796	2720	2723	2726	rVV	218	165	0.01%	0.002%
65	9.841	2733	2737	2740	rBV2	207	199	0.01%	0.002%
66	10.072	2804	2809	2811	rBV	199	192	0.01%	0.002%
67	10.152	2822	2834	2864	rVV	405338	651448	46.06%	6.163%
68	10.368	2895	2901	2906	rBV3	310	367	0.03%	0.003%
69	10.548	2948	2957	2958	rBV	251	295	0.02%	0.003%
70	10.808	3035	3038	3042	rVB2	210	155	0.01%	0.001%
71	10.979	3086	3091	3093	rBV2	148	135	0.01%	0.001%
72	10.992	3093	3095	3098	rVB2	329	143	0.01%	0.001%
73	11.085	3120	3124	3128	rBV	338	310	0.02%	0.003%
74	11.130	3128	3138	3144	rVV4	8125	12189	0.86%	0.115%
75	11.185	3145	3155	3189	rVB	562430	932689	65.94%	8.824%
76	11.349	3203	3206	3207	rBV	437	235	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
 Data File : VV034770.D
 Acq On : 20 Mar 2024 18:07
 Operator : SY/MD
 Sample : P1778-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	11.484	3244	3248	3250	rBV2	324	168	0.01%	0.002%
78	11.561	3259	3272	3300	rBV	606459	1011826	71.53%	9.573%
79	11.805	3346	3348	3354	rBV3	323	189	0.01%	0.002%
80	11.834	3354	3357	3359	rBV2	281	137	0.01%	0.001%
81	11.918	3378	3383	3384	rBV2	360	229	0.02%	0.002%
82	12.059	3424	3427	3431	rVB2	328	203	0.01%	0.002%
83	12.162	3457	3459	3462	rVB	311	145	0.01%	0.001%
84	12.201	3466	3471	3474	rBV2	276	237	0.02%	0.002%
85	12.413	3534	3537	3540	rBV2	339	195	0.01%	0.002%
86	12.535	3571	3575	3580	rBV2	540	468	0.03%	0.004%
87	12.561	3580	3583	3585	rBV2	313	160	0.01%	0.002%
88	12.667	3613	3616	3621	rBV2	367	339	0.02%	0.003%
89	12.837	3667	3669	3673	rBV3	244	148	0.01%	0.001%
90	13.014	3722	3724	3730	rVB	290	207	0.01%	0.002%
91	13.040	3730	3732	3734	rBV	270	139	0.01%	0.001%
92	13.204	3775	3783	3794	rBV5	10613	18299	1.29%	0.173%
93	13.458	3856	3862	3864	rBV3	406	388	0.03%	0.004%
94	13.529	3881	3884	3886	rBV3	362	267	0.02%	0.003%
95	13.622	3910	3913	3917	rBV2	379	306	0.02%	0.003%
96	13.686	3927	3933	3946	rVB4	5873	9221	0.65%	0.087%
97	13.799	3966	3968	3970	rBV2	338	154	0.01%	0.001%
98	14.020	4035	4037	4040	rVB	565	284	0.02%	0.003%
99	14.046	4041	4045	4046	rBV	316	239	0.02%	0.002%
100	14.368	4143	4145	4152	rVB3	509	445	0.03%	0.004%




Sum of corrected areas: 10569855

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034770.D
Acq On : 20 Mar 2024 18:07
Operator : SY/MD
Sample : P1778-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

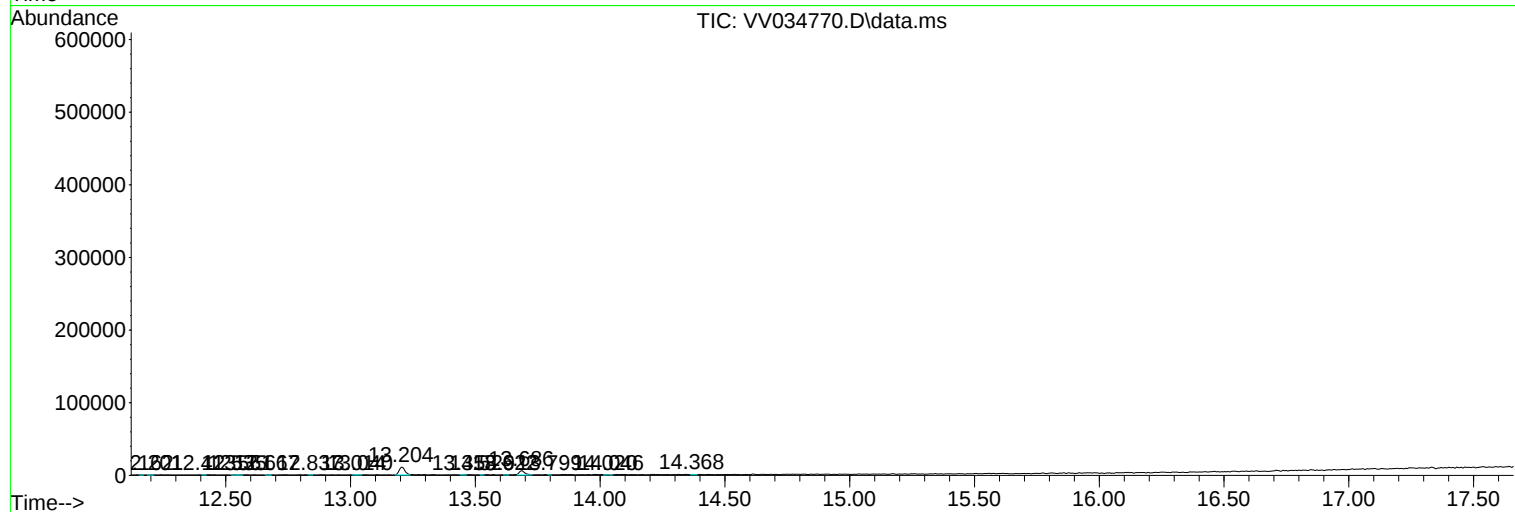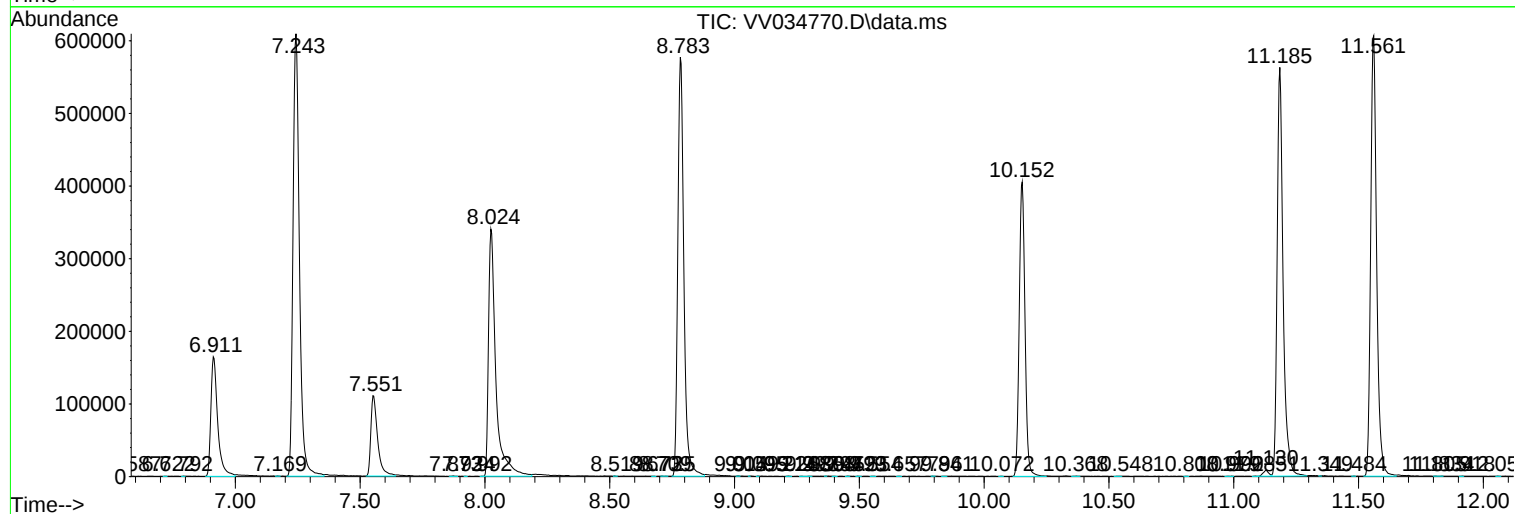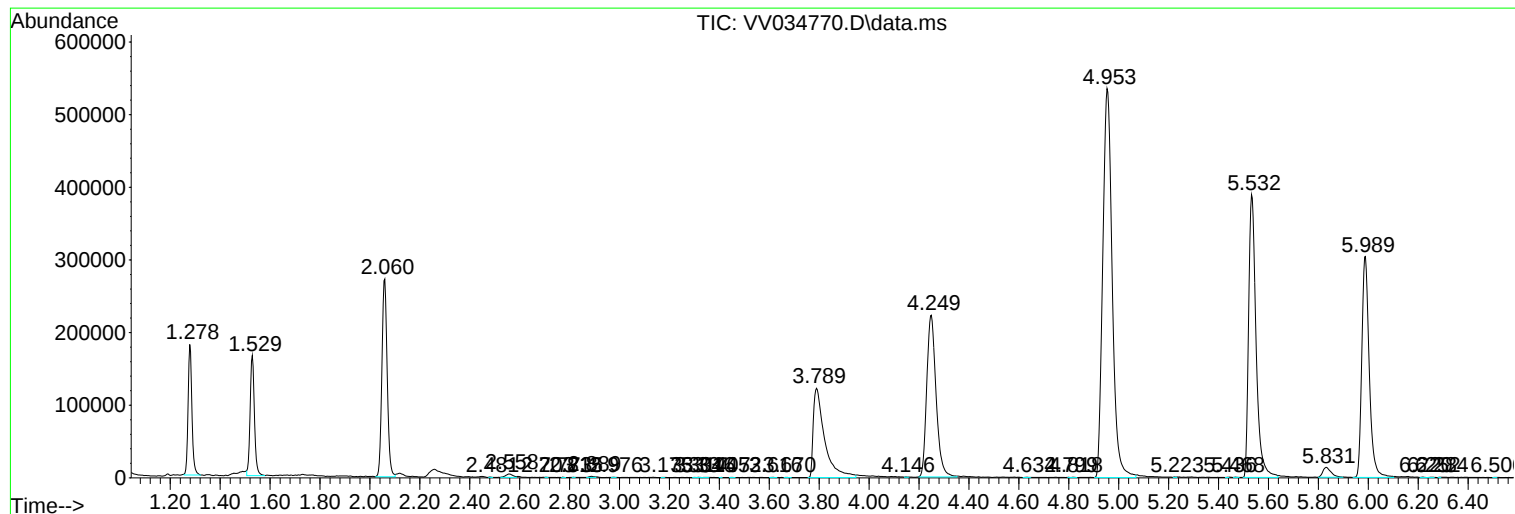

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034770.D
Acq On : 20 Mar 2024 18:07
Operator : SY/MD
Sample : P1778-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034770.D
Acq On : 20 Mar 2024 18:07
Operator : SY/MD
Sample : P1778-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
