


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032024\
Data File : VV034748.D
Acq On : 20 Mar 2024 08:25
Operator : SY/MD
Sample : BFB272
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB272

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis
Last Update : Fri Mar 22 01:59:49 2024

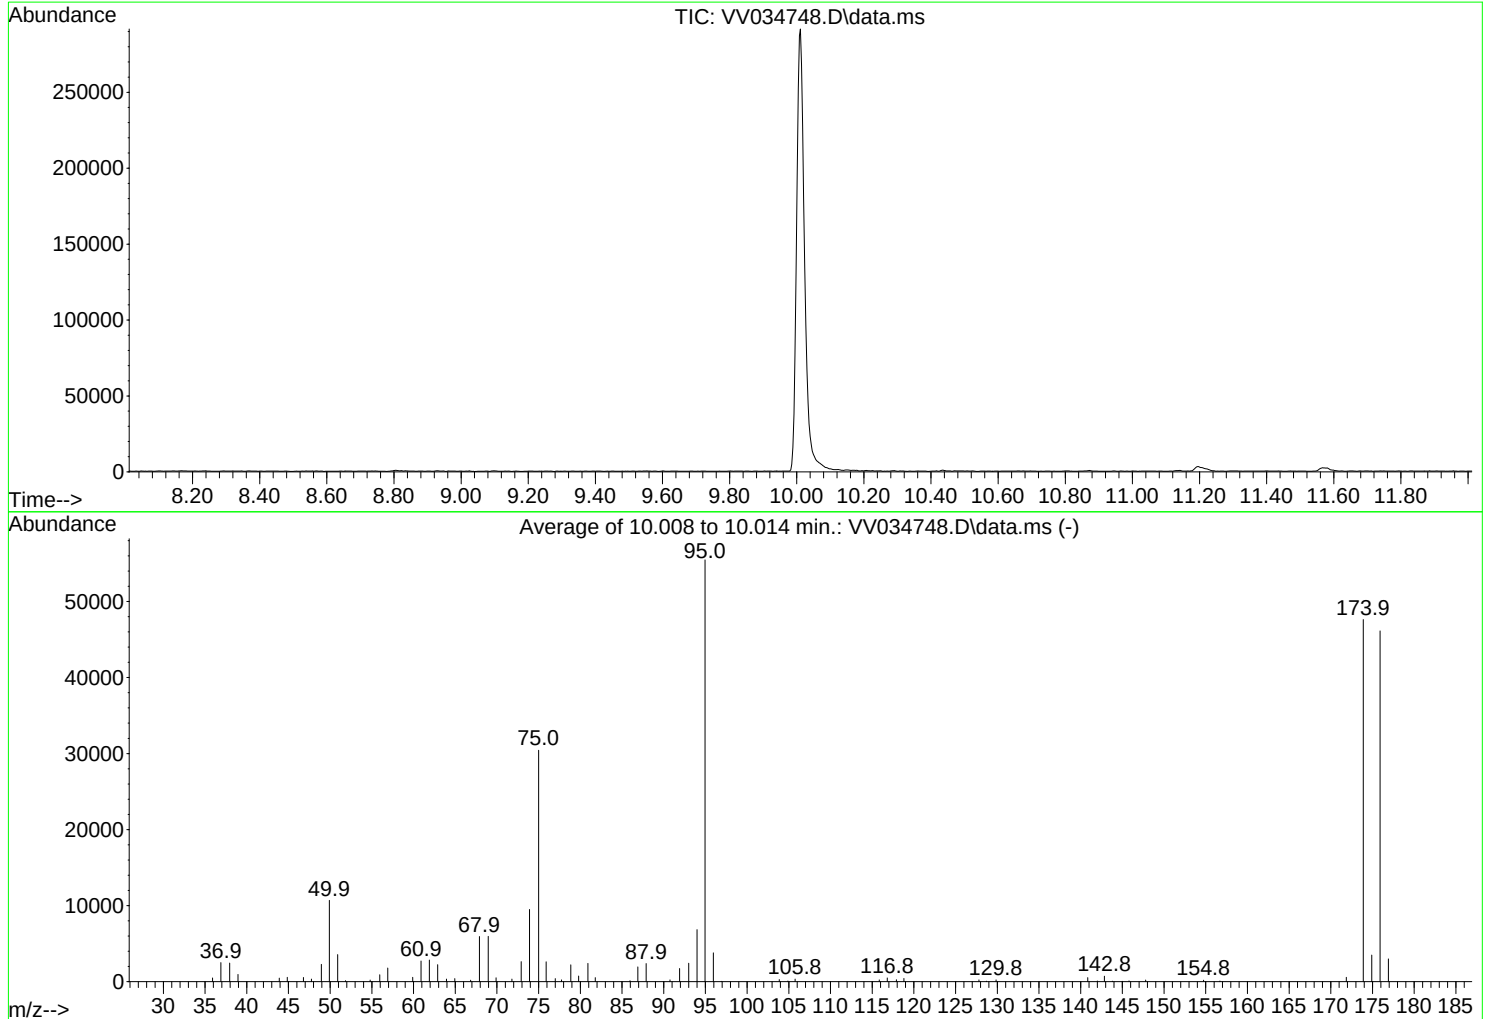

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	10683	PASS
75	95	30	80	54.8	30429	PASS
95	95	100	100	100.0	55480	PASS
96	95	5	9	6.8	3792	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.9	47637	PASS
175	174	5	9	7.3	3501	PASS
176	174	95	105	96.8	46133	PASS
177	176	5	10	6.5	2997	PASS

m/z	Abundance
39.80	328.0
43.90	208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

m/z	Abundance
35.90	519.0
36.90	2683.0
37.90	2623.0
39.00	1071.0
39.80	340.0
43.90	589.0
44.90	583.0
46.80	509.0
47.80	352.0
48.90	2335.0
49.90	11355.0
50.90	3551.0
51.90	121.0
54.80	252.0
56.00	964.0
56.90	1813.0
59.90	631.0
60.90	2856.0
61.90	2989.0
62.90	2389.0
63.90	368.0
64.90	415.0
66.90	194.0
67.90	6057.0
69.00	5979.0
69.90	547.0
71.80	355.0
72.90	2631.0
73.90	9886.0
75.00	31240.0
75.90	2849.0
77.00	324.0
77.70	245.0
78.80	2266.0
79.80	752.0
80.90	2448.0
81.80	491.0
85.90	116.0
86.90	1994.0
87.90	2396.0
90.80	219.0
91.90	1699.0
93.00	2555.0
94.00	7029.0
94.90	56360.0
95.90	3894.0
96.90	108.0
103.90	274.0
104.90	122.0
105.80	365.0
115.90	249.0
116.80	426.0
117.90	276.0
118.80	427.0
127.70	225.0
129.80	250.0
140.80	513.0
142.00	125.0
142.90	667.0
145.00	118.0
147.80	188.0
154.70	172.0
156.70	135.0
171.80	547.0
173.90	47584.0
174.90	3568.0
175.90	45792.0
176.90	3288.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

m/z	Abundance
35.90	492.0
36.90	2553.0
37.90	2473.0
39.00	981.0
39.80	312.0
43.90	696.0
44.90	584.0
46.80	569.0
47.70	358.0
49.00	2357.0
49.90	10958.0
50.90	3689.0
51.80	118.0
54.80	207.0
56.00	954.0
56.90	1855.0
59.90	584.0
60.90	2704.0
61.90	2904.0
62.90	2289.0
63.90	349.0
64.90	398.0
66.80	194.0
67.90	6130.0
68.90	6163.0
69.90	517.0
71.80	343.0
72.90	2734.0
73.90	9611.0
75.00	31544.0
75.90	2686.0
77.00	410.0
77.70	243.0
78.80	2281.0
79.80	757.0
80.90	2485.0
81.80	522.0
86.00	157.0
86.90	1945.0
87.90	2478.0
90.70	237.0
91.90	1791.0
93.00	2495.0
94.00	7013.0
94.90	57216.0
96.00	3925.0
103.80	270.0
104.90	109.0
105.70	332.0
115.90	225.0
116.80	490.0
117.90	252.0
118.80	426.0
127.80	244.0
128.70	107.0
129.90	244.0
140.90	522.0
142.00	103.0
142.90	740.0
143.80	107.0
145.80	154.0
147.80	207.0
154.70	218.0
156.70	118.0
171.80	597.0
173.90	49416.0
174.90	3636.0
175.90	47800.0
176.90	3093.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

m/z	Abundance
35.90	425.0
36.90	2292.0
38.00	2233.0
38.90	796.0
39.80	310.0
43.90	708.0
44.80	518.0
46.80	579.0
47.70	286.0
48.90	2116.0
49.90	9736.0
50.90	3441.0
51.80	139.0
54.80	168.0
55.90	806.0
56.90	1671.0
59.90	509.0
60.90	2581.0
61.90	2615.0
62.90	2025.0
64.00	303.0
65.00	366.0
66.80	202.0
67.90	5642.0
68.90	5711.0
69.90	445.0
71.80	331.0
72.90	2522.0
73.90	8967.0
75.00	28504.0
75.90	2301.0
77.00	464.0
77.80	234.0
78.90	2105.0
79.80	677.0
80.90	2256.0
81.80	540.0
86.00	126.0
86.90	1845.0
87.90	2245.0
90.70	220.0
91.90	1693.0
93.00	2243.0
94.00	6464.0
95.00	52864.0
96.00	3556.0
103.80	265.0
105.80	317.0
115.80	200.0
116.80	528.0
117.90	219.0
118.80	394.0
127.90	233.0
128.70	114.0
129.90	212.0
140.90	521.0
142.80	753.0
143.80	106.0
145.80	173.0
147.80	210.0
154.80	203.0
171.90	551.0
173.90	45912.0
174.90	3300.0
175.90	44808.0
176.90	2610.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272