

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032122\
 Data File : VV025107.D
 Acq On : 21 Mar 2022 10:15
 Operator : SY/MD
 Sample : VV0321WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK320

Quant Time: Mar 21 12:13:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 19 00:53:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	159337	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	145312	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	65304	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	52931	4.208	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.200%
7) Chloroethane-d5	1.564	69	44530	4.834	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.600%
11) 1,1-Dichloroethene-d2	2.105	63	68829	3.385	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.800%
20) 2-Butanone-d5	3.905	46	80532	52.972	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.940%
24) Chloroform-d	4.342	84	97152	4.657	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
26) 1,2-Dichloroethane-d4	5.030	65	42729	4.899	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.000%
32) Benzene-d6	5.043	84	207693	4.927	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.600%
36) 1,2-Dichloropropane-d6	6.066	67	60339	4.978	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.600%
41) Toluene-d8	7.313	98	180199	4.691	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%
43) trans-1,3-Dichloroprop...	7.622	79	19454	4.604	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.000%
46) 2-Hexanone-d5	8.088	63	72239	50.119	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.240%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	36198	5.076	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	56670	5.126	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.600%
Target Compounds						
16) Methylene chloride	2.506	84	2642	0.215	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV032122\
Data File : VV025107.D
Acq On : 21 Mar 2022 10:15
Operator : SY/MD
Sample : VV0321WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK320


Quant Time: Mar 21 12:13:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 19 00:53:30 2022
Response via : Initial Calibration

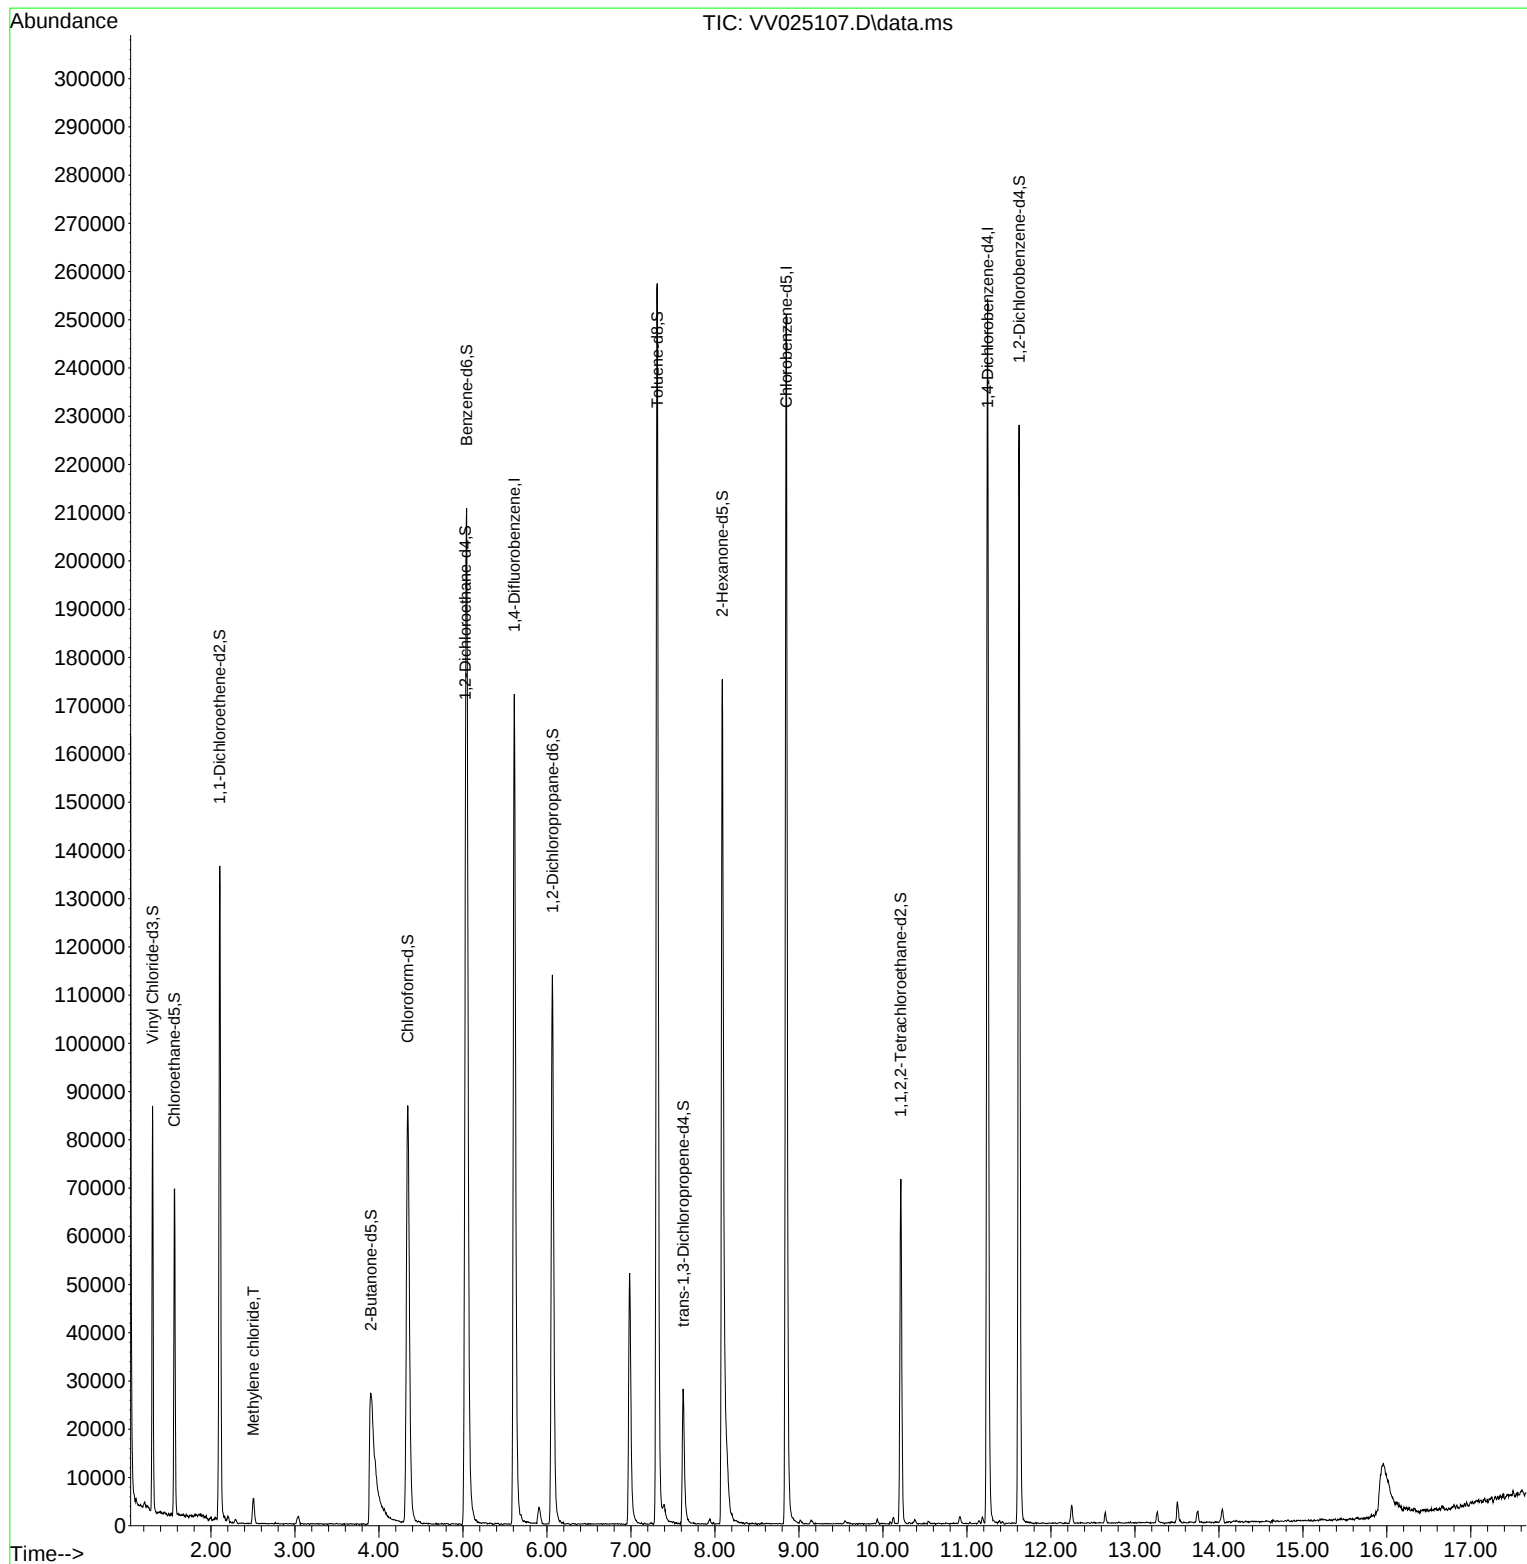

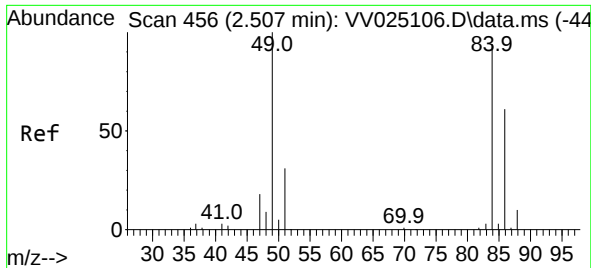

#16
Methylene chloride
Concen: 0.215 ug/L
RT: 2.506 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV025107.D
Acq: 21 Mar 2022 10:15

Instrument :
MSVOA_V
ClientSampleId :
VBLK320

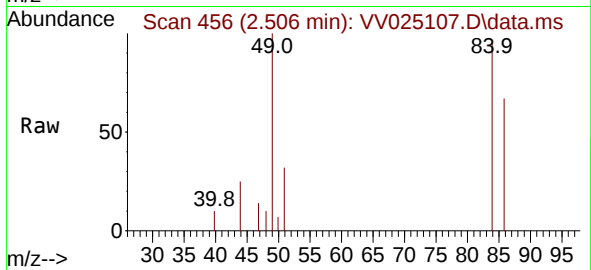

Tgt Ion: 84 Resp: 2642

Ion	Ratio	Lower	Upper
84	100		
86	70.1	45.5	84.5
49	105.1	75.0	139.2

